

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062318\
 Data File : FG001461.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jun 2018 16:49
 Operator : UA\AJ
 Sample : J3241-17 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 04:31:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.531	196486	1.607 ug/ml
Target Compounds			
3) N-DODECANE	6.288	166391	1.200 ug/ml
4) N-TETRADECANE	8.080	169034	1.210 ug/ml
7) N-EICOSANE	12.475	352688	2.505 ug/ml
10) N-TETRACOSANE	14.696f	167698	1.206 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062318\
Data File : FG001461.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2018 16:49
Operator : UA\AJ
Sample : J3241-17 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 04:31:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

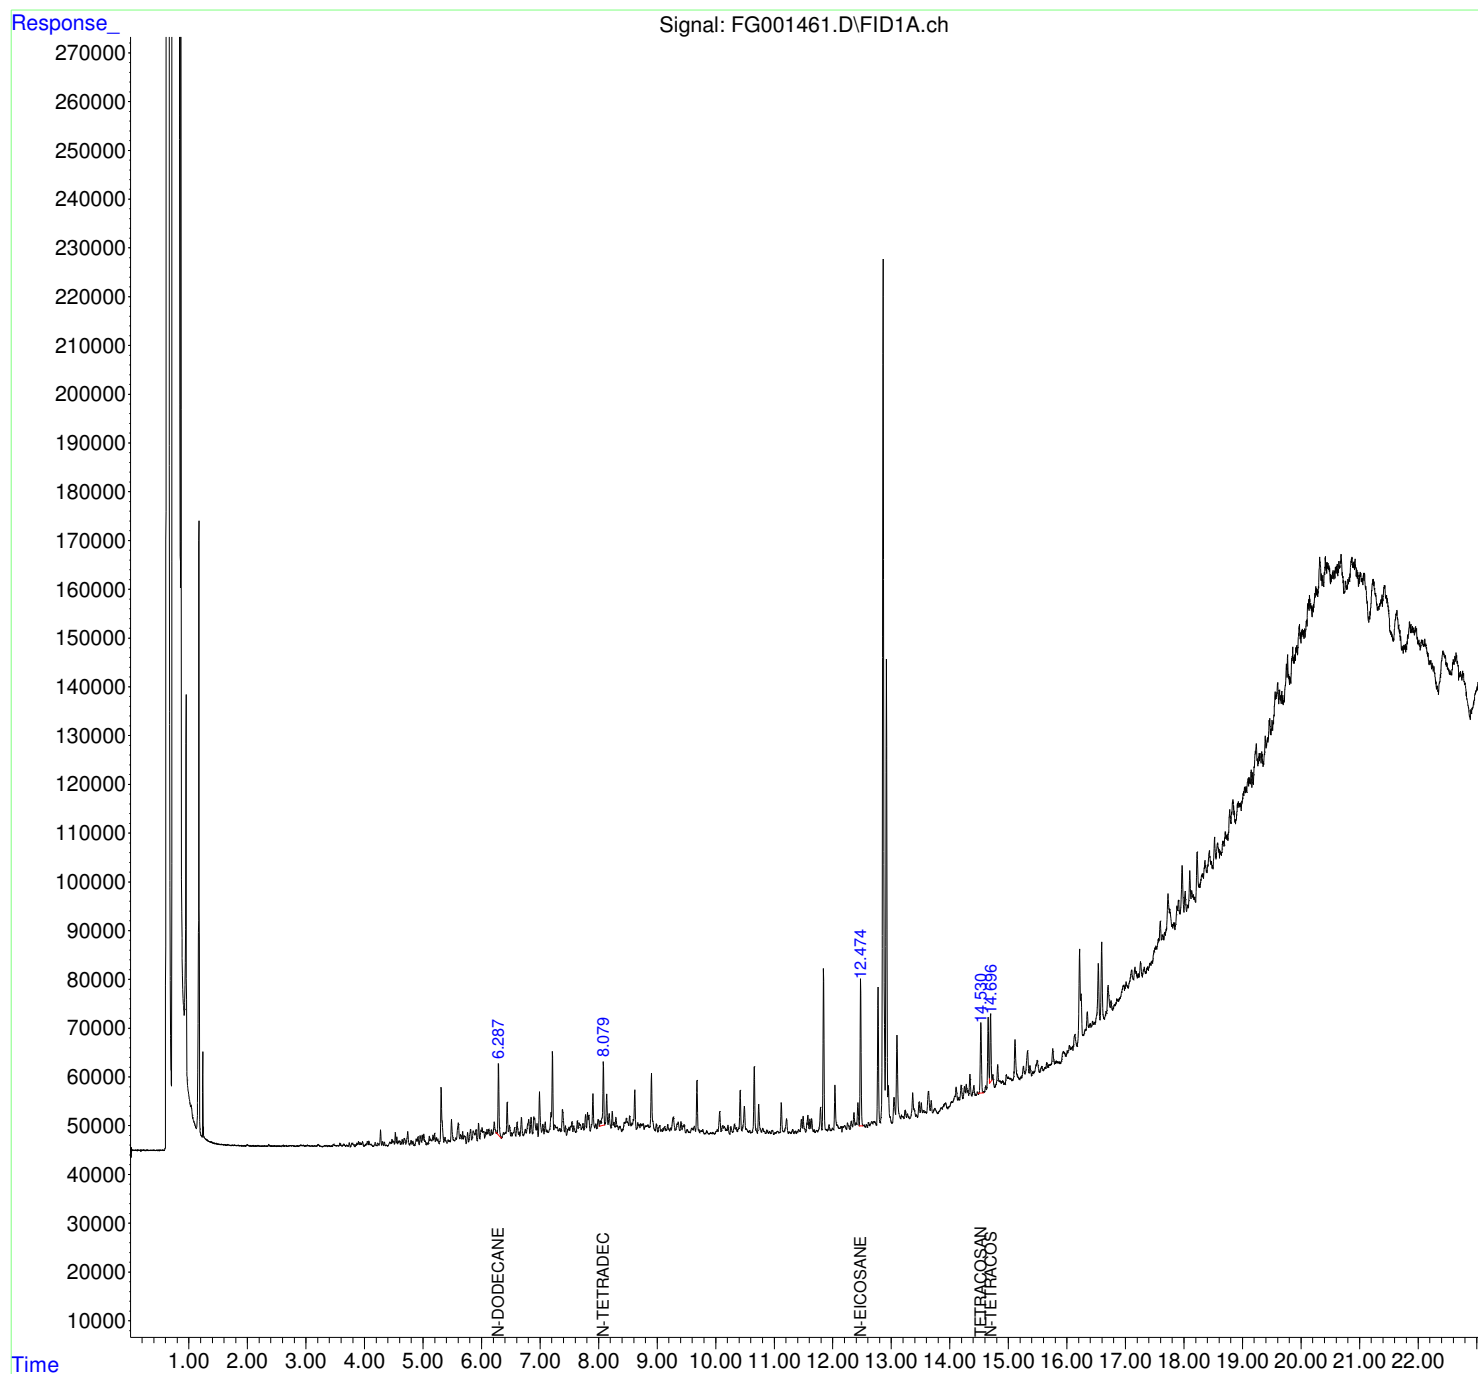


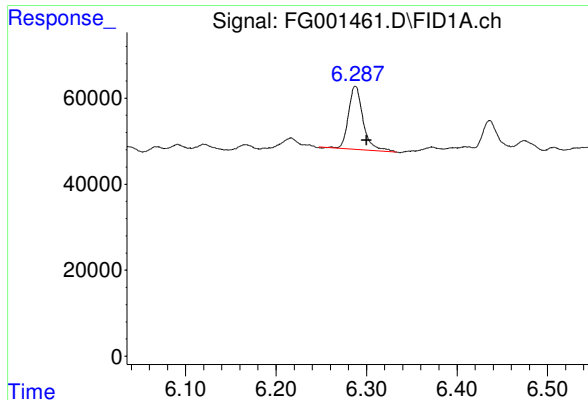

#3 N-DODECANE


R.T.: 6.288 min
Delta R.T.: -0.012 min
Response: 166391
Conc: 1.20 ug/ml

Instrument :
FID_G
ClientSampleId :

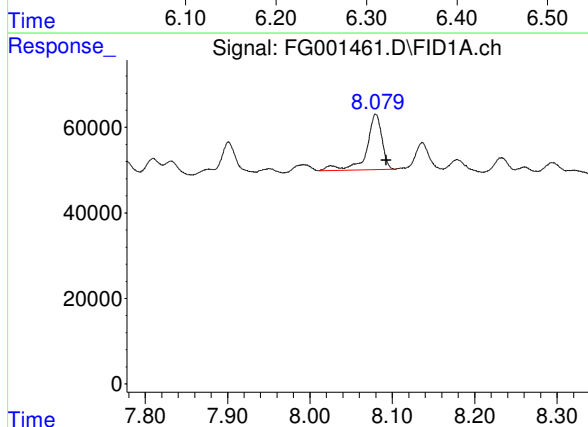


#4 N-TETRADECANE

R.T.: 8.080 min
Delta R.T.: -0.013 min
Response: 169034
Conc: 1.21 ug/ml

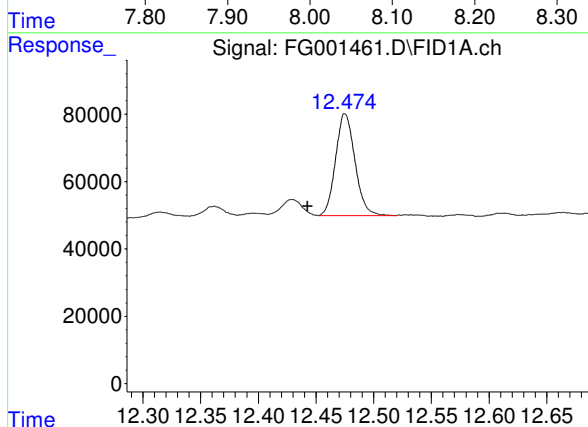


#7 N-EICOSANE

R.T.: 12.475 min
Delta R.T.: 0.033 min
Response: 352688
Conc: 2.50 ug/ml

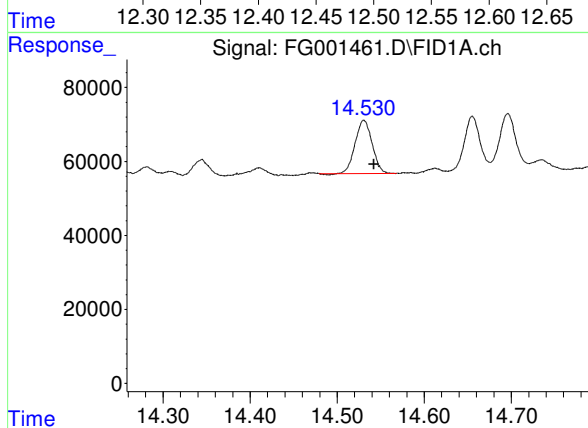

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.531 min
Delta R.T.: -0.012 min
Response: 196486
Conc: 1.61 ug/ml

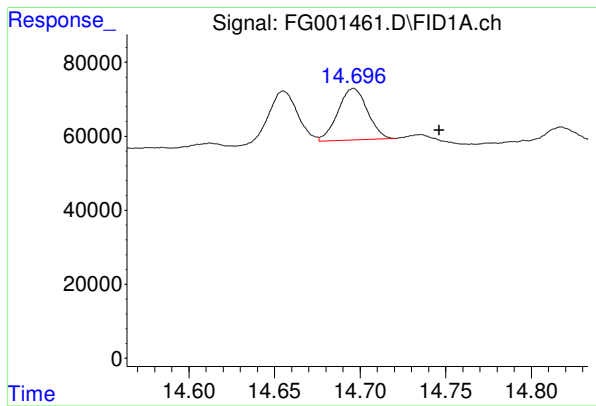

#10 N-TETRACOSANE

R.T.: 14.696 min
Delta R.T.: -0.050 min
Response: 167698
Conc: 1.21 ug/ml

Instrument :
FID_G
ClientSampleId :