

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062318\
 Data File : FG001462.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jun 2018 17:19
 Operator : UA\AJ
 Sample : J3241-13 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 04:31:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.530	237023	1.939 ug/ml
Target Compounds			
2) N-DECANE	4.272	170797	1.246 ug/ml
3) N-DODECANE	6.287	644078	4.646 ug/ml
4) N-TETRADECANE	8.080	530893	3.799 ug/ml
5) N-HEXADECANE	9.679	352390	2.504 ug/ml
6) N-OCTADECANE	11.120	203388	1.435 ug/ml
7) N-EICOSANE	12.430	188702	1.340 ug/ml
10) N-TETRACOSANE	14.696f	364449	2.621 ug/ml
12) N-OCTACOSANE	16.705	277249	2.009 ug/ml
13) N-TRIACONTANE	17.596	294140	2.144 ug/ml
14) N-DOTRIACONTANE	18.434	190503	1.424 ug/ml
15) N-TETRATRIACONTANE	19.224	430080	3.265 ug/ml
16) N-HEXATRIACONTANE	19.968	181156	1.441 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062318\
Data File : FG001462.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2018 17:19
Operator : UA\AJ
Sample : J3241-13 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 04:31:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

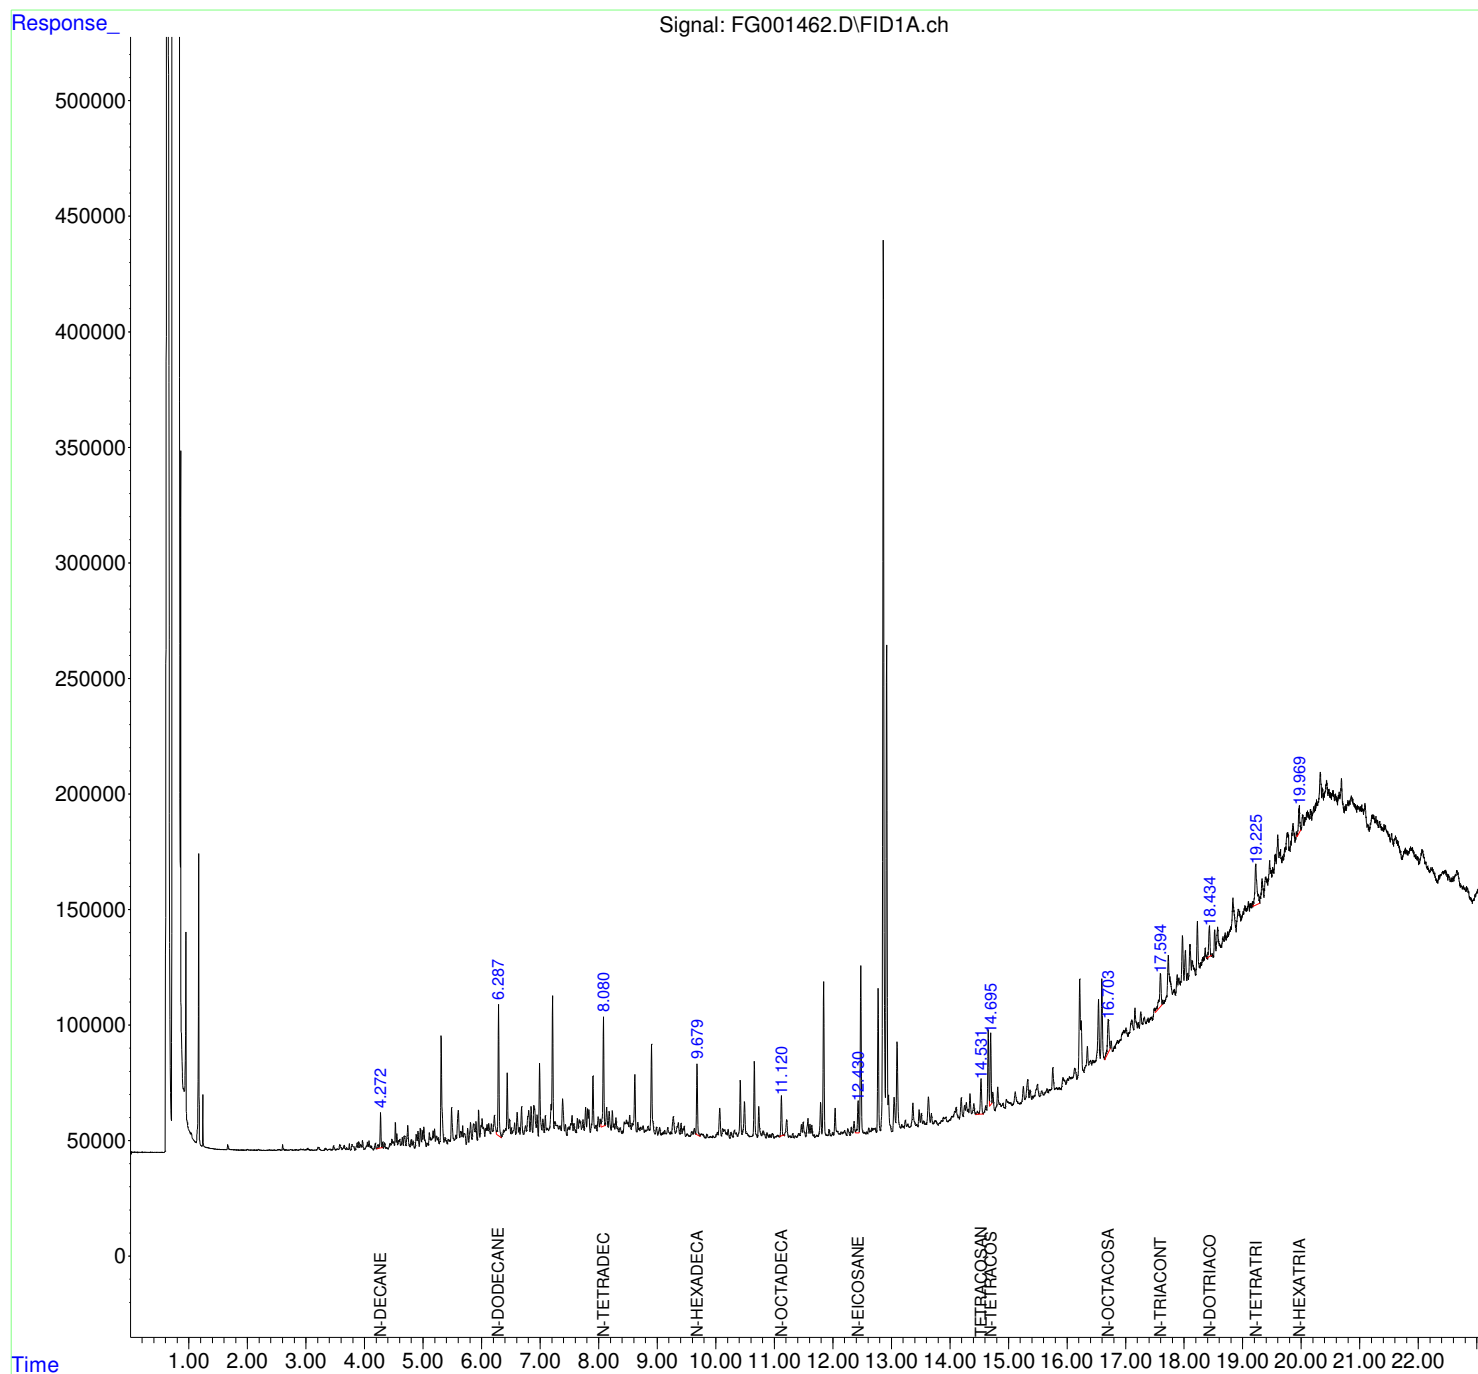


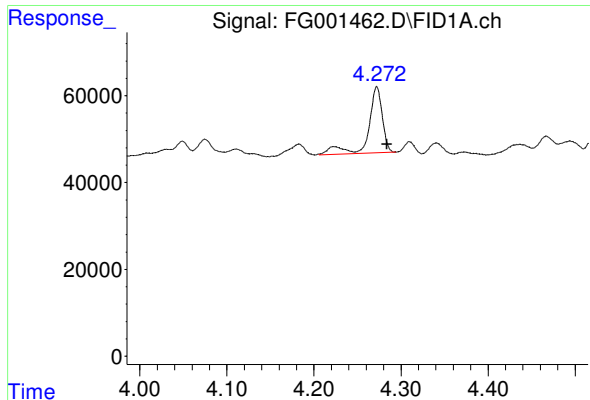

#2 N-DECANE


R.T.: 4.272 min
Delta R.T.: -0.012 min
Response: 170797
Conc: 1.25 ug/ml

Instrument :
FID_G
ClientSampleId :

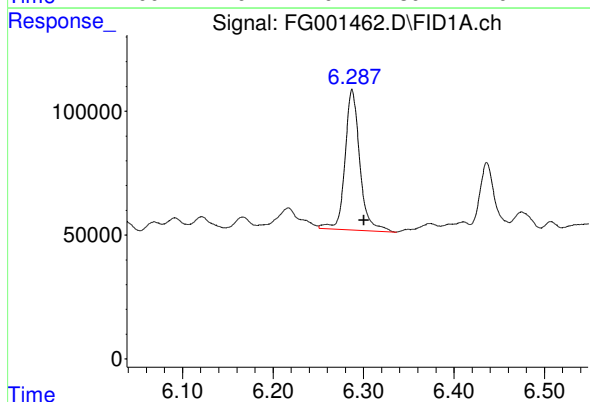


#3 N-DODECANE

R.T.: 6.287 min
Delta R.T.: -0.013 min
Response: 644078
Conc: 4.65 ug/ml

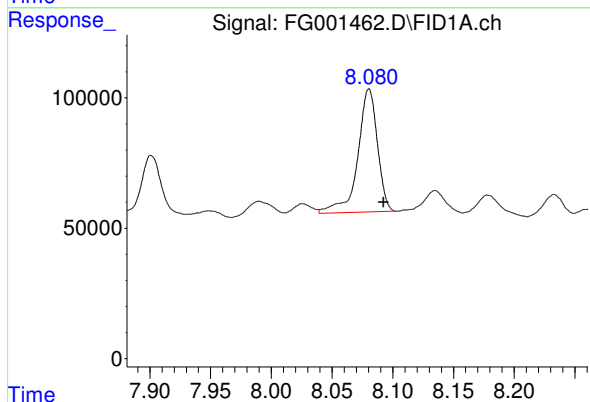


#4 N-TETRADECANE

R.T.: 8.080 min
Delta R.T.: -0.012 min
Response: 530893
Conc: 3.80 ug/ml

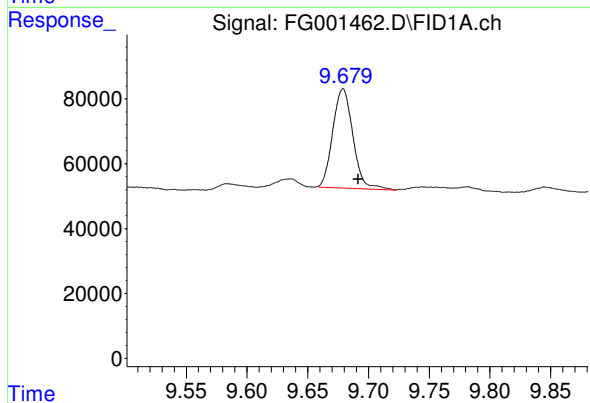

#5 N-HEXADECANE


R.T.: 9.679 min
Delta R.T.: -0.013 min
Response: 352390
Conc: 2.50 ug/ml

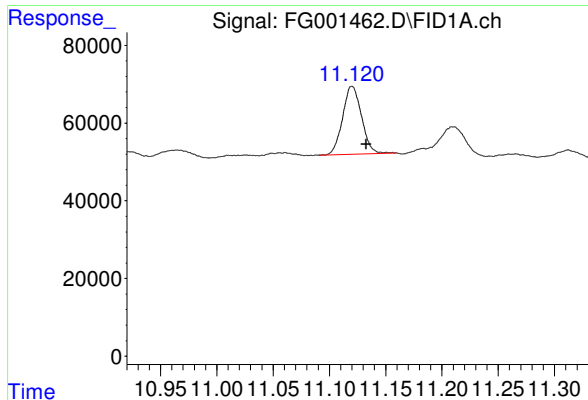

#6 N-OCTADECANE


R.T.: 11.120 min
Delta R.T.: -0.013 min
Response: 203388
Conc: 1.43 ug/ml

Instrument :
FID_G
ClientSampleId :

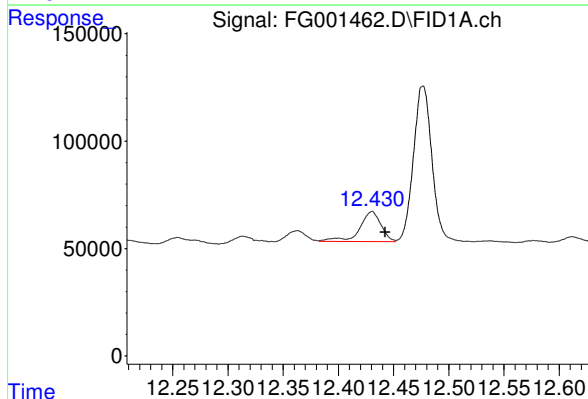


#7 N-EICOSANE

R.T.: 12.430 min
Delta R.T.: -0.012 min
Response: 188702
Conc: 1.34 ug/ml

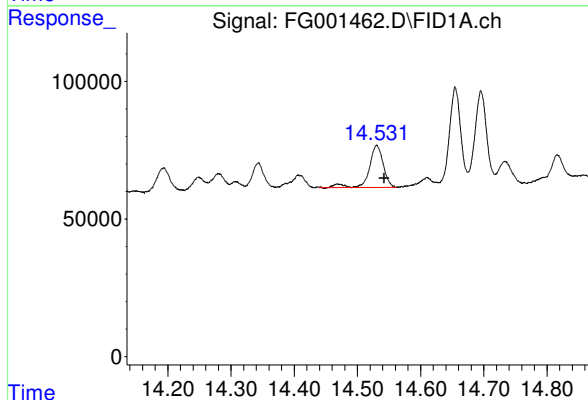


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.530 min
Delta R.T.: -0.012 min
Response: 237023
Conc: 1.94 ug/ml

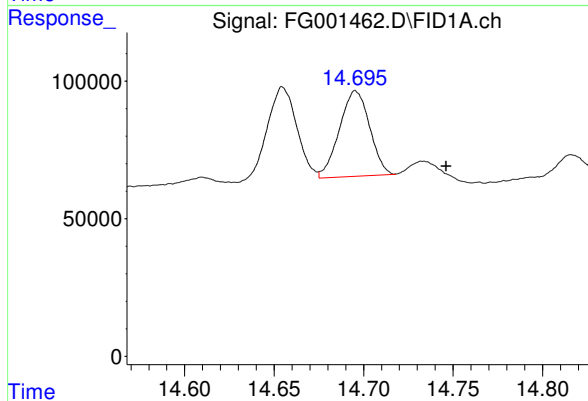

#10 N-TETRACOSANE


R.T.: 14.696 min
Delta R.T.: -0.051 min
Response: 364449
Conc: 2.62 ug/ml

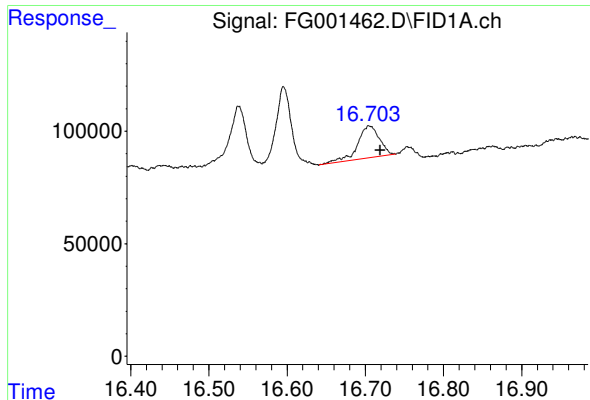

#12 N-OCTACOSANE


R.T.: 16.705 min
Delta R.T.: -0.014 min
Response: 277249
Conc: 2.01 ug/ml

Instrument :
FID_G
ClientSampleId :

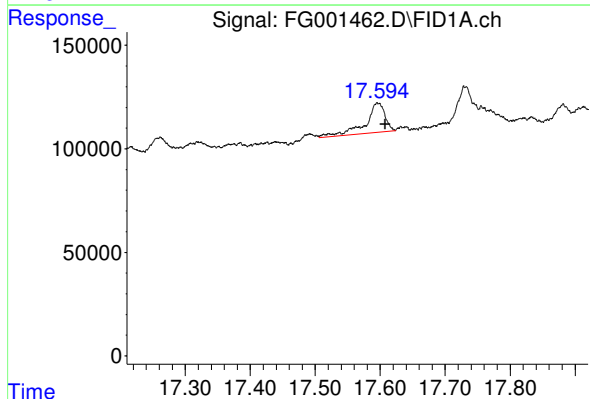


#13 N-TRIACONTANE

R.T.: 17.596 min
Delta R.T.: -0.011 min
Response: 294140
Conc: 2.14 ug/ml

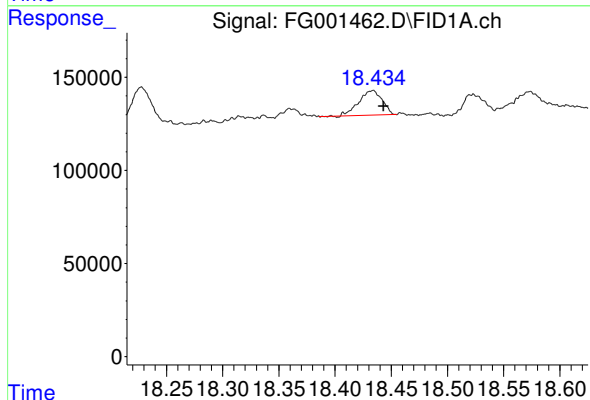


#14 N-DOTRIACONTANE

R.T.: 18.434 min
Delta R.T.: -0.010 min
Response: 190503
Conc: 1.42 ug/ml

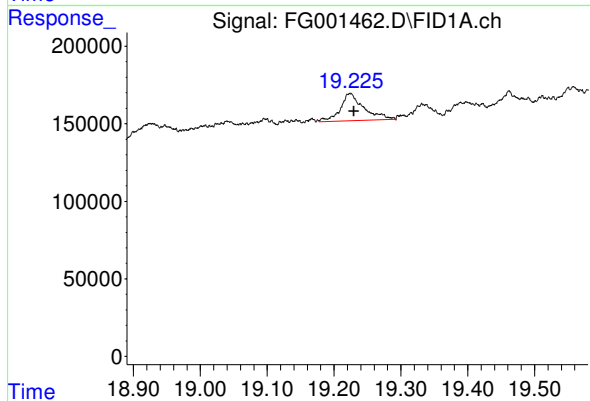

#15 N-TETRATRIACONTANE

R.T.: 19.224 min
Delta R.T.: -0.005 min
Response: 430080
Conc: 3.26 ug/ml

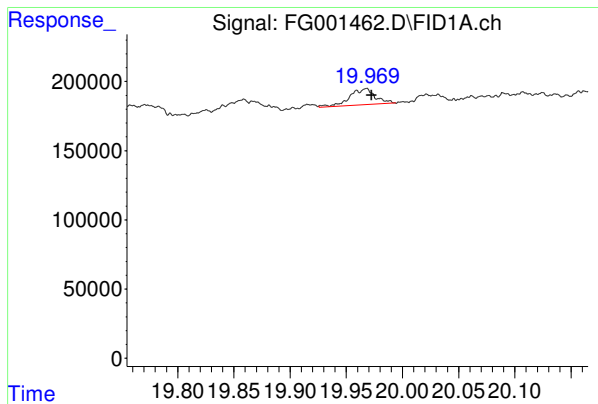

#16 N-HEXATRIACONTANE

R.T.: 19.968 min
Delta R.T.: -0.005 min
Response: 181156
Conc: 1.44 ug/ml

Instrument :
FID_G
ClientSampleId :