

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062318\
 Data File : FG001466.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jun 2018 19:48
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 04:31:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.533	5592278	45.745 ug/ml
Target Compounds			
2) N-DECANE	4.274	6758891	49.309 ug/ml
3) N-DODECANE	6.290	6782205	48.924 ug/ml
4) N-TETRADECANE	8.083	6762976	48.399 ug/ml
5) N-HEXADECANE	9.683	6730663	47.828 ug/ml
6) N-OCTADECANE	11.125	6689137	47.189 ug/ml
7) N-EICOSANE	12.435	6562041	46.600 ug/ml
8) N-DOCOSANE	13.633	6441260	45.961 ug/ml
10) N-TETRACOSANE	14.737	6324366	45.483 ug/ml
11) N-HEXACOSANE	15.760	6214832	44.863 ug/ml
12) N-OCTACOSANE	16.712	6136875	44.478 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062318\
Data File : FG001466.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2018 19:48
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 04:31:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

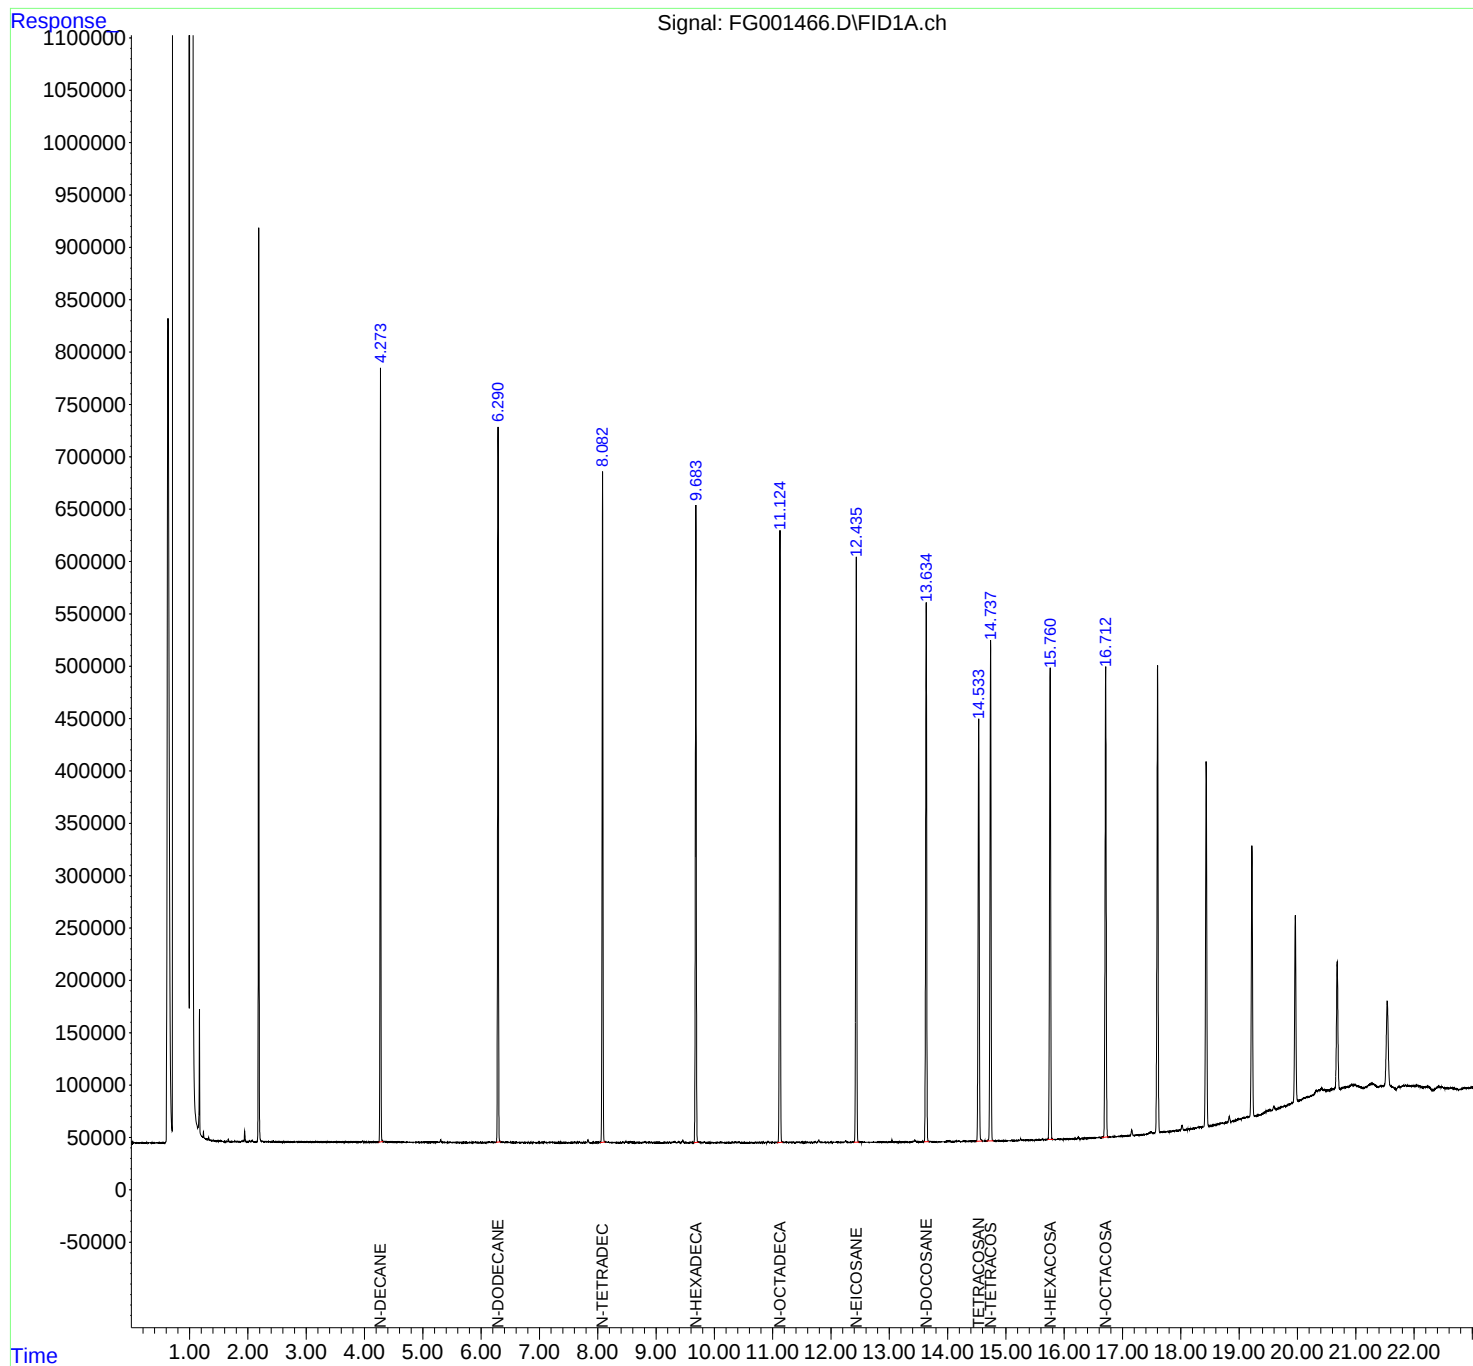


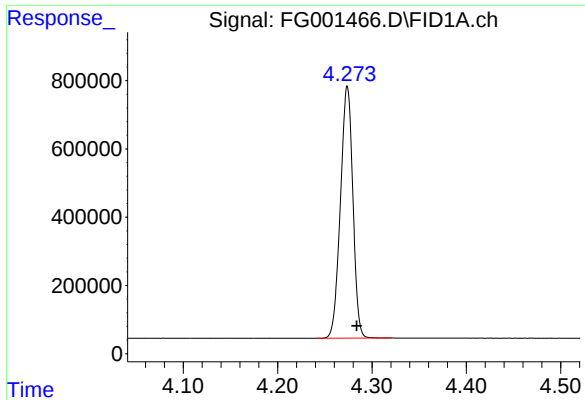

#2 N-DECANE


R.T.: 4.274 min
Delta R.T.: -0.010 min
Response: 6758891
Conc: 49.31 ug/ml

Instrument :
FID_G
ClientSampleId :

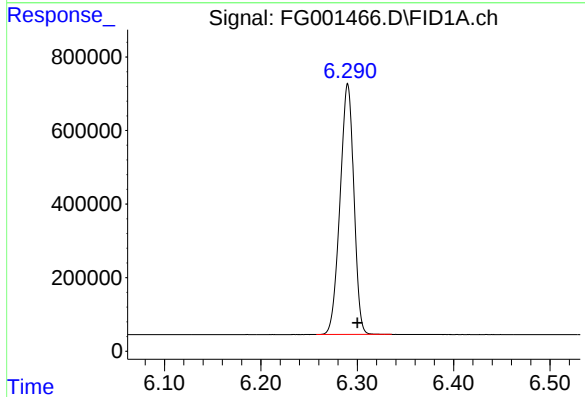


#3 N-DODECANE

R.T.: 6.290 min
Delta R.T.: -0.010 min
Response: 6782205
Conc: 48.92 ug/ml

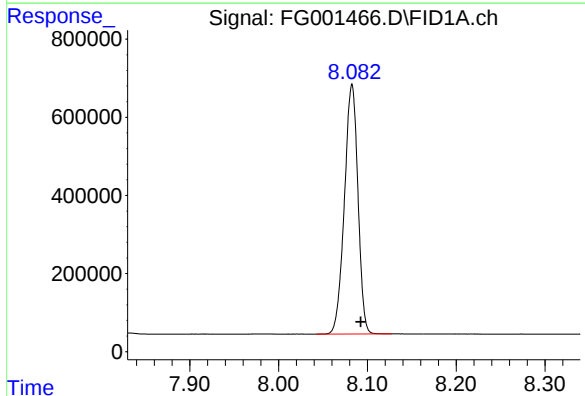


#4 N-TETRADECANE

R.T.: 8.083 min
Delta R.T.: -0.010 min
Response: 6762976
Conc: 48.40 ug/ml

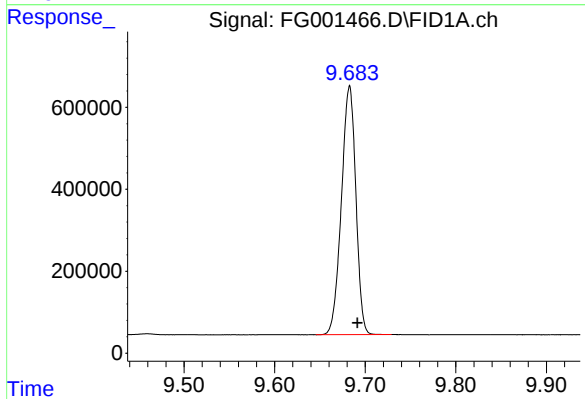

#5 N-HEXADECANE


R.T.: 9.683 min
Delta R.T.: -0.009 min
Response: 6730663
Conc: 47.83 ug/ml

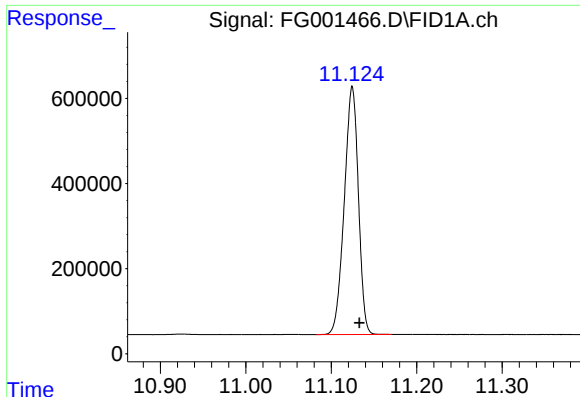

#6 N-OCTADECANE


R.T.: 11.125 min
Delta R.T.: -0.008 min
Response: 6689137
Conc: 47.19 ug/ml

Instrument :
FID_G
ClientSampleId :

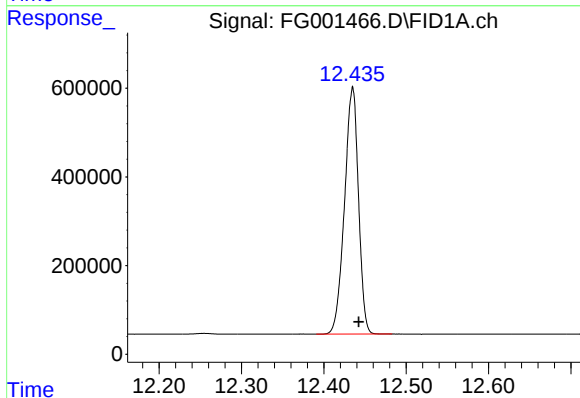


#7 N-EICOSANE

R.T.: 12.435 min
Delta R.T.: -0.007 min
Response: 6562041
Conc: 46.60 ug/ml

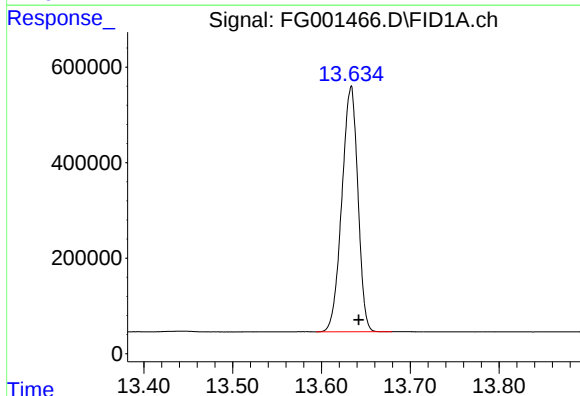


#8 N-DOCOSANE

R.T.: 13.633 min
Delta R.T.: -0.009 min
Response: 6441260
Conc: 45.96 ug/ml

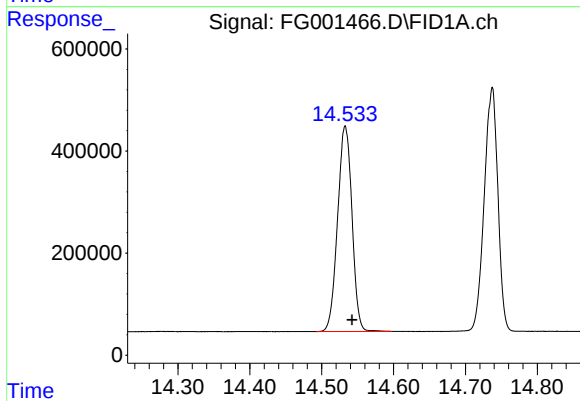

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.533 min
Delta R.T.: -0.009 min
Response: 5592278
Conc: 45.74 ug/ml

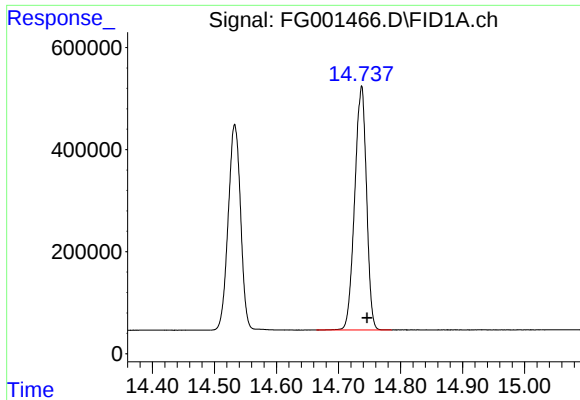

#10 N-TETRACOSANE


R.T.: 14.737 min
Delta R.T.: -0.009 min
Response: 6324366
Conc: 45.48 ug/ml

Instrument :
FID_G
ClientSampleId :

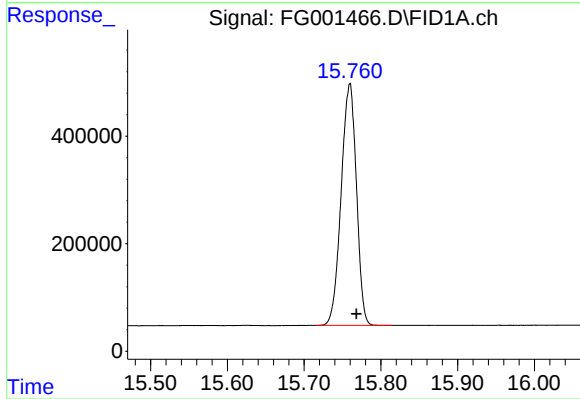

#11 N-HEXACOSANE

R.T.: 15.760 min
Delta R.T.: -0.009 min
Response: 6214832
Conc: 44.86 ug/ml

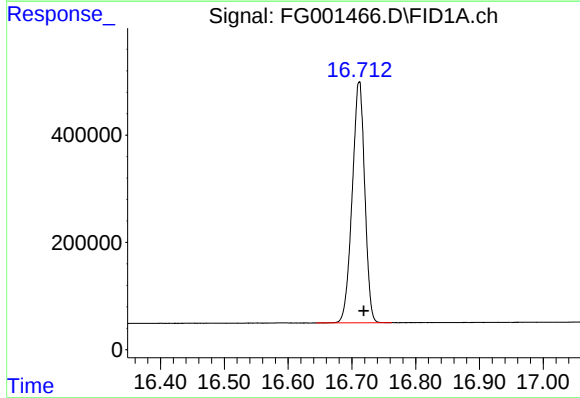

#12 N-OCTACOSANE

R.T.: 16.712 min
Delta R.T.: -0.007 min
Response: 6136875
Conc: 44.48 ug/ml