

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062321\
 Data File : FG008395.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jun 2021 10:55
 Operator : DD\AJ
 Sample : M2791-05 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 23 13:30:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
 Quant Title :
 QLast Update : Wed May 26 08:20:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.766	809849	6.824 ug/ml
Target Compounds			
6) N-OCTADECANE	11.401	161725	1.167 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062321\
Data File : FG008395.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2021 10:55
Operator : DD\AJ
Sample : M2791-05 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 13:30:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052521.M
Quant Title :
QLast Update : Wed May 26 08:20:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

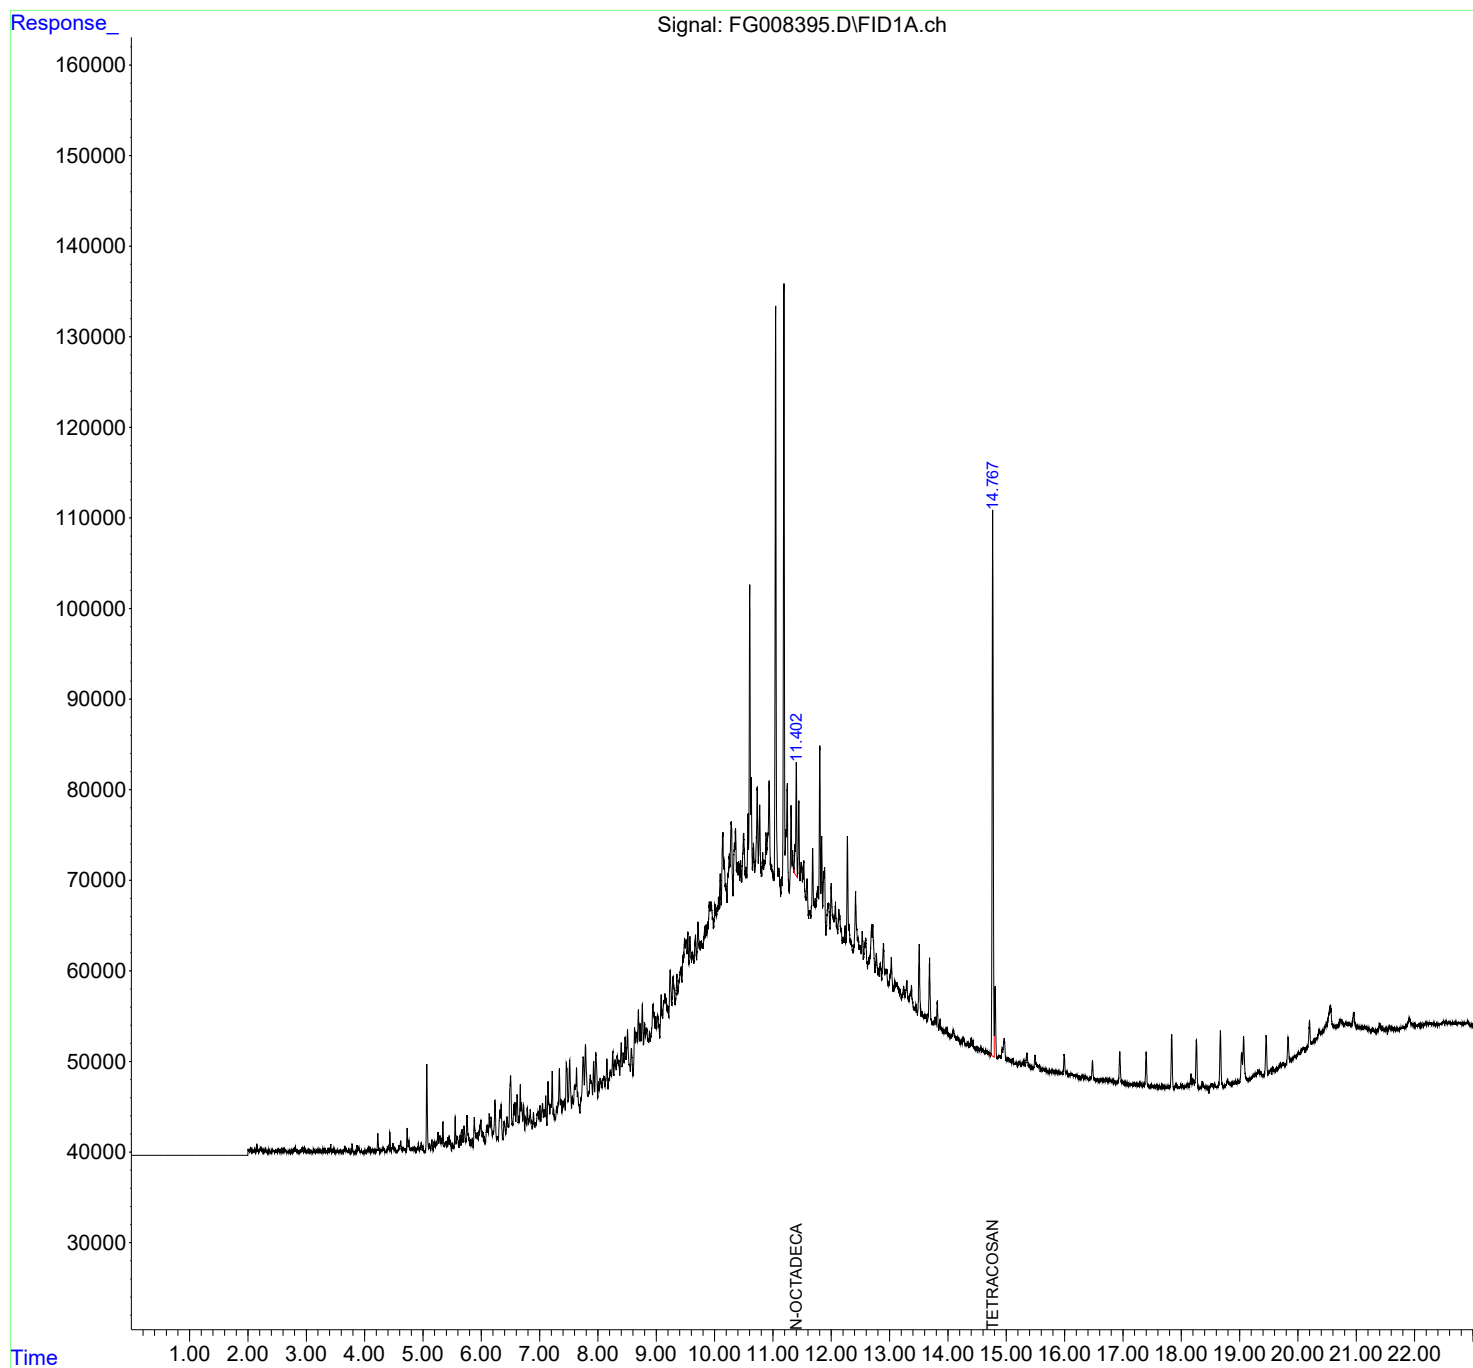


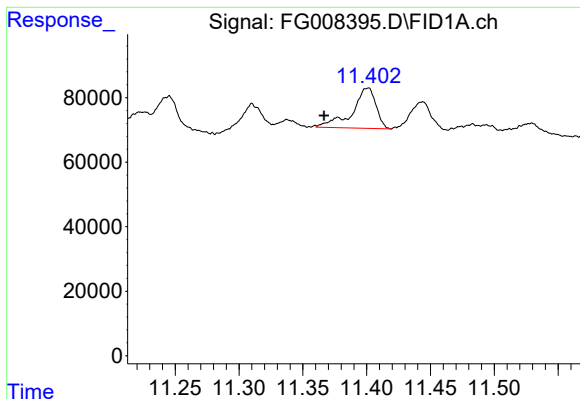

#6 N-OCTADECANE

R.T.: 11.401 min
Delta R.T.: 0.034 min
Response: 161725
Conc: 1.17 ug/ml

Instrument :
FID_G
ClientSampleId :

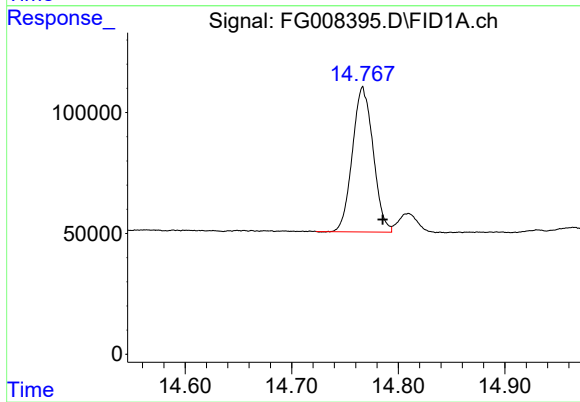

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.766 min
Delta R.T.: -0.019 min
Response: 809849
Conc: 6.82 ug/ml