

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062322\
Data File : FG009939.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2022 09:21
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 01:31:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13)	N-TRIACONTANE	17.899	125271	1.163 ug/ml
14)	N-DOTRIACONTANE	18.736	118055	1.122 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062322\
Data File : FG009939.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2022 09:21
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 01:31:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

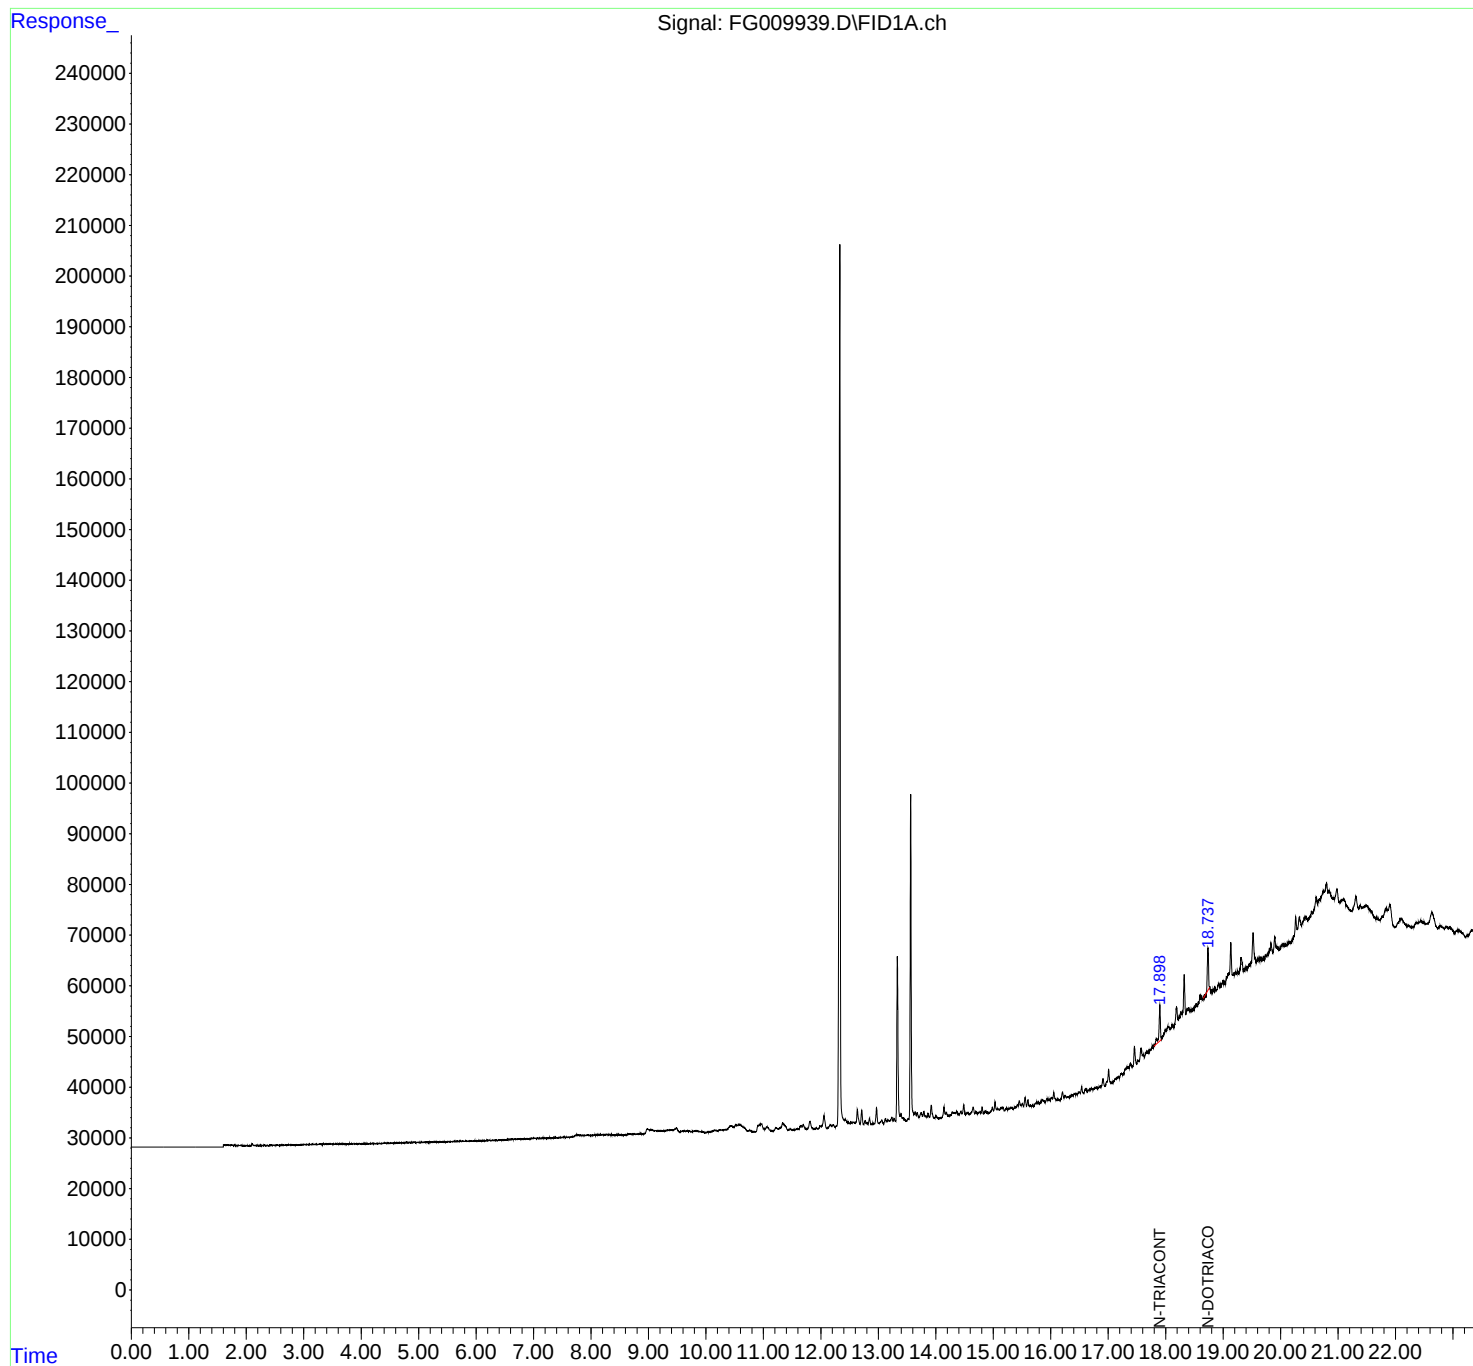


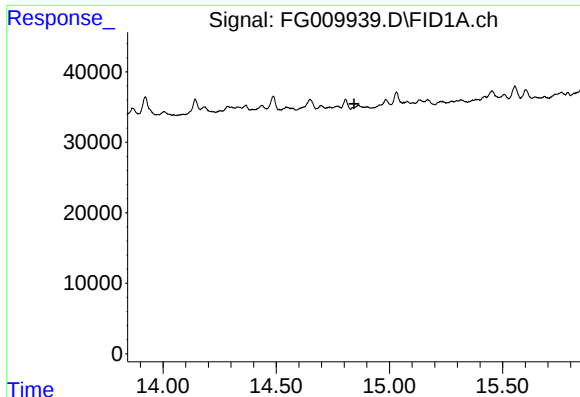

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.843 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

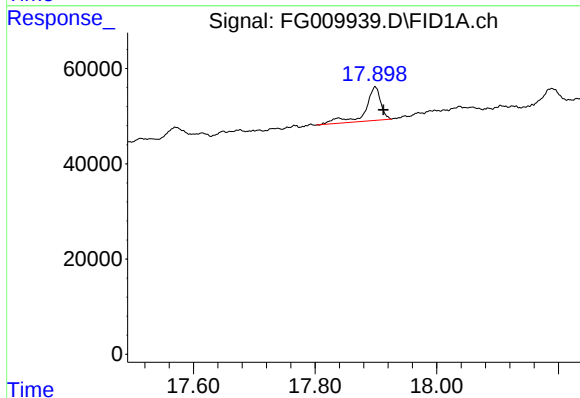

#13 N-TRIACONTANE

R.T.: 17.899 min
Delta R.T.: -0.014 min
Response: 125271
Conc: 1.16 ug/ml

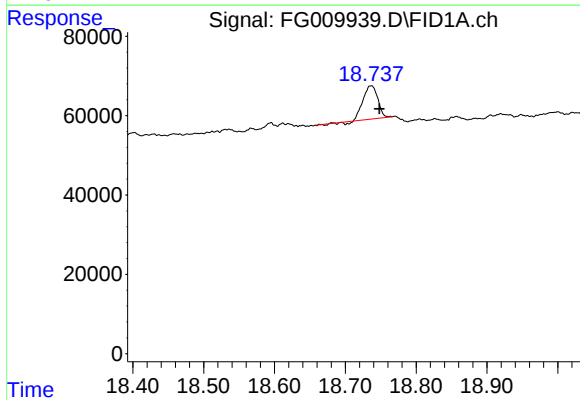

#14 N-DOTRIACONTANE

R.T.: 18.736 min
Delta R.T.: -0.012 min
Response: 118055
Conc: 1.12 ug/ml