

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062322\
 Data File : FG009942.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jun 2022 11:47
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 24 01:32:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
 Quant Title :
 QLast Update : Wed Jun 01 13:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.523	4090090	32.421 ug/ml
12) N-OCTACOSANE	17.009	4003214	34.983 ug/ml
13) N-TRIACONTANE	17.897	250703	2.328 ug/ml
14) N-DOTRIACONTANE	18.732	305843	2.906 ug/ml
15) N-TETRATRIACONTANE	19.518	235627	2.454 ug/ml
16) N-HEXATRIACONTANE	20.261	146706	1.815 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062322\
Data File : FG009942.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2022 11:47
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 01:32:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

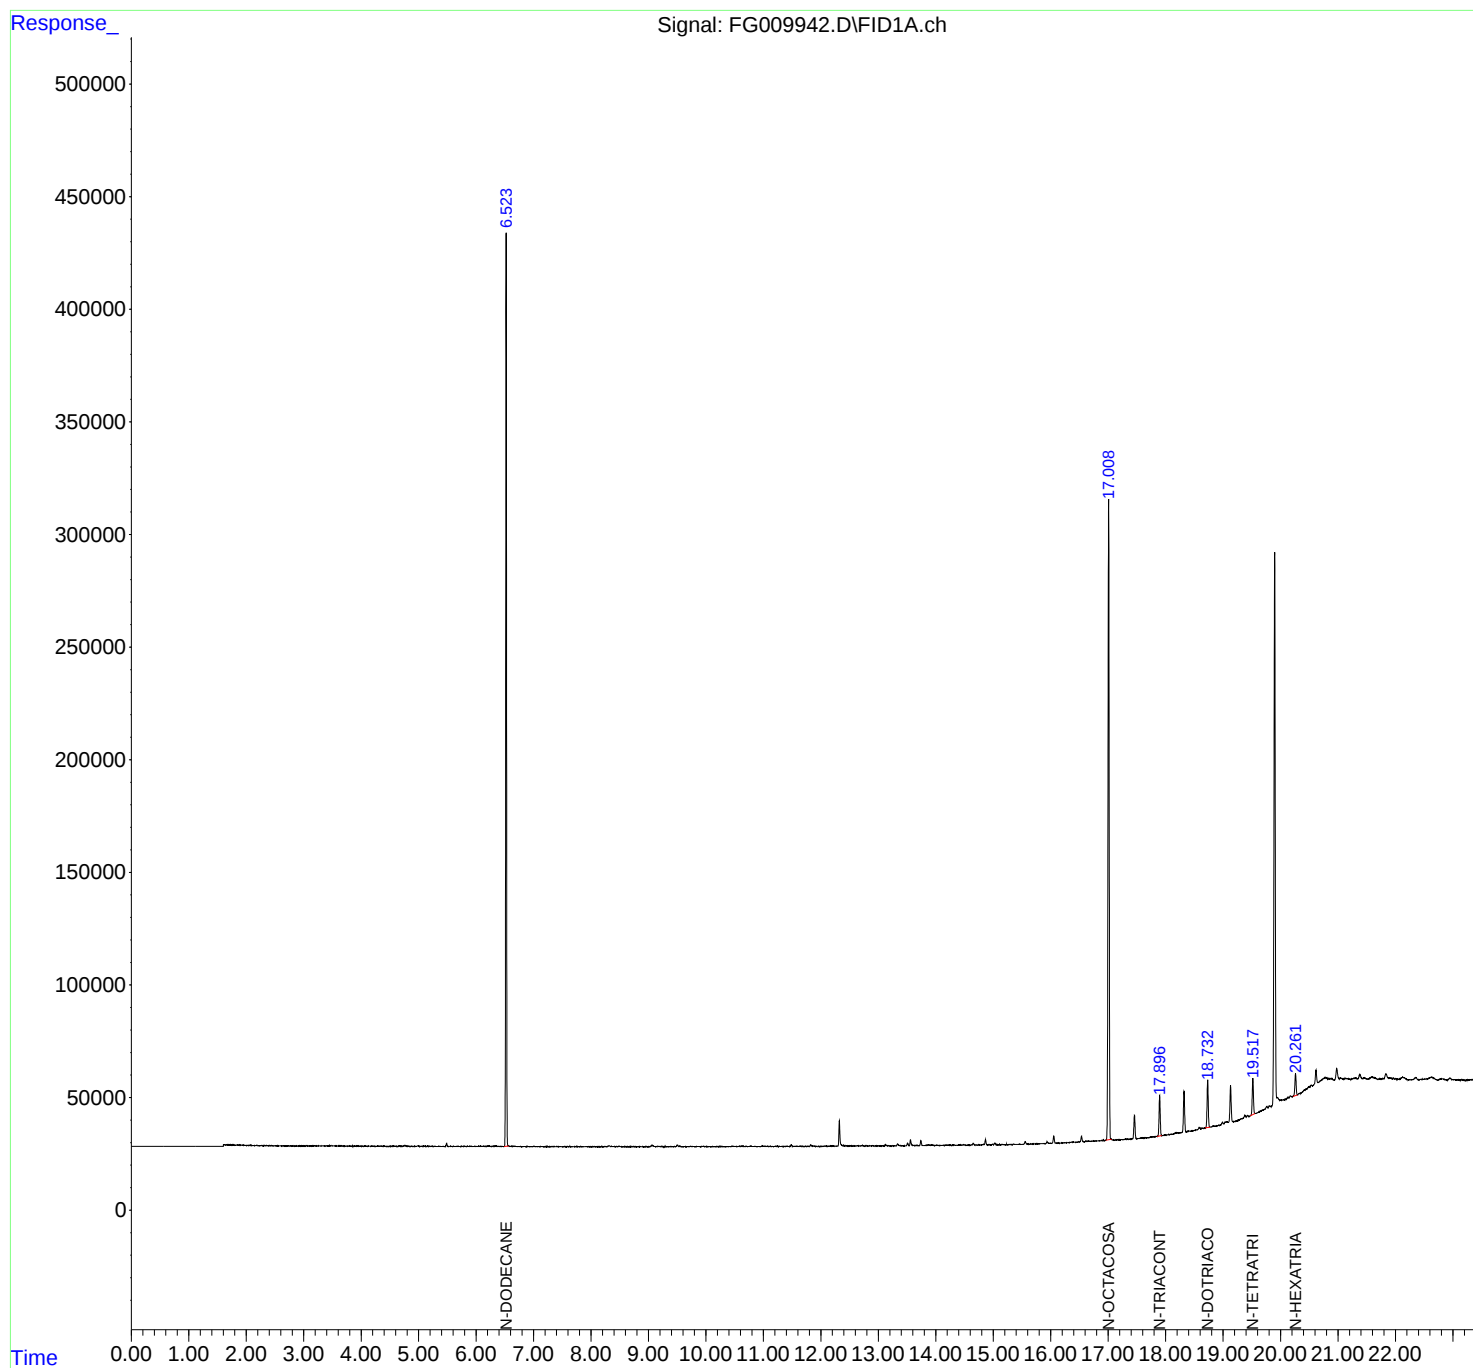


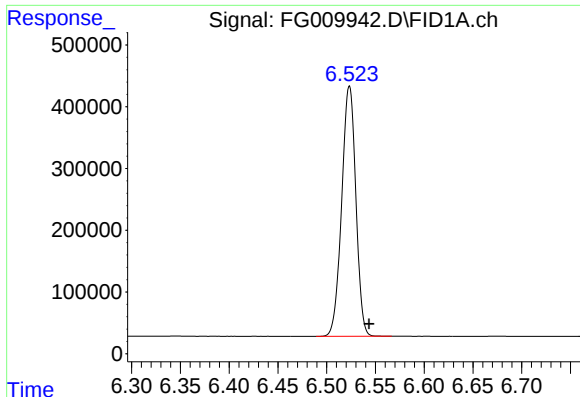

#3 N-DODECANE


R.T.: 6.523 min
Delta R.T.: -0.020 min
Response: 4090090
Conc: 32.42 ug/ml

Instrument :
FID_G
ClientSampleId :

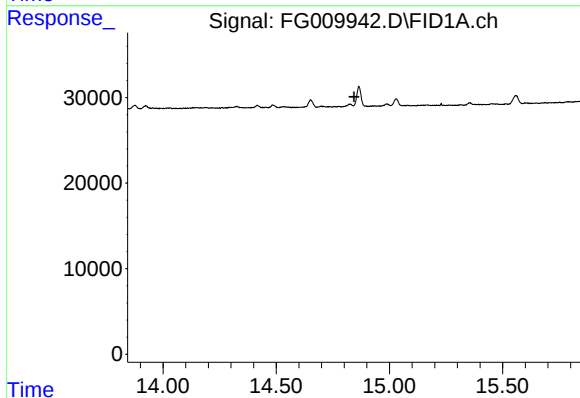


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.843 min
Response: 0
Conc: N.D.

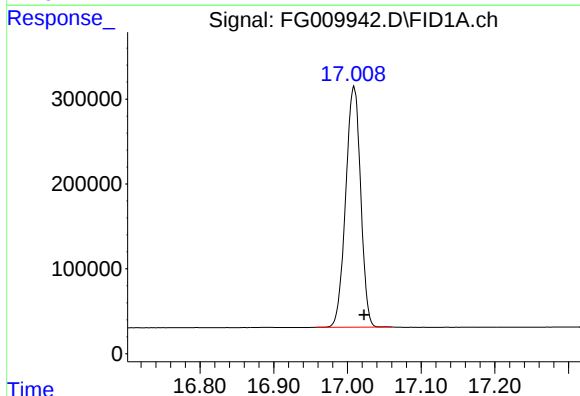


#12 N-OCTACOSANE

R.T.: 17.009 min
Delta R.T.: -0.014 min
Response: 4003214
Conc: 34.98 ug/ml

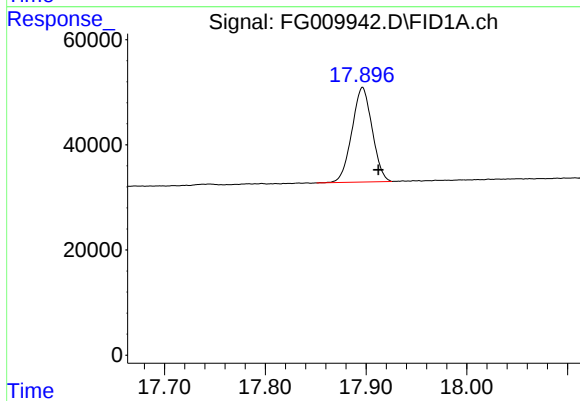

#13 N-TRIACONTANE


R.T.: 17.897 min
Delta R.T.: -0.016 min
Response: 250703
Conc: 2.33 ug/ml

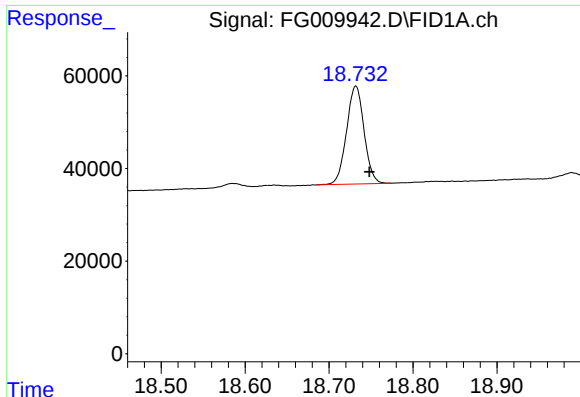

#14 N-DOTRIACONTANE


R.T.: 18.732 min
Delta R.T.: -0.016 min
Response: 305843
Conc: 2.91 ug/ml

Instrument :
FID_G
ClientSampleId :

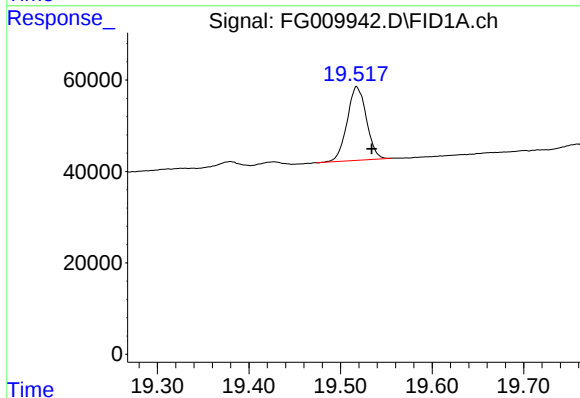

#15 N-TETRATRIACONTANE

R.T.: 19.518 min
Delta R.T.: -0.017 min
Response: 235627
Conc: 2.45 ug/ml

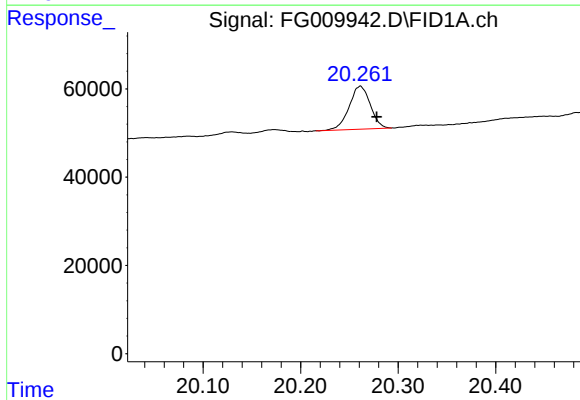

#16 N-HEXATRIACONTANE

R.T.: 20.261 min
Delta R.T.: -0.017 min
Response: 146706
Conc: 1.82 ug/ml