

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062322\
 Data File : FG009946.D
 Signal(s) : FID1A.ch
 Acq On : 23 Jun 2022 13:48
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 24 01:34:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
 Quant Title :
 QLast Update : Wed Jun 01 13:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.822	2025243	19.241 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.892	110533	1.026 ug/ml
14) N-DOTRIACONTANE	18.726	138153	1.313 ug/ml
15) N-TETRATRIACONTANE	19.514	104131	1.085 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062322\
Data File : FG009946.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2022 13:48
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 01:34:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

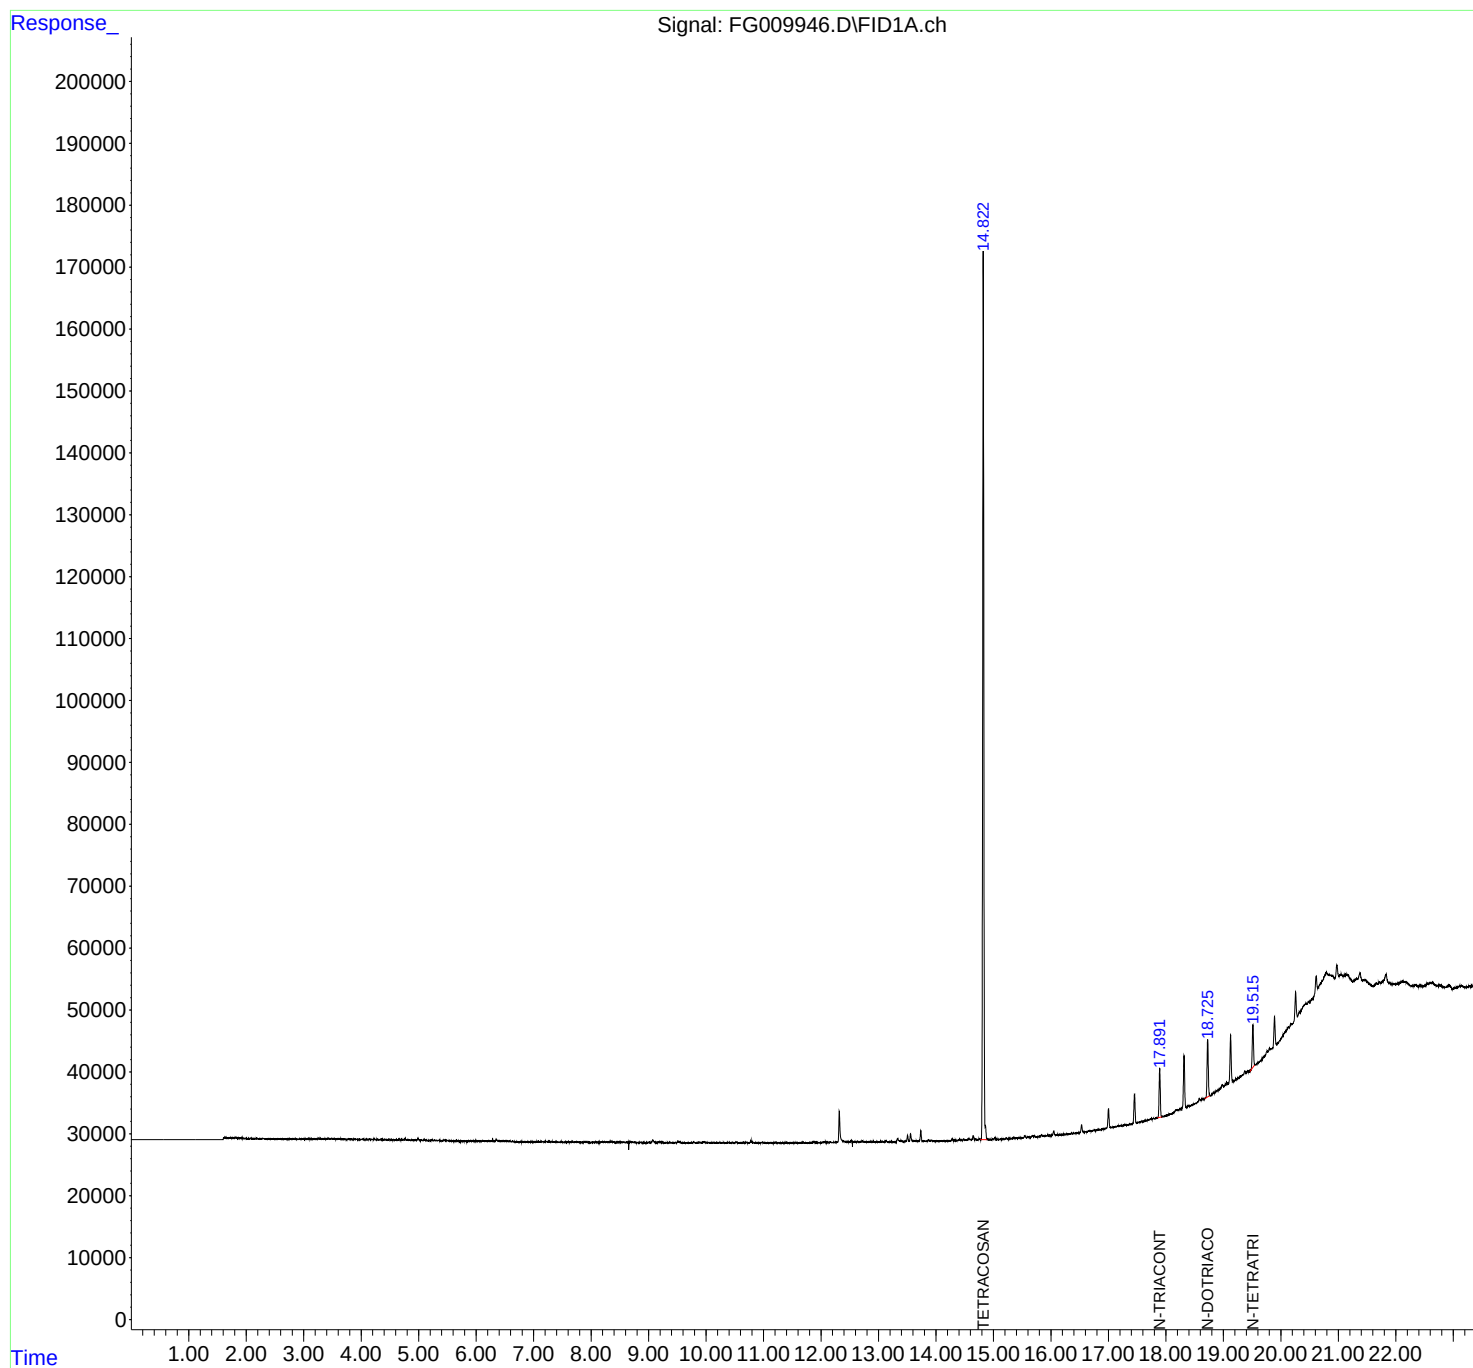


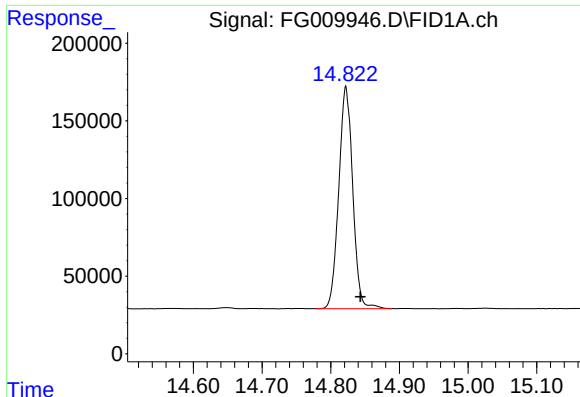

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.822 min
Delta R.T.: -0.021 min
Response: 2025243
Conc: 19.24 ug/ml

Instrument :
FID_G
ClientSampleId :

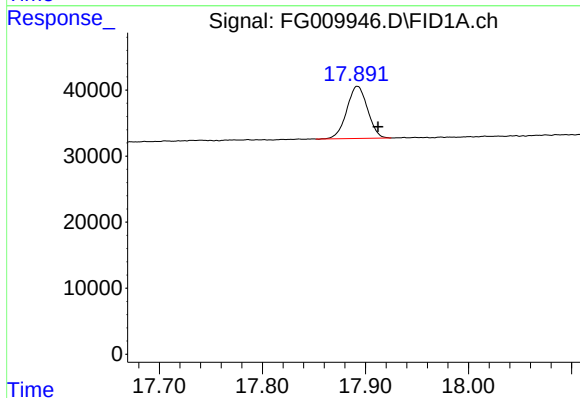


#13 N-TRIACONTANE

R.T.: 17.892 min
Delta R.T.: -0.020 min
Response: 110533
Conc: 1.03 ug/ml

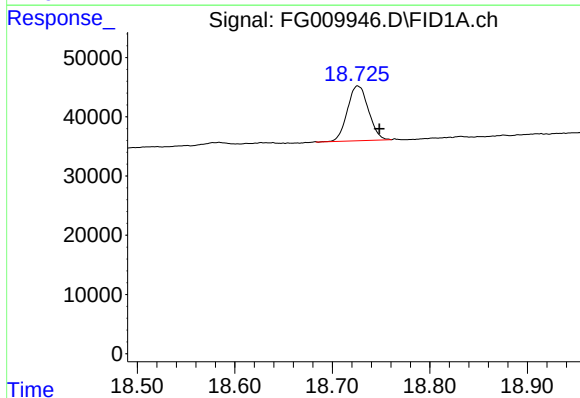

#14 N-DOTRIACONTANE

R.T.: 18.726 min
Delta R.T.: -0.022 min
Response: 138153
Conc: 1.31 ug/ml

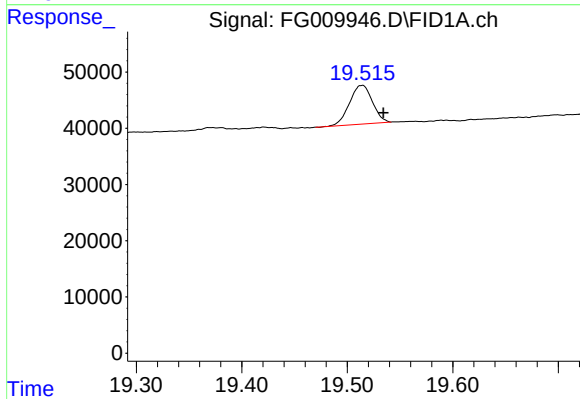

#15 N-TETRATRIACONTANE

R.T.: 19.514 min
Delta R.T.: -0.020 min
Response: 104131
Conc: 1.08 ug/ml