

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062323\
Data File : FG012265.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2023 09:25
Operator : YP\AJ
Sample : 03333-04 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
DOMINICK-SP-TPH

Integration File: autoint1.e
Quant Time: Jun 24 06:23:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.990	209299	1.570 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062323\
Data File : FG012265.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2023 09:25
Operator : YP\AJ
Sample : 03333-04 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
DOMINICK-SP-TPH

Integration File: autoint1.e
Quant Time: Jun 24 06:23:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

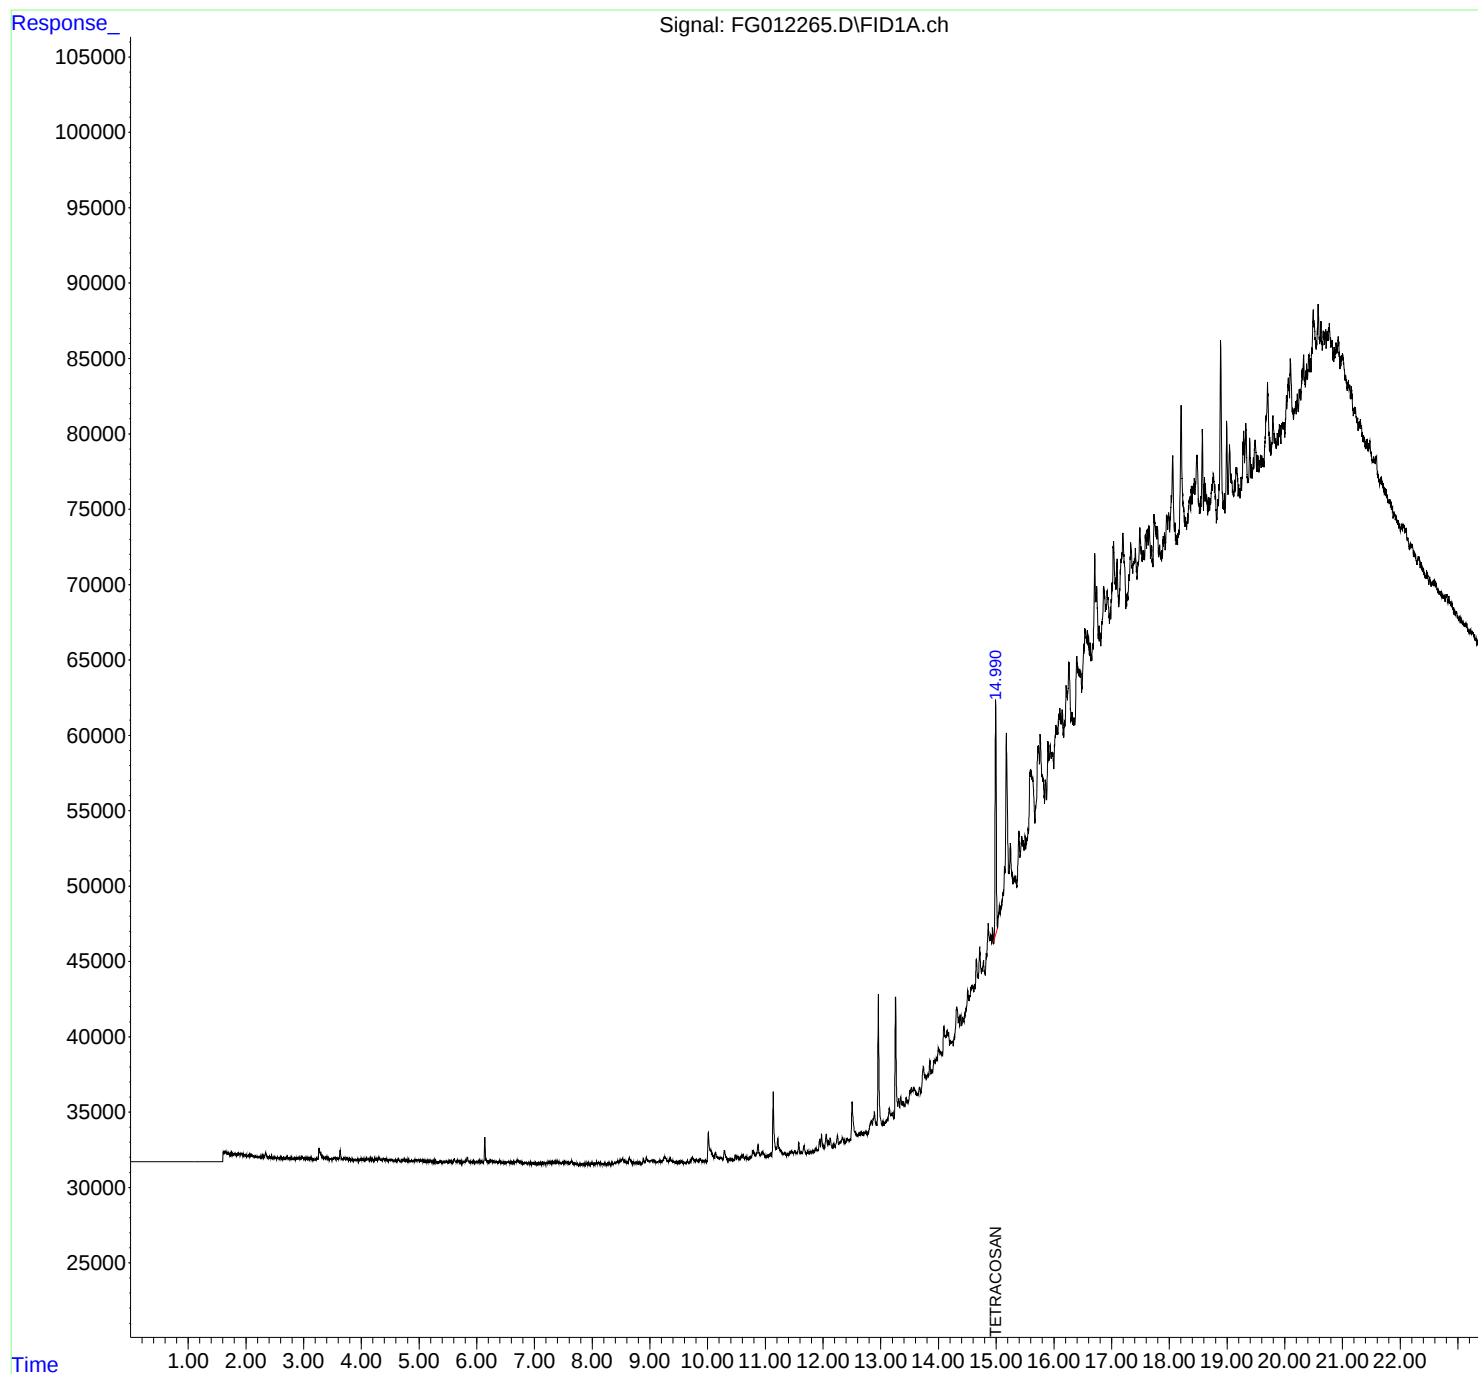

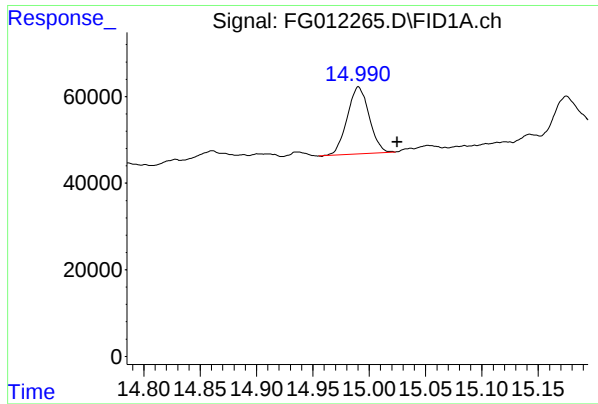

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.990 min
Delta R.T.: -0.035 min
Response: 209299
Conc: 1.57 ug/ml

Instrument :
FID_G
ClientSampleId :
DOMINICK-SP-TPH