

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062323\
Data File : FG012266.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2023 09:54
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/24/2023
Supervised By :Ankita Jodhani 06/26/2023

Integration File: autoint1.e
Quant Time: Jun 24 06:23:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.991	2046973	15.352 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062323\
Data File : FG012266.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2023 09:54
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 06/24/2023
Supervised By : Ankita Jodhani 06/26/2023

Integration File: autoint1.e
Quant Time: Jun 24 06:23:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060223.M
Quant Title :
QLast Update : Thu Jun 01 17:30:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

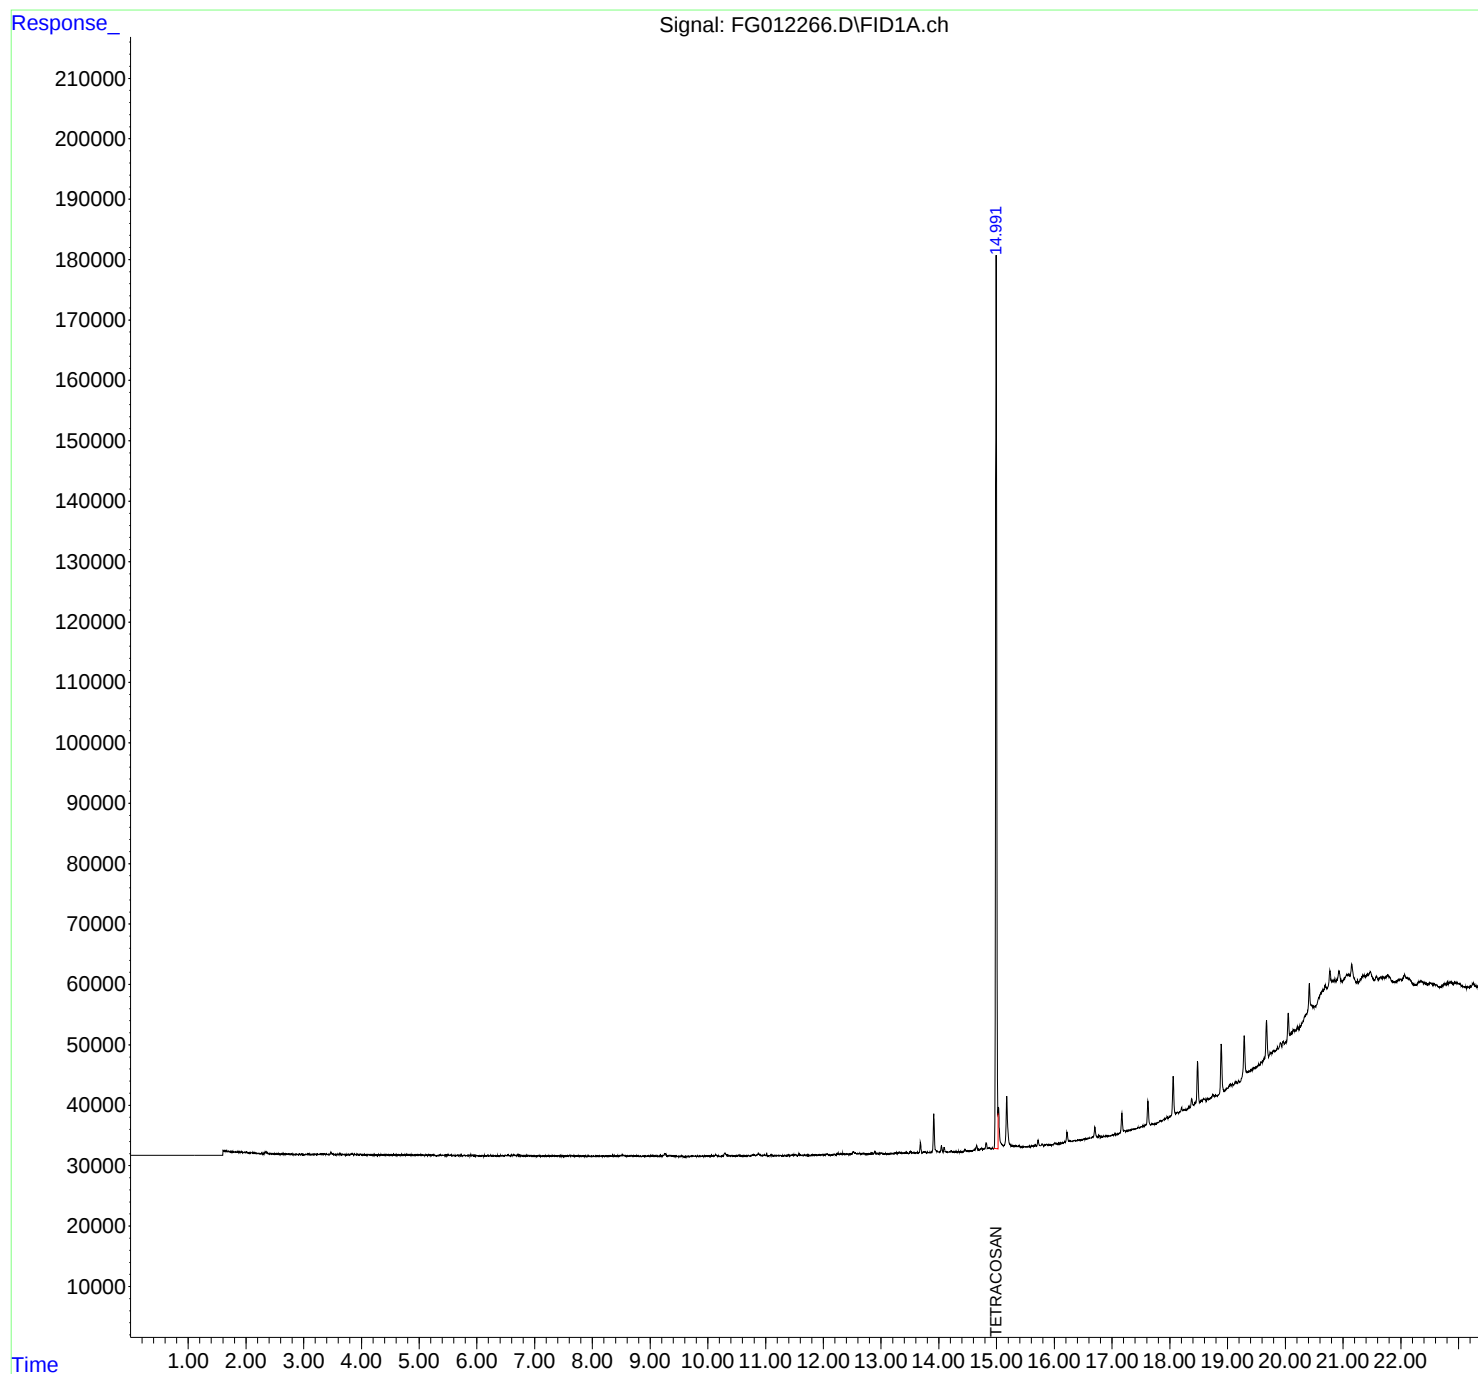

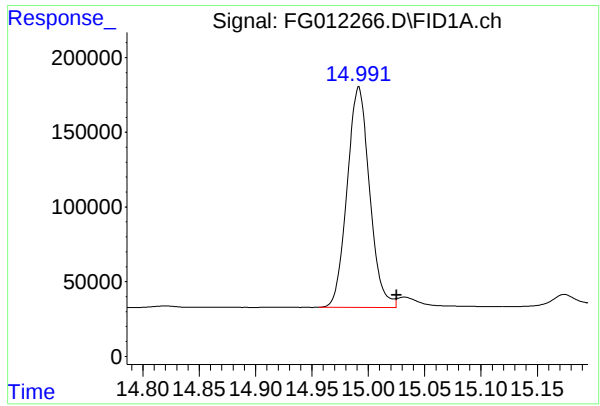

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.991 min
Delta R.T.: -0.034 min
Response: 2046973
Conc: 15.35 ug/ml

Instrument :

FID_G

ClientSampleId :

I.BLK

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 06/24/2023

Supervised By :Ankita Jodhani 06/26/2023