

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062323AL\
Data File : FG012269.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2023 14:46
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 17:12:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 062023.M
Quant Title : GC Extractables
QLast Update : Tue Jun 20 14:37:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14) T	n-Tetracosane (C24)	14.173	86747	0.652 ug/ml
18) T	n-Dotriacontane (C32)	17.892	23341	0.188 ug/ml
19) T	n-Tetratriacontane (C34)	18.678	14839	0.124 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062323AL\
Data File : FG012269.D
Signal(s) : FID1A.ch
Acq On : 23 Jun 2023 14:46
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 17:12:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 062023.M
Quant Title : GC Extractables
QLast Update : Tue Jun 20 14:37:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

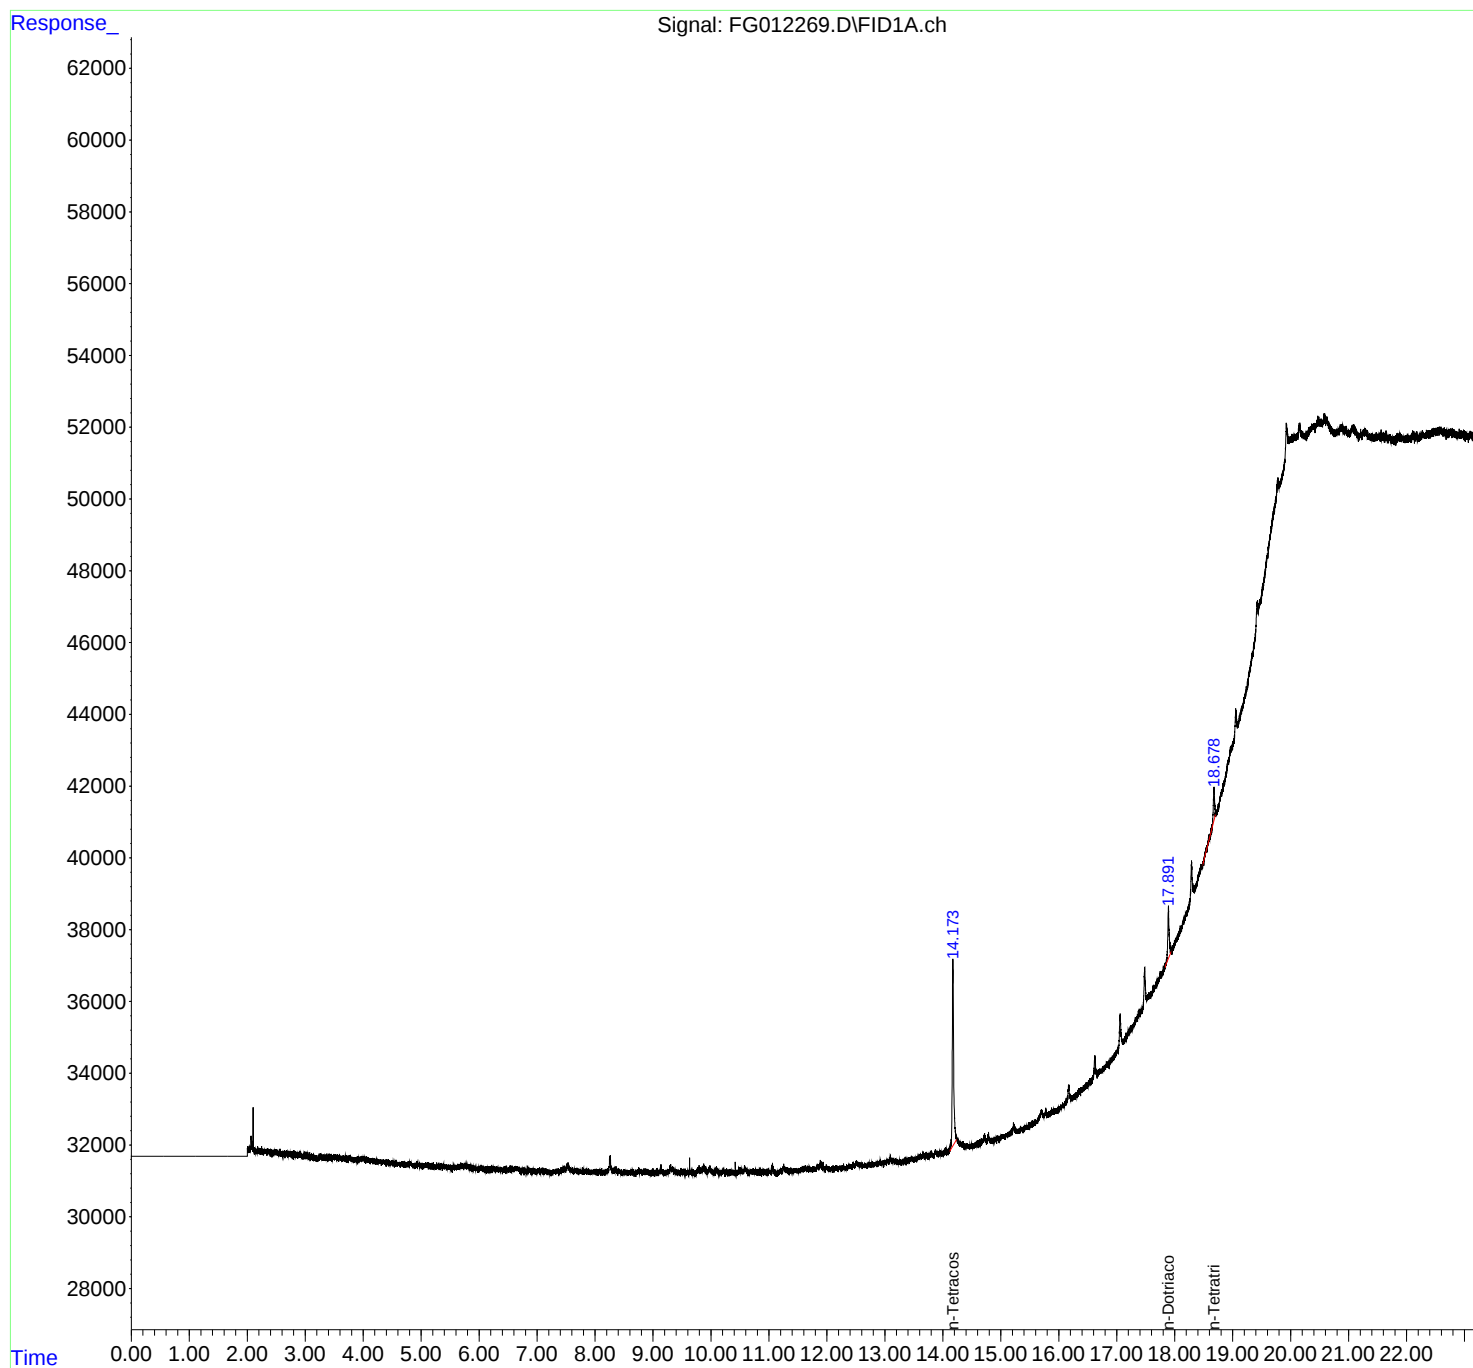


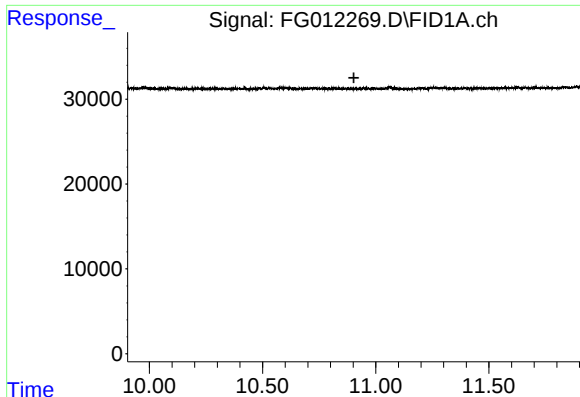

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.903 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

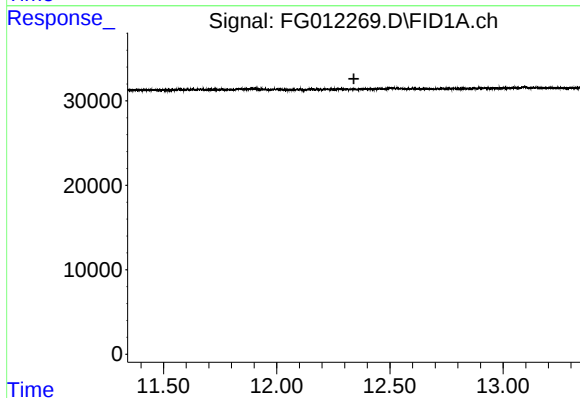


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 12.341 min
Response: 0
Conc: N.D.

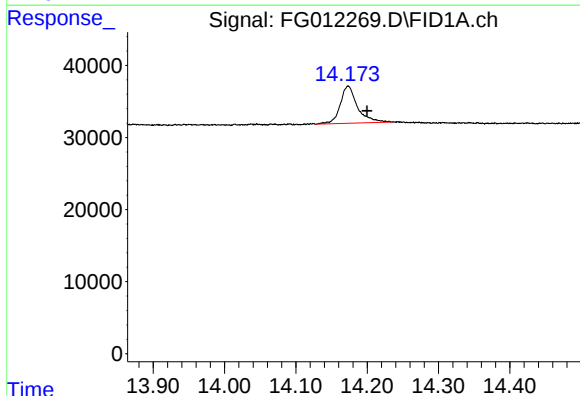


#14 n-Tetracosane (C24)

R.T.: 14.173 min
Delta R.T.: -0.027 min
Response: 86747
Conc: 0.65 ug/ml

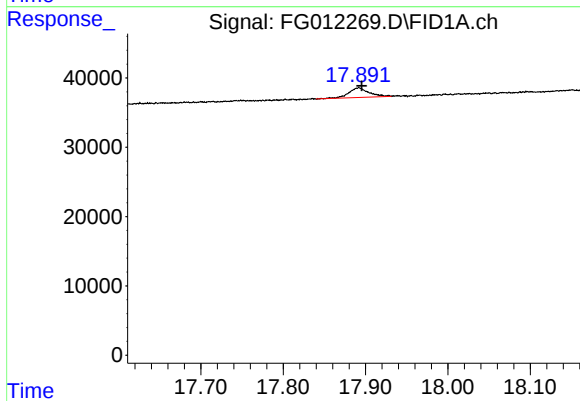

#18 n-Dotriacontane (C32)

R.T.: 17.892 min
Delta R.T.: -0.003 min
Response: 23341
Conc: 0.19 ug/ml

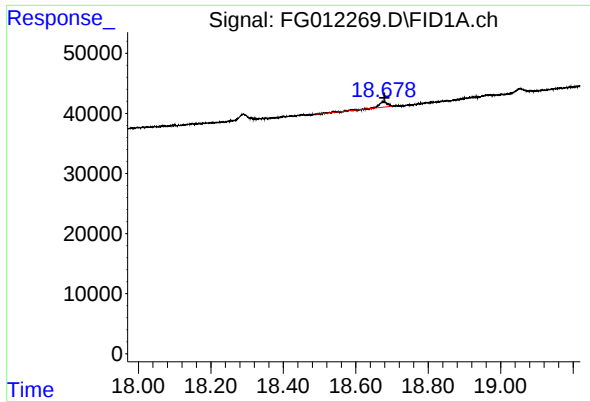

#19 n-Tetratriacontane (C34)

R.T.: 18.678 min
Delta R.T.: -0.001 min
Response: 14839
Conc: 0.12 ug/ml

Instrument :
FID_G
ClientSampleId :