

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG062422\  
 Data File : FG009950.D  
 Signal(s) : FID1A.ch  
 Acq On : 24 Jun 2022 09:36  
 Operator : AJ\MA  
 Sample : 50 PPM TRPH STD  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jun 25 01:00:24 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG060122.M  
 Quant Title :  
 QLast Update : Wed Jun 01 13:06:30 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.860 | 95976    | 0.912 ug/ml  |
| Target Compounds              |        |          |              |
| 1) N-OCTANE                   | 1.832  | 5085911  | 40.587 ug/ml |
| 2) N-DECANE                   | 4.343  | 5522002  | 43.725 ug/ml |
| 3) N-DODECANE                 | 6.522  | 5604093  | 44.422 ug/ml |
| 4) N-TETRADECANE              | 8.353  | 5714514  | 44.974 ug/ml |
| 5) N-HEXADECANE               | 9.962  | 5768345  | 45.734 ug/ml |
| 6) N-OCTADECANE               | 11.407 | 5841536  | 46.283 ug/ml |
| 7) N-EICOSANE                 | 12.720 | 5762237  | 47.115 ug/ml |
| 8) N-DOCOSANE                 | 13.921 | 5736833  | 47.576 ug/ml |
| 10) N-TETRACOSANE             | 15.028 | 5645712  | 48.171 ug/ml |
| 11) N-HEXACOSANE              | 16.050 | 5577091  | 49.160 ug/ml |
| 12) N-OCTACOSANE              | 17.002 | 5466493  | 47.771 ug/ml |
| 13) N-TRIACONTANE             | 17.894 | 5403163  | 50.178 ug/ml |
| 14) N-DOTRIACONTANE           | 18.727 | 5091152  | 48.368 ug/ml |
| 15) N-TETRATRIACONTANE        | 19.513 | 4551253  | 47.401 ug/ml |
| 16) N-HEXATRIACONTANE         | 20.256 | 3790487  | 46.902 ug/ml |
| 17) N-OCTATRIACONTANE         | 20.970 | 3329154  | 46.358 ug/ml |
| 18) N-TETRACONTANE            | 21.824 | 3406026  | 48.503 ug/ml |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG062422\  
Data File : FG009950.D  
Signal(s) : FID1A.ch  
Acq On : 24 Jun 2022 09:36  
Operator : AJ\MA  
Sample : 50 PPM TRPH STD  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jun 25 01:00:24 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG060122.M  
Quant Title :  
QLast Update : Wed Jun 01 13:06:30 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

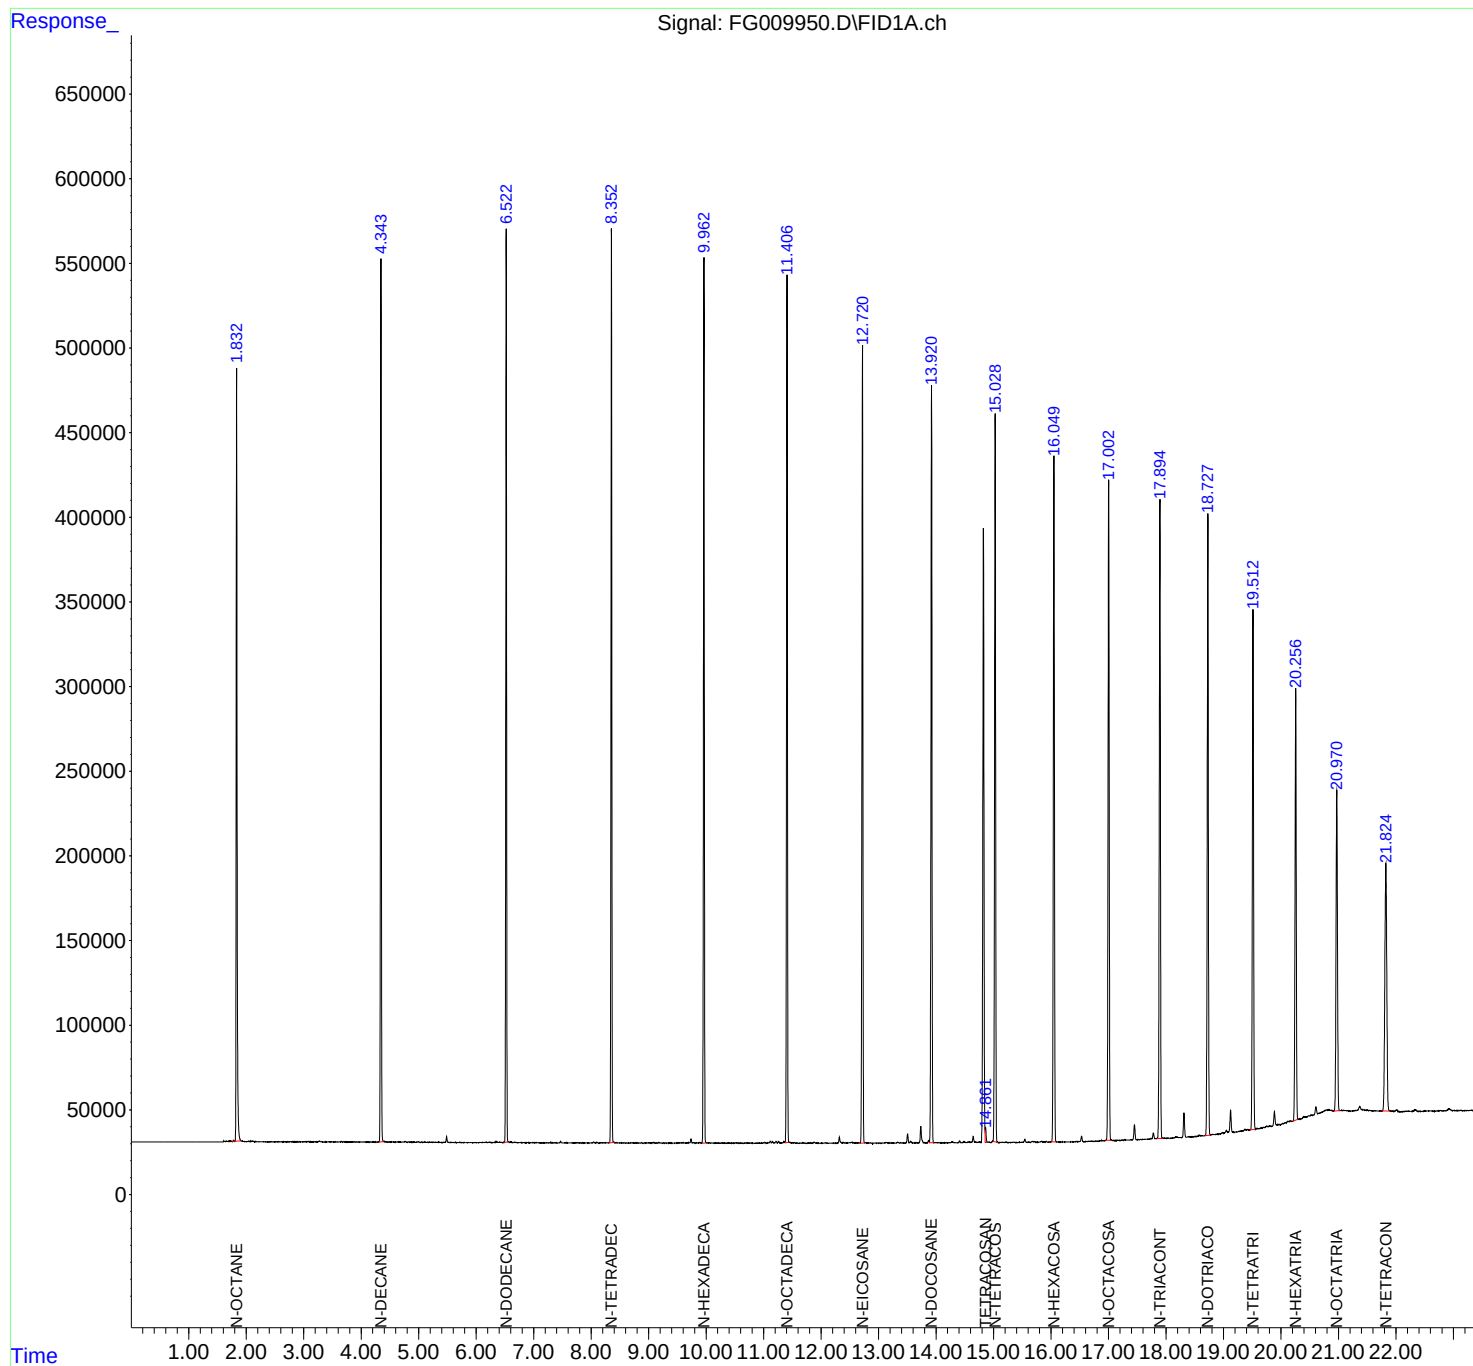


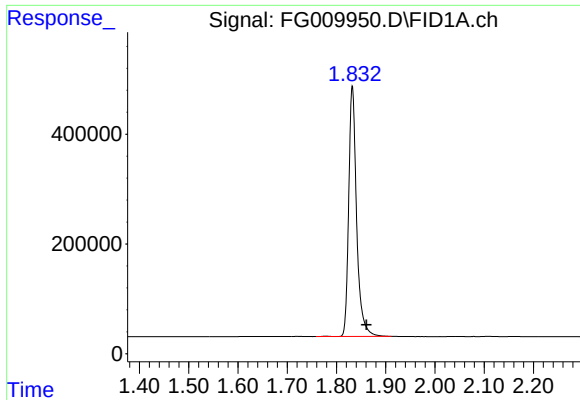

#1 N-OCTANE


R.T.: 1.832 min  
Delta R.T.: -0.029 min  
Response: 5085911  
Conc: 40.59 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

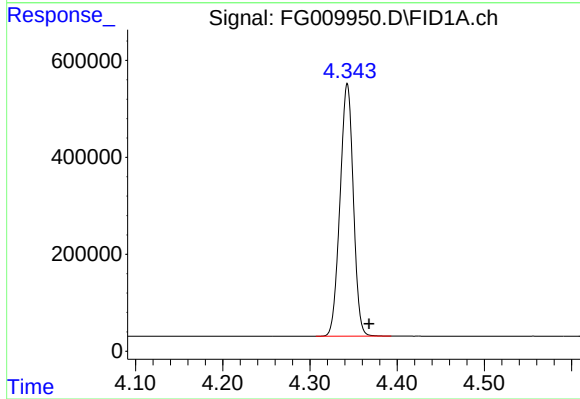


#2 N-DECANE

R.T.: 4.343 min  
Delta R.T.: -0.025 min  
Response: 5522002  
Conc: 43.73 ug/ml

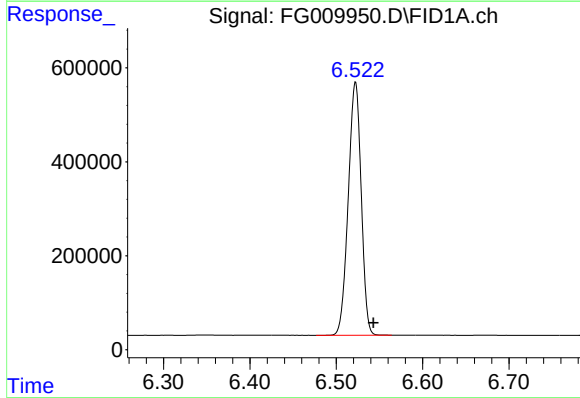


#3 N-DODECANE

R.T.: 6.522 min  
Delta R.T.: -0.021 min  
Response: 5604093  
Conc: 44.42 ug/ml

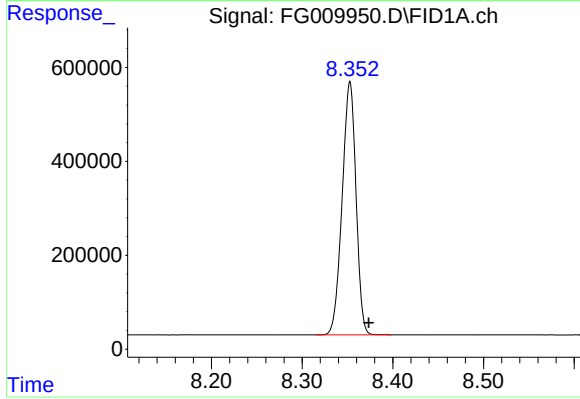

#4 N-TETRADECANE


R.T.: 8.353 min  
Delta R.T.: -0.020 min  
Response: 5714514  
Conc: 44.97 ug/ml

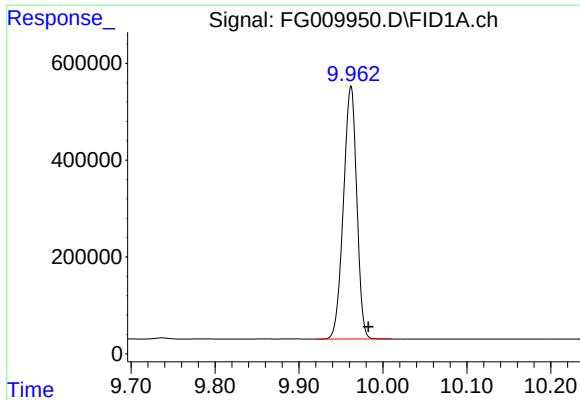

#5 N-HEXADECANE


R.T.: 9.962 min  
Delta R.T.: -0.021 min  
Response: 5768345  
Conc: 45.73 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

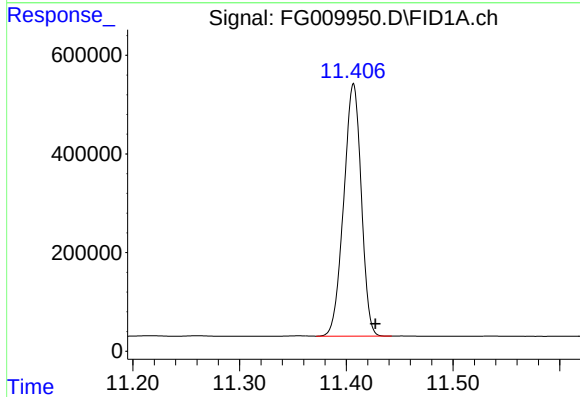


#6 N-OCTADECANE

R.T.: 11.407 min  
Delta R.T.: -0.021 min  
Response: 5841536  
Conc: 46.28 ug/ml

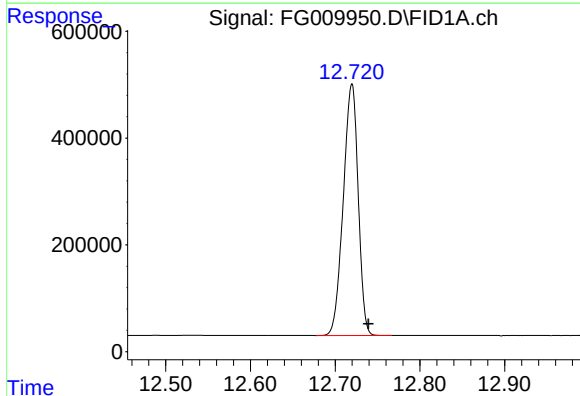


#7 N-EICOSANE

R.T.: 12.720 min  
Delta R.T.: -0.019 min  
Response: 5762237  
Conc: 47.11 ug/ml

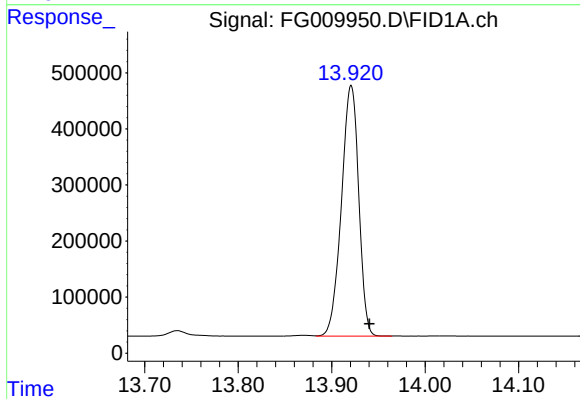

#8 N-DOCOSANE


R.T.: 13.921 min  
Delta R.T.: -0.019 min  
Response: 5736833  
Conc: 47.58 ug/ml

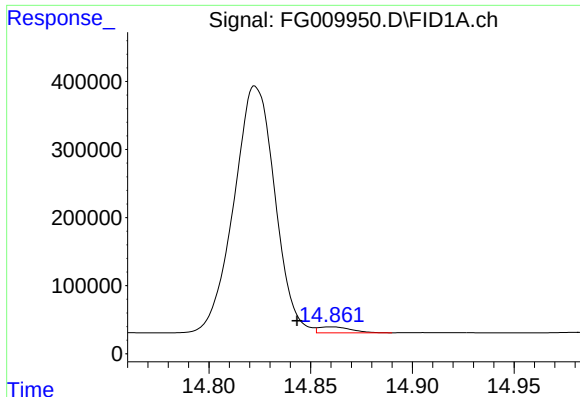

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.860 min  
Delta R.T.: 0.017 min  
Response: 95976  
Conc: 0.91 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

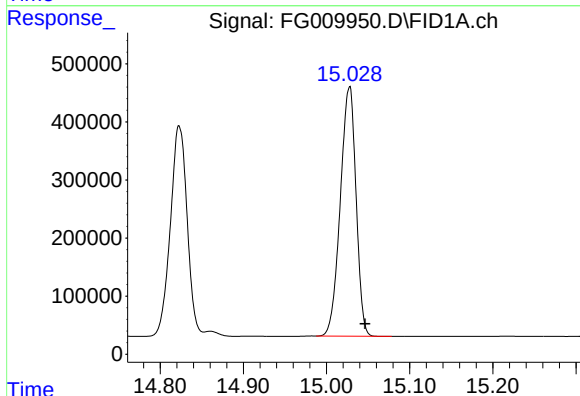


#10 N-TETRACOSANE

R.T.: 15.028 min  
Delta R.T.: -0.019 min  
Response: 5645712  
Conc: 48.17 ug/ml

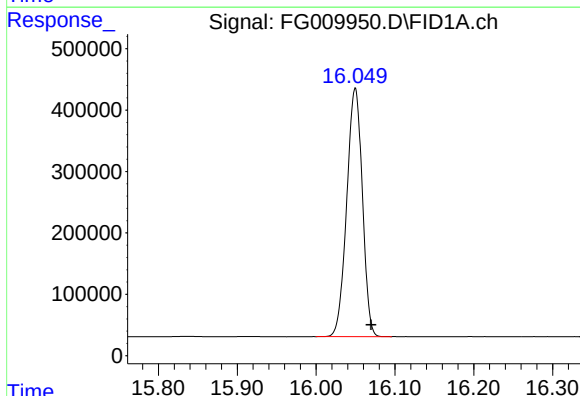


#11 N-HEXACOSANE

R.T.: 16.050 min  
Delta R.T.: -0.020 min  
Response: 5577091  
Conc: 49.16 ug/ml

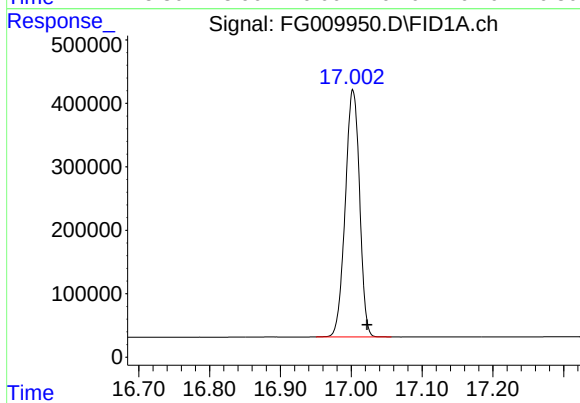

#12 N-OCTACOSANE


R.T.: 17.002 min  
Delta R.T.: -0.020 min  
Response: 5466493  
Conc: 47.77 ug/ml

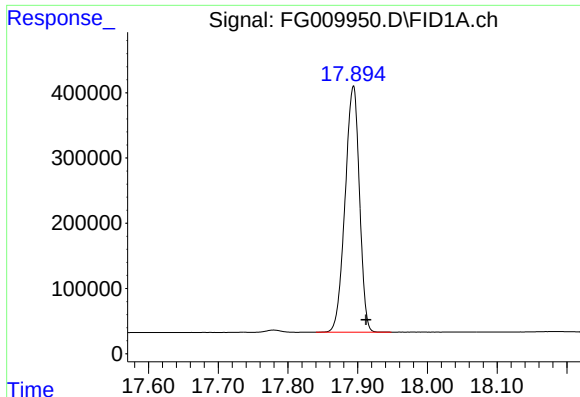

#13 N-TRIACONTANE


R.T.: 17.894 min  
Delta R.T.: -0.018 min  
Response: 5403163  
Conc: 50.18 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

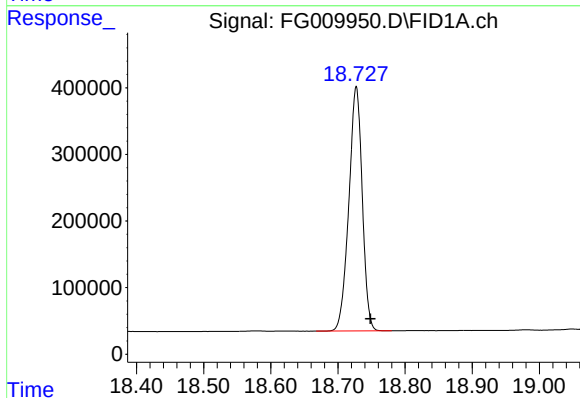


#14 N-DOTRIACONTANE

R.T.: 18.727 min  
Delta R.T.: -0.021 min  
Response: 5091152  
Conc: 48.37 ug/ml

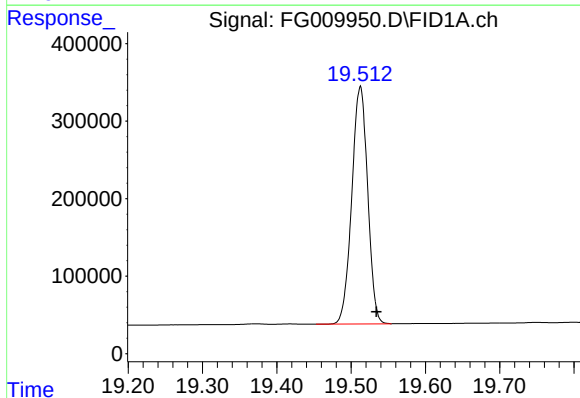


#15 N-TETRATRIACONTANE

R.T.: 19.513 min  
Delta R.T.: -0.022 min  
Response: 4551253  
Conc: 47.40 ug/ml

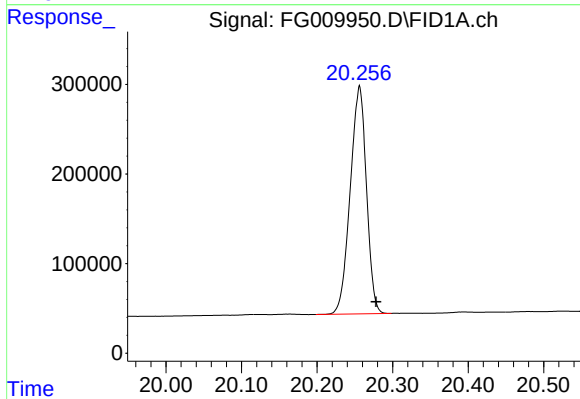

#16 N-HEXATRIACONTANE


R.T.: 20.256 min  
Delta R.T.: -0.022 min  
Response: 3790487  
Conc: 46.90 ug/ml

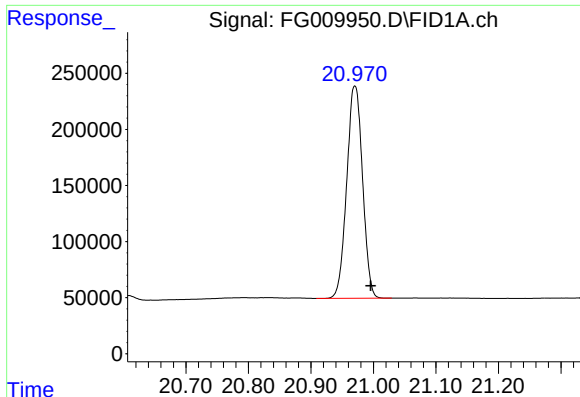

#17 N-OCTATRIACONTANE

R.T.: 20.970 min  
Delta R.T.: -0.025 min  
Response: 3329154  
Conc: 46.36 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

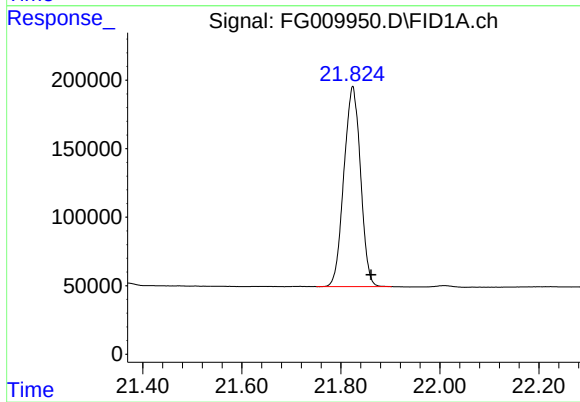

#18 N-TETRACONTANE

R.T.: 21.824 min  
Delta R.T.: -0.037 min  
Response: 3406026  
Conc: 48.50 ug/ml