

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062422\
Data File : FG009971.D
Signal(s) : FID1A.ch
Acq On : 25 Jun 2022 03:53
Operator : AJ\MA
Sample : N3455-13 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SP-EXC-2-3-GR

Integration File: autoint1.e
Quant Time: Jun 25 05:00:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.825	150753	1.432 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062422\
Data File : FG009971.D
Signal(s) : FID1A.ch
Acq On : 25 Jun 2022 03:53
Operator : AJ\MA
Sample : N3455-13 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SP-EXC-2-3-GR

Integration File: autoint1.e
Quant Time: Jun 25 05:00:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

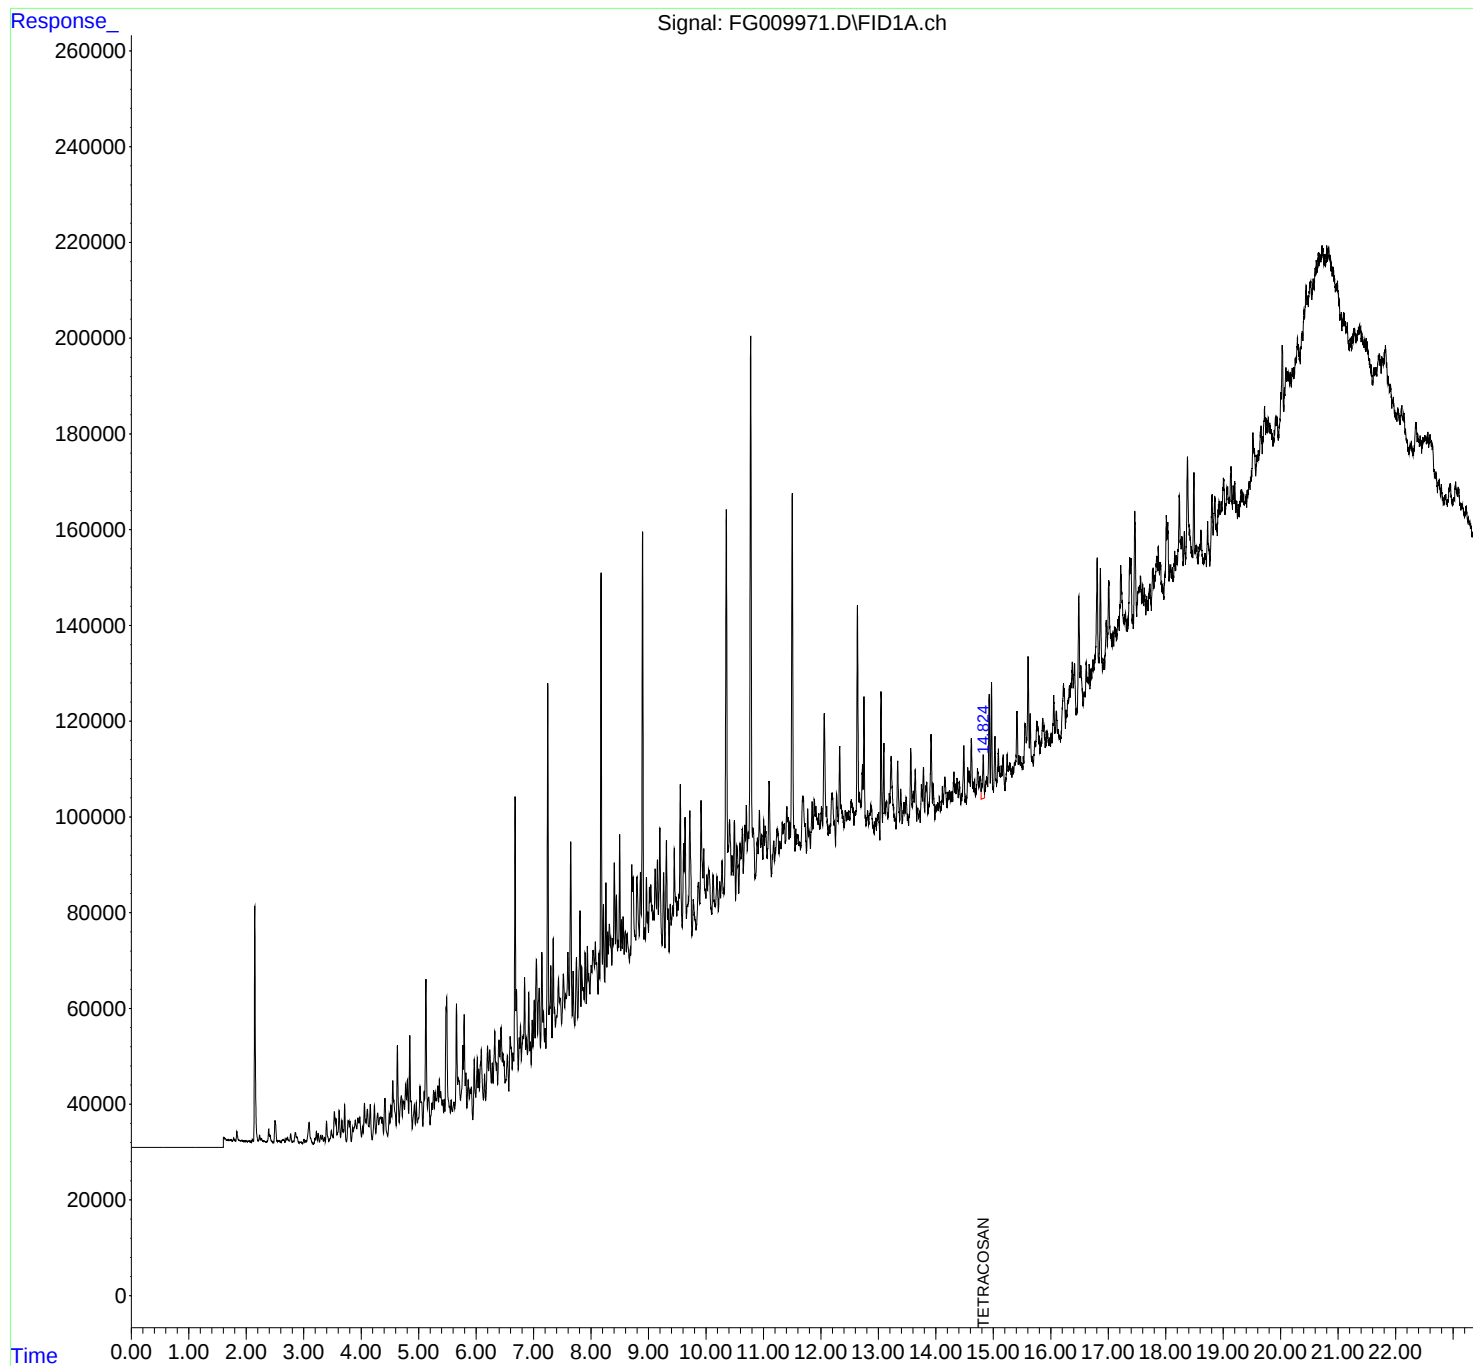

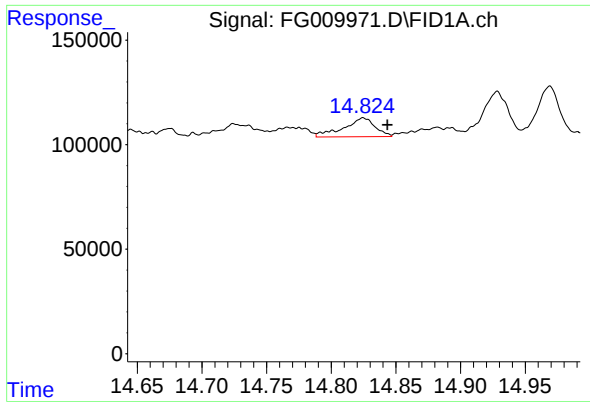

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.825 min
Delta R.T.: -0.019 min
Response: 150753
Conc: 1.43 ug/ml

Instrument :
FID_G
ClientSampleId :
SP-EXC-2-3-GR