

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062423\
Data File : FG012288.D
Signal(s) : FID1A.ch
Acq On : 24 Jun 2023 14:11
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 02:48:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FG062423.M
Quant Title :
QLast Update : Sun Jun 25 02:41:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) N-TETRACOSANE	15.170	115192	0.727 ug/ml
16) N-HEXATRIACONTANE	20.453	58475	0.436 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062423\
Data File : FG012288.D
Signal(s) : FID1A.ch
Acq On : 24 Jun 2023 14:11
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 02:48:11 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FG062423.M
Quant Title :
QLast Update : Sun Jun 25 02:41:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

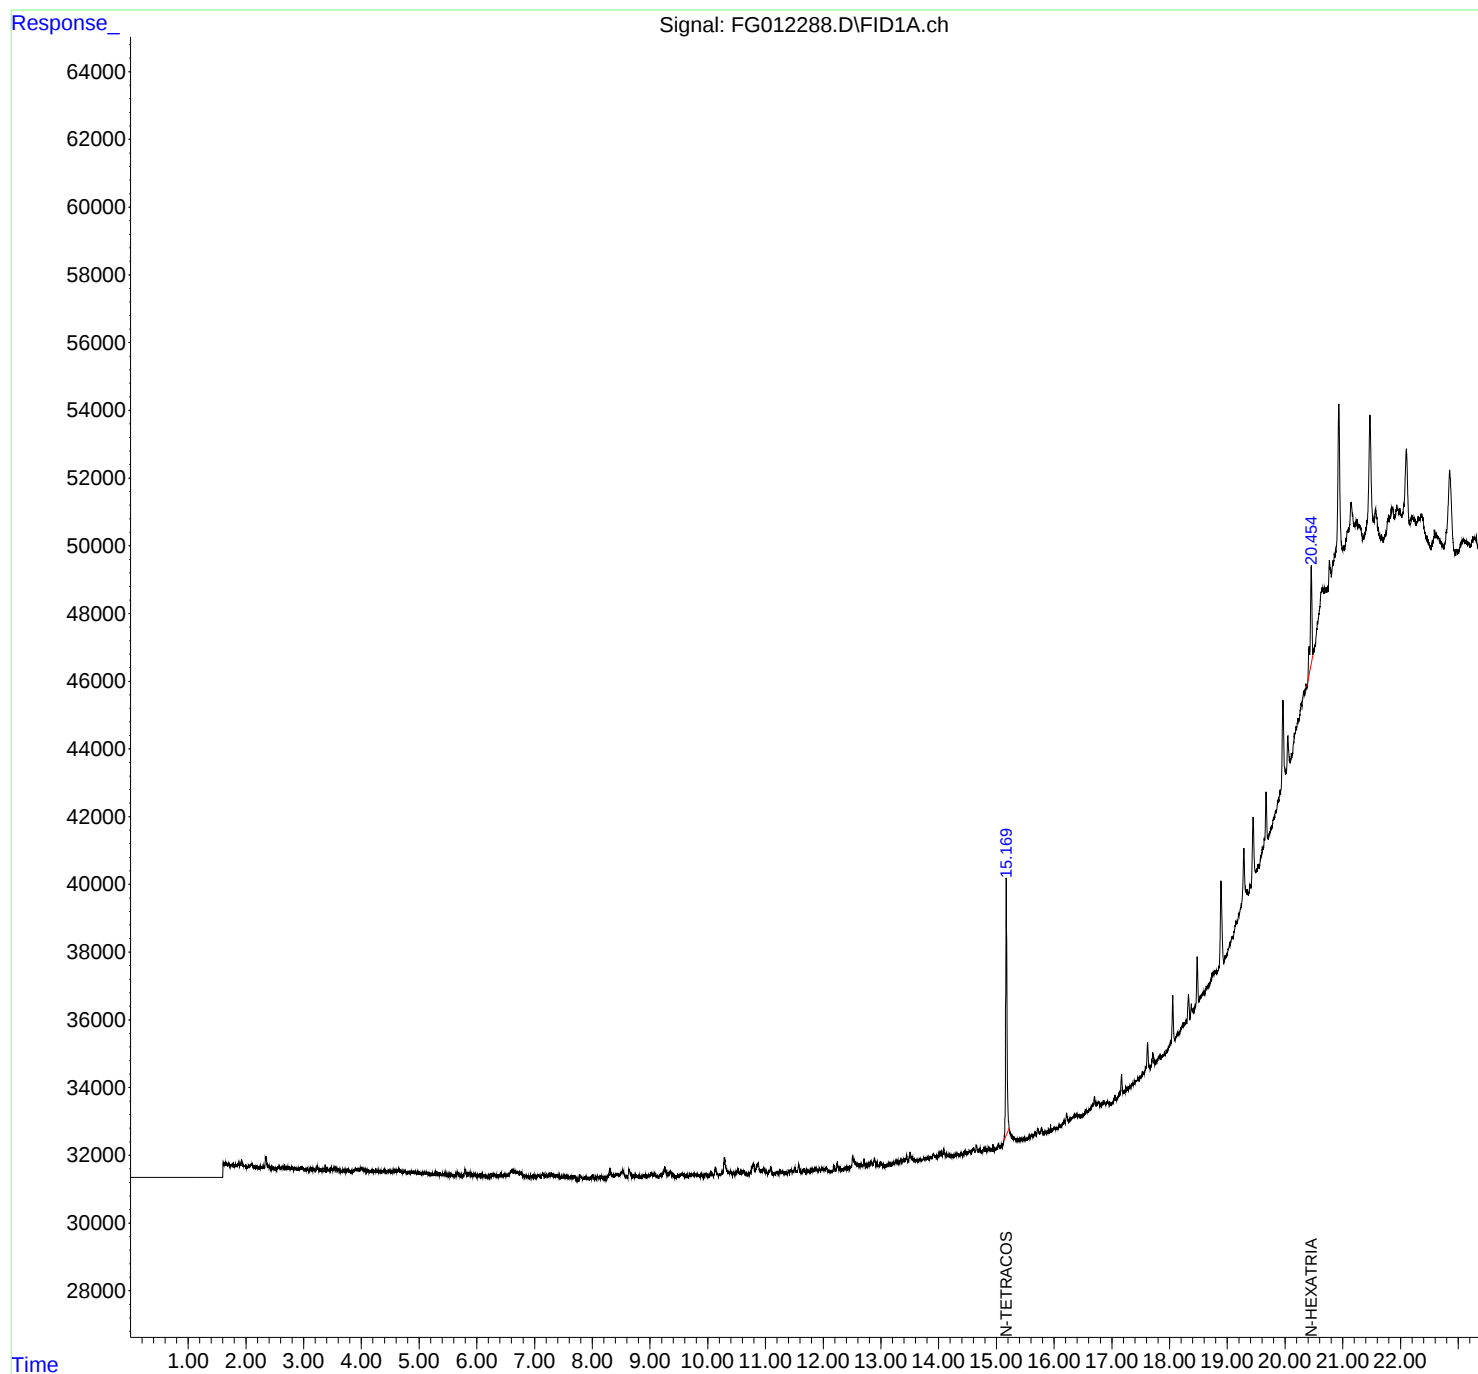


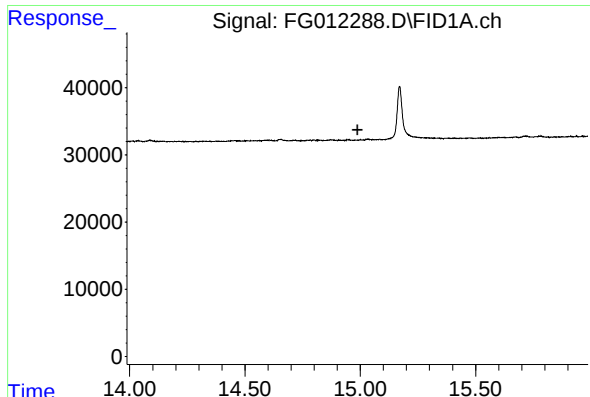

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.988 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

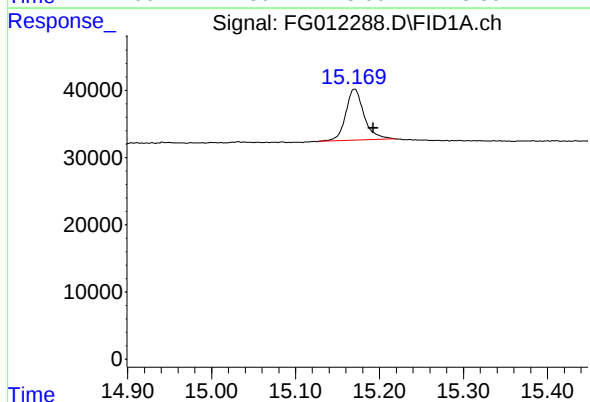

#10 N-TETRACOSANE

R.T.: 15.170 min
Delta R.T.: -0.023 min
Response: 115192
Conc: 0.73 ug/ml

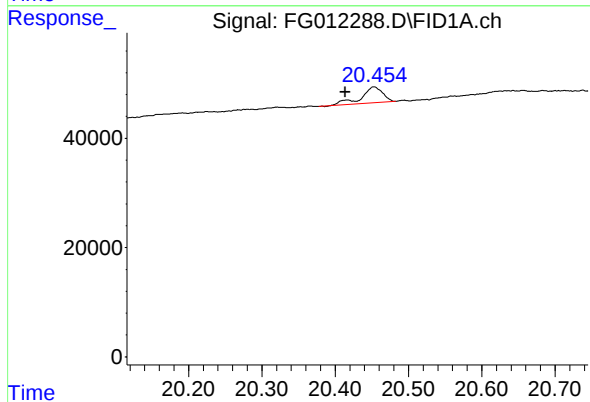

#16 N-HEXATRIACONTANE

R.T.: 20.453 min
Delta R.T.: 0.039 min
Response: 58475
Conc: 0.44 ug/ml