

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062424\
Data File : FG013884.D
Signal(s) : FID1A.ch
Acq On : 24 Jun 2024 14:25
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 04:20:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052824.M
Quant Title :
QLast Update : Tue May 28 12:12:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.892	80550	0.717 ug/ml
18) N-TETRACONTANE	22.108	144195	2.208 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062424\
Data File : FG013884.D
Signal(s) : FID1A.ch
Acq On : 24 Jun 2024 14:25
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 04:20:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052824.M
Quant Title :
QLast Update : Tue May 28 12:12:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

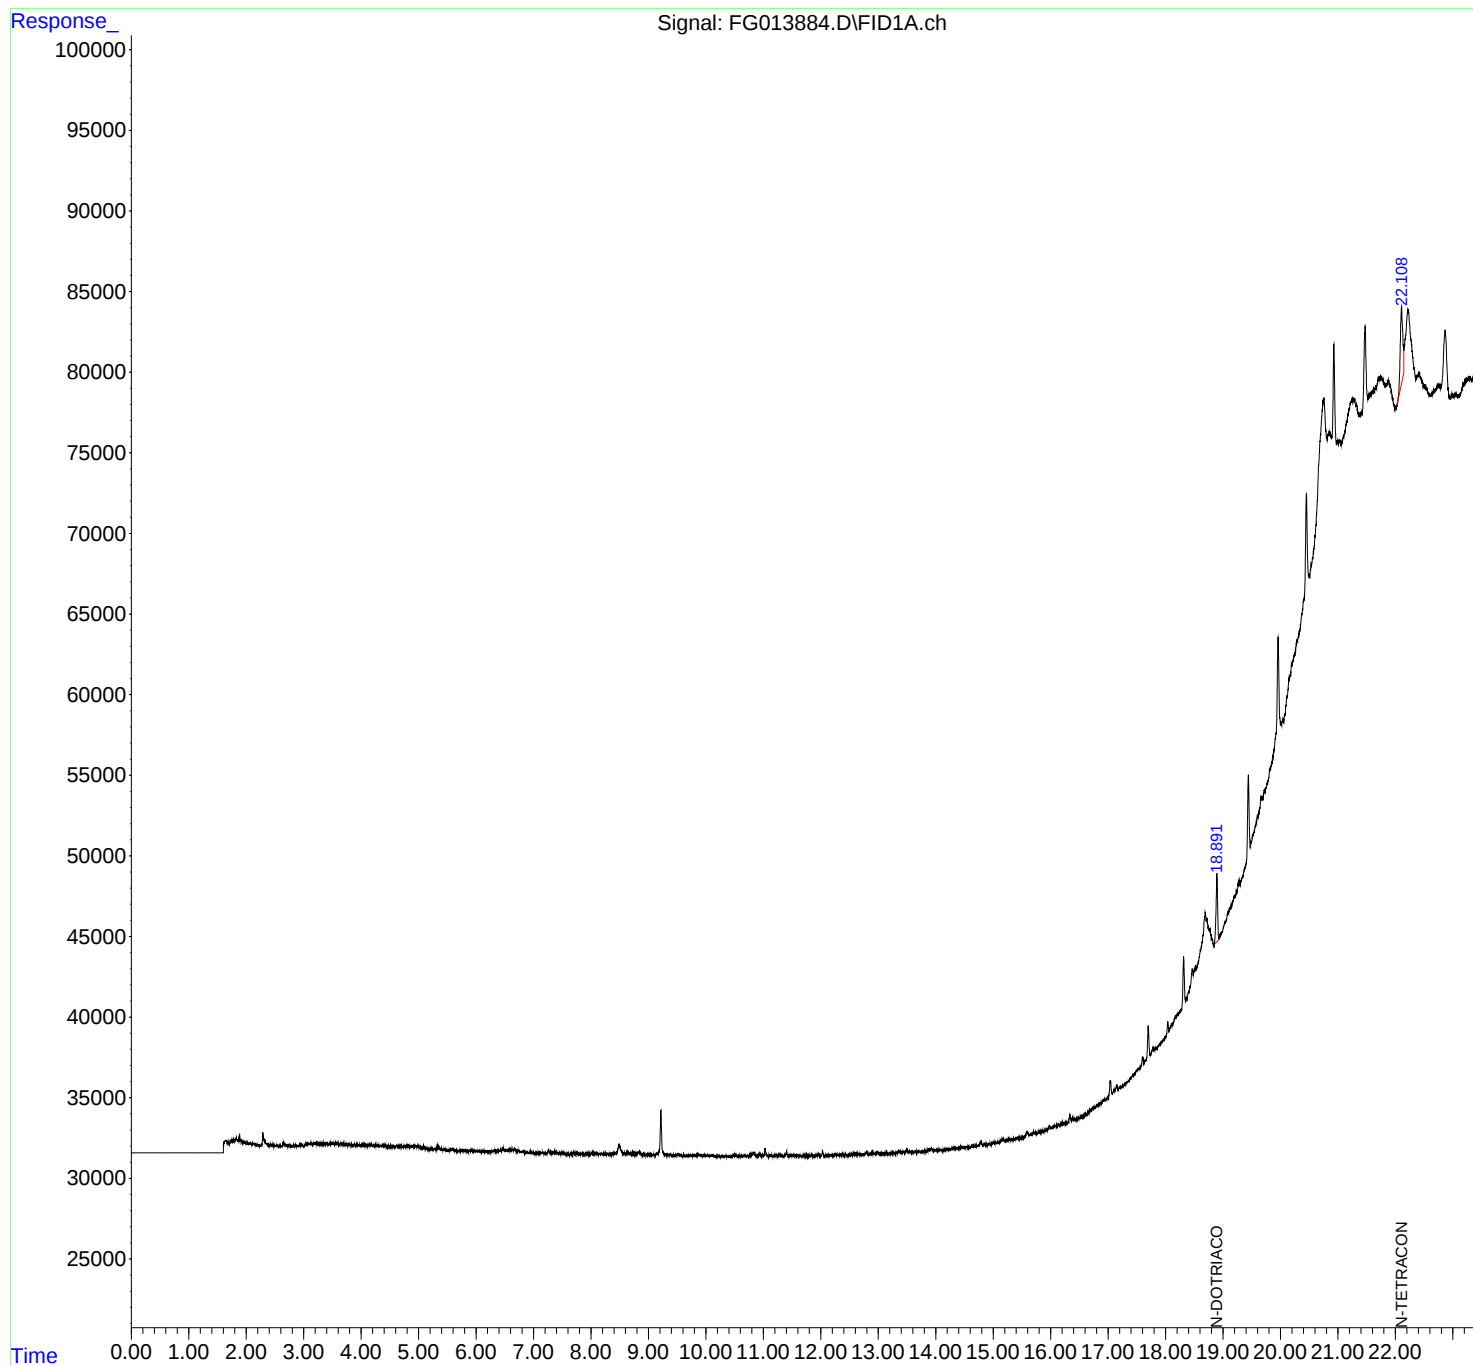


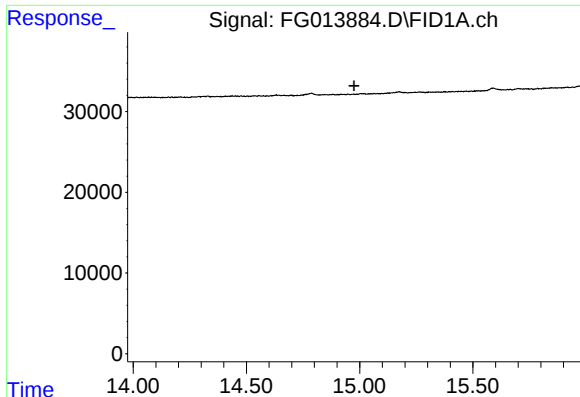

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.975 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

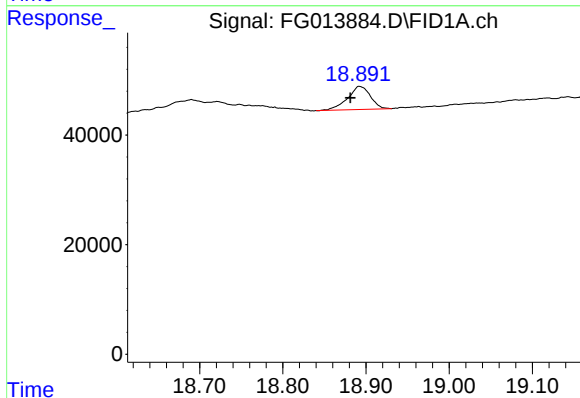

#14 N-DOTRIACONTANE

R.T.: 18.892 min
Delta R.T.: 0.011 min
Response: 80550
Conc: 0.72 ug/ml

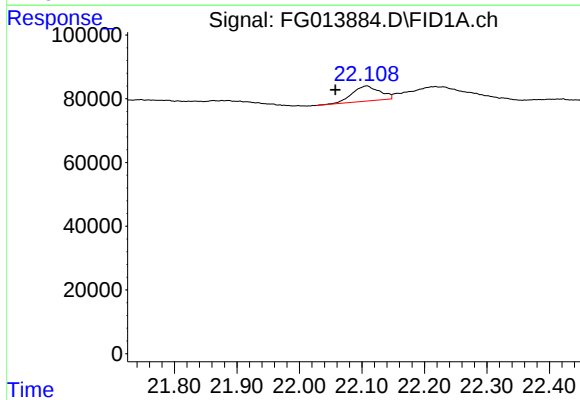

#18 N-TETRACONTANE

R.T.: 22.108 min
Delta R.T.: 0.050 min
Response: 144195
Conc: 2.21 ug/ml