

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062424\
Data File : FG013885.D
Signal(s) : FID1A.ch
Acq On : 24 Jun 2024 14:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 25 04:21:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052824.M
Quant Title :
QLast Update : Tue May 28 12:12:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.967	1807391	16.401 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062424\
Data File : FG013885.D
Signal(s) : FID1A.ch
Acq On : 24 Jun 2024 14:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 25 04:21:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG052824.M
Quant Title :
QLast Update : Tue May 28 12:12:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

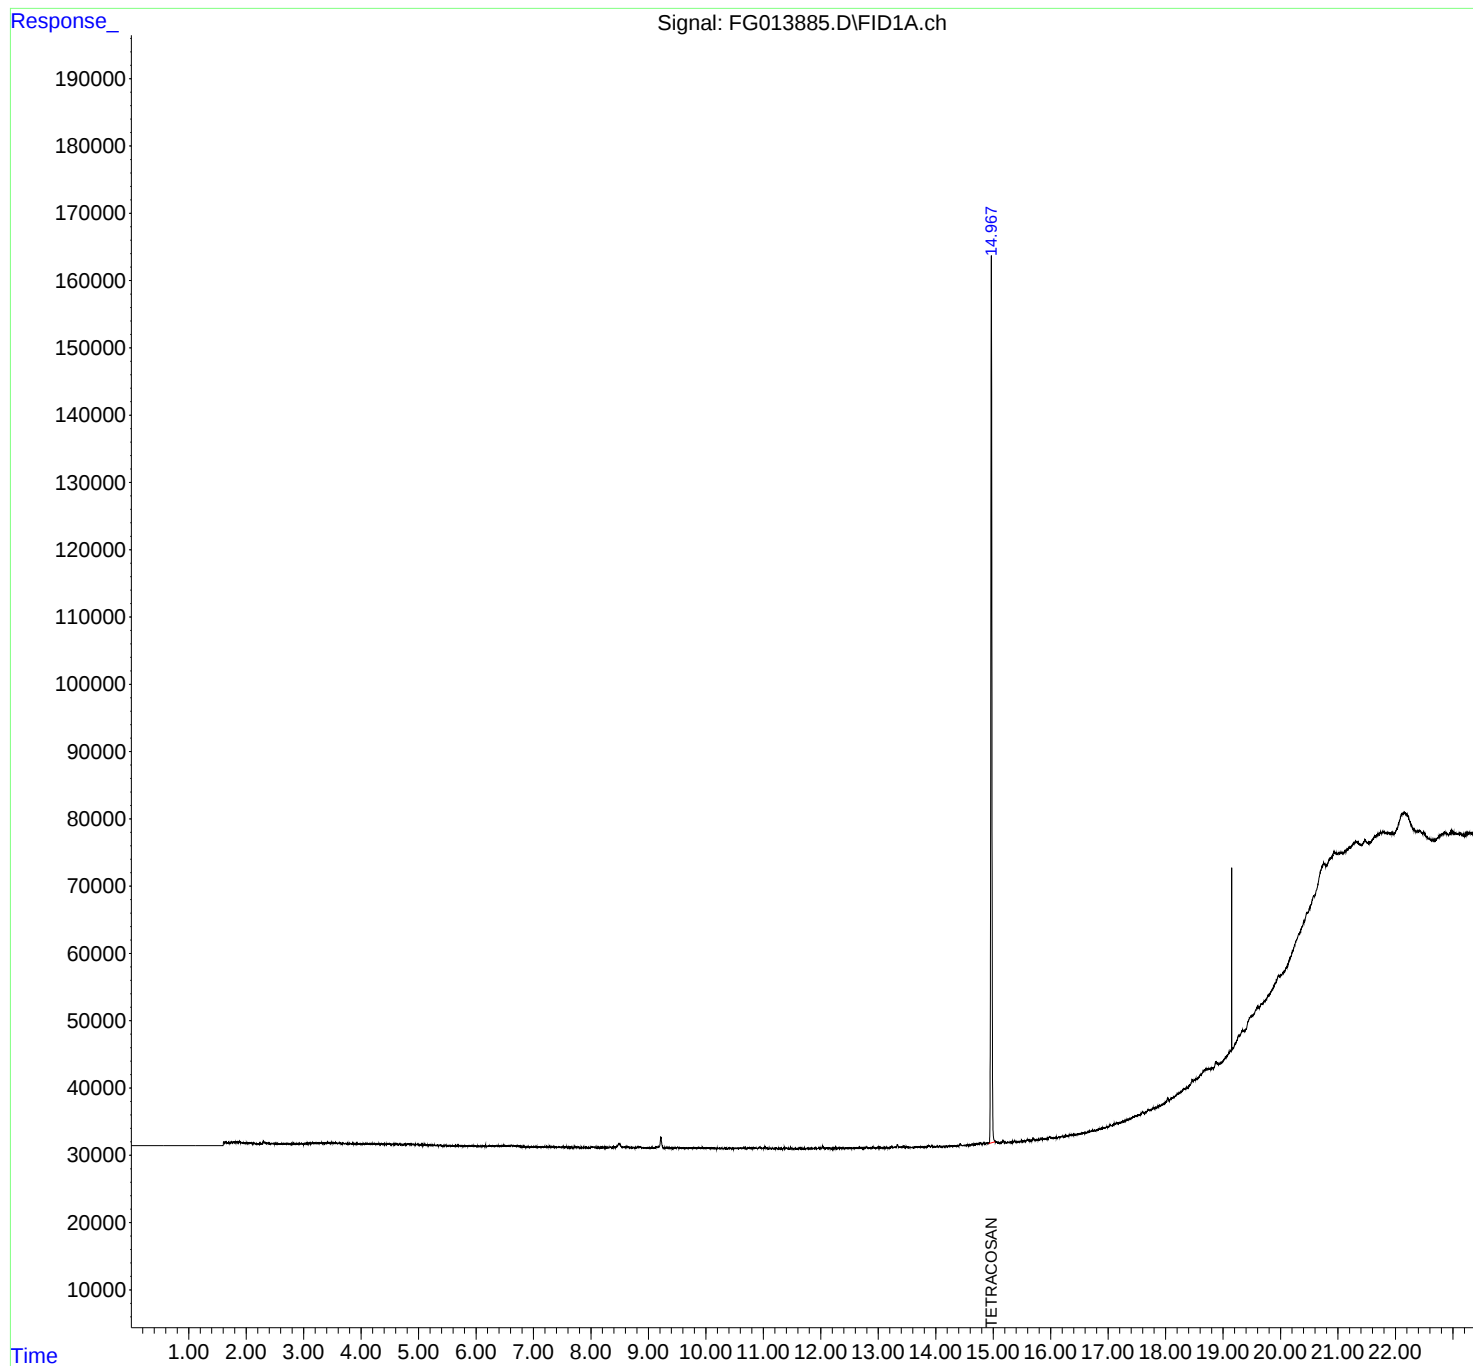

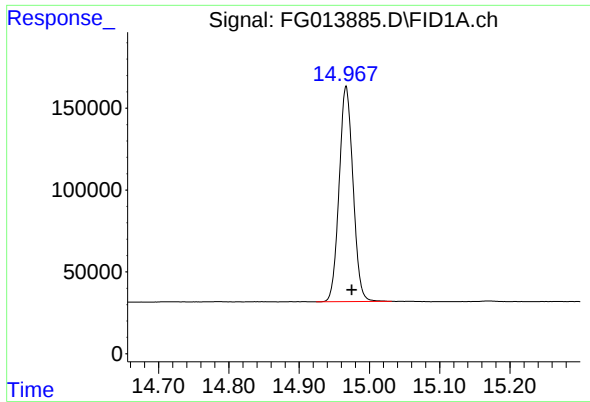

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.967 min
Delta R.T.: -0.008 min
Response: 1807391
Conc: 16.40 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK