

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062518\
 Data File : FG001470.D
 Signal(s) : FID1A.ch
 Acq On : 25 Jun 2018 11:55
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Jun 26 01:09:13 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.533	6478837	52.997 ug/ml
Target Compounds			
2) N-DECANE	4.273	7351594	53.633 ug/ml
3) N-DODECANE	6.289	7476142	53.930 ug/ml
4) N-TETRADECANE	8.082	7541528	53.970 ug/ml
5) N-HEXADECANE	9.682	7580538	53.867 ug/ml
6) N-OCTADECANE	11.124	7606922	53.664 ug/ml
7) N-EICOSANE	12.434	7526748	53.451 ug/ml
8) N-DOCOSANE	13.633	7436790	53.064 ug/ml
10) N-TETRACOSANE	14.737	7329272	52.710 ug/ml
11) N-HEXACOSANE	15.759	7228571	52.181 ug/ml
12) N-OCTACOSANE	16.711	7123742	51.630 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062518\
Data File : FG001470.D
Signal(s) : FID1A.ch
Acq On : 25 Jun 2018 11:55
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Jun 26 01:09:13 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

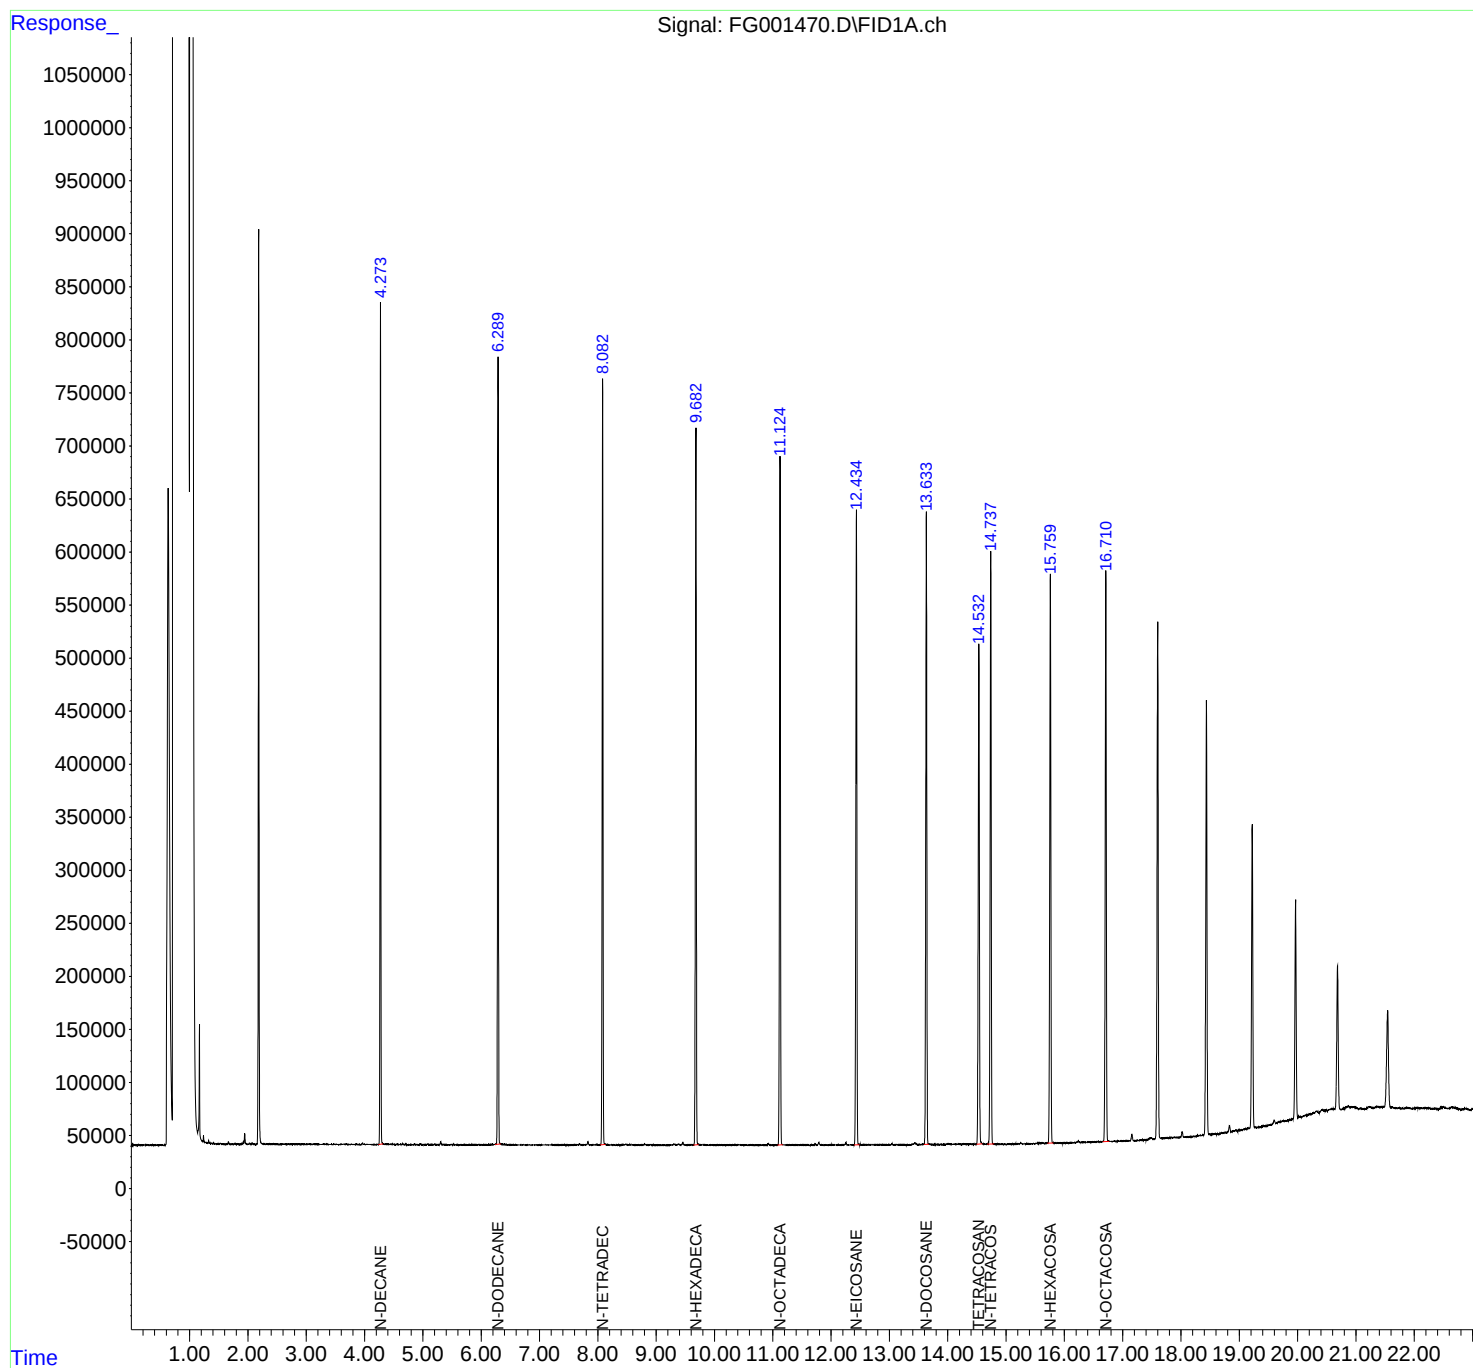

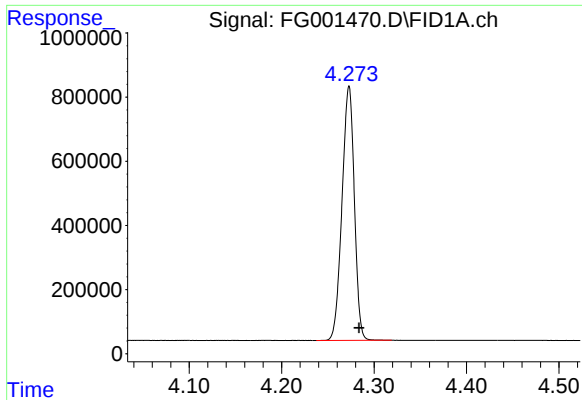


#2 N-DECANE

R.T.: 4.273 min
Delta R.T.: -0.011 min
Response: 7351594
Conc: 53.63 ug/ml

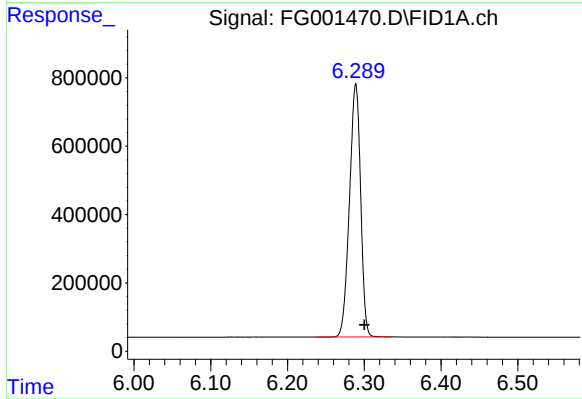


#3 N-DODECANE

R.T.: 6.289 min
Delta R.T.: -0.011 min
Response: 7476142
Conc: 53.93 ug/ml

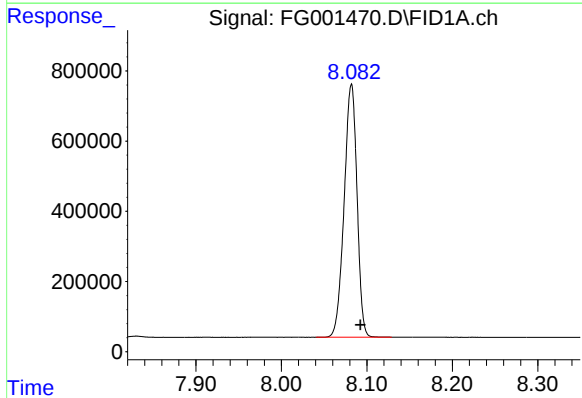


#4 N-TETRADECANE

R.T.: 8.082 min
Delta R.T.: -0.011 min
Response: 7541528
Conc: 53.97 ug/ml

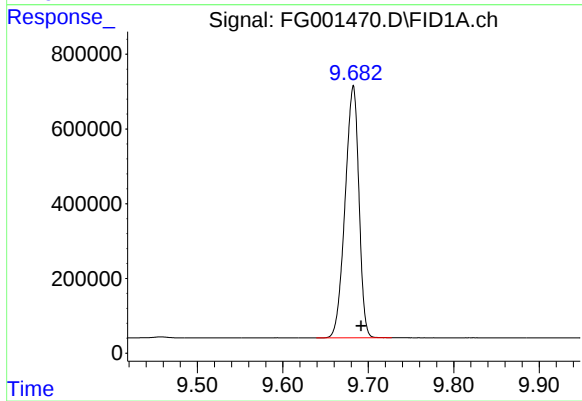


#5 N-HEXADECANE

R.T.: 9.682 min
Delta R.T.: -0.009 min
Response: 7580538
Conc: 53.87 ug/ml

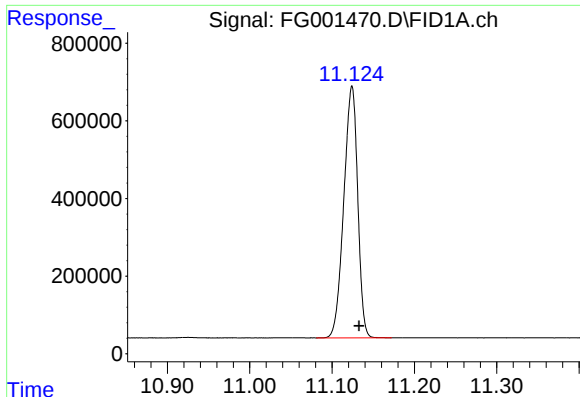


#6 N-OCTADECANE

R.T.: 11.124 min
Delta R.T.: -0.009 min
Response: 7606922
Conc: 53.66 ug/ml

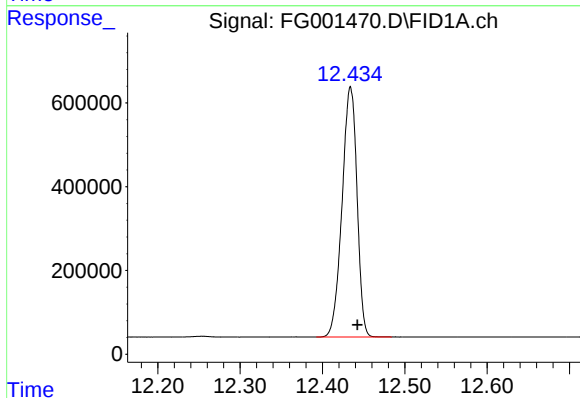


#7 N-EICOSANE

R.T.: 12.434 min
Delta R.T.: -0.008 min
Response: 7526748
Conc: 53.45 ug/ml

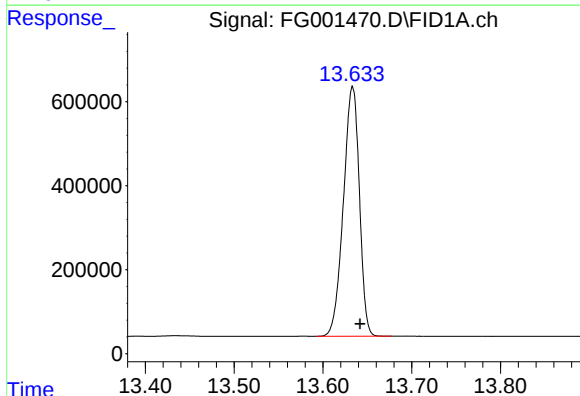


#8 N-DOCOSANE

R.T.: 13.633 min
Delta R.T.: -0.008 min
Response: 7436790
Conc: 53.06 ug/ml

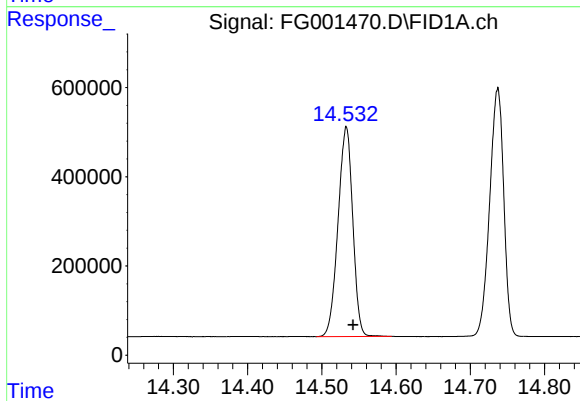


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.533 min
Delta R.T.: -0.009 min
Response: 6478837
Conc: 53.00 ug/ml

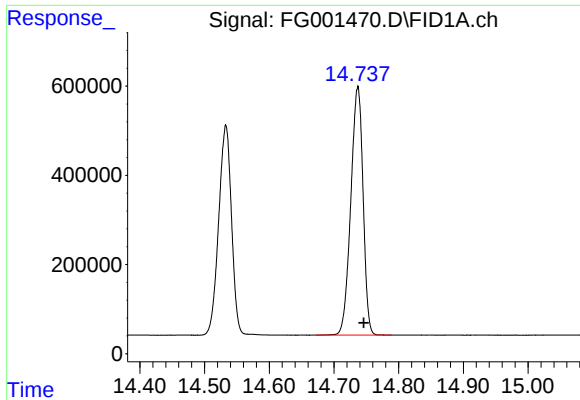


#10 N-TETRACOSANE

R.T.: 14.737 min
Delta R.T.: -0.009 min
Response: 7329272
Conc: 52.71 ug/ml

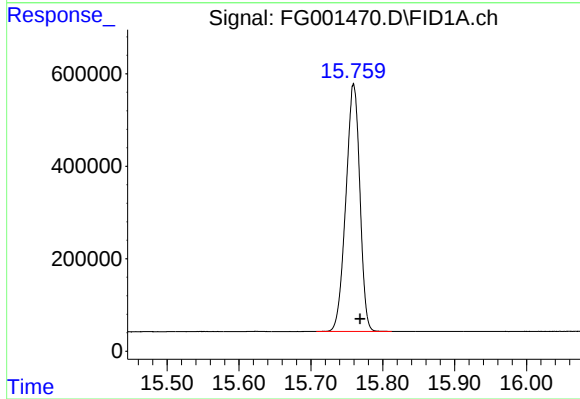

#11 N-HEXACOSANE

R.T.: 15.759 min
Delta R.T.: -0.009 min
Response: 7228571
Conc: 52.18 ug/ml

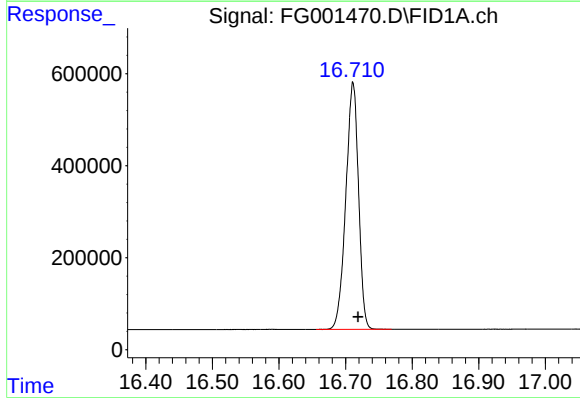

#12 N-OCTACOSANE

R.T.: 16.711 min
Delta R.T.: -0.007 min
Response: 7123742
Conc: 51.63 ug/ml