

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062519\
Data File : FG005191.D
Signal(s) : FID1A.ch
Acq On : 25 Jun 2019 13:11
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 26 03:24:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.503	4784503	32.197 ug/ml
11)	N-HEXACOSANE	15.997	34308	0.236 ug/ml
12)	N-OCTACOSANE	16.952	3900982	27.425 ug/ml
13)	N-TRIACONTANE	17.839	121258	0.866 ug/ml
14)	N-DOTRIACONTANE	18.676	117768	0.875 ug/ml
15)	N-TETRATRIACONTANE	19.461	78007	0.608 ug/ml
16)	N-HEXATRIACONTANE	20.205	47469	0.398 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062519\
Data File : FG005191.D
Signal(s) : FID1A.ch
Acq On : 25 Jun 2019 13:11
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 26 03:24:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

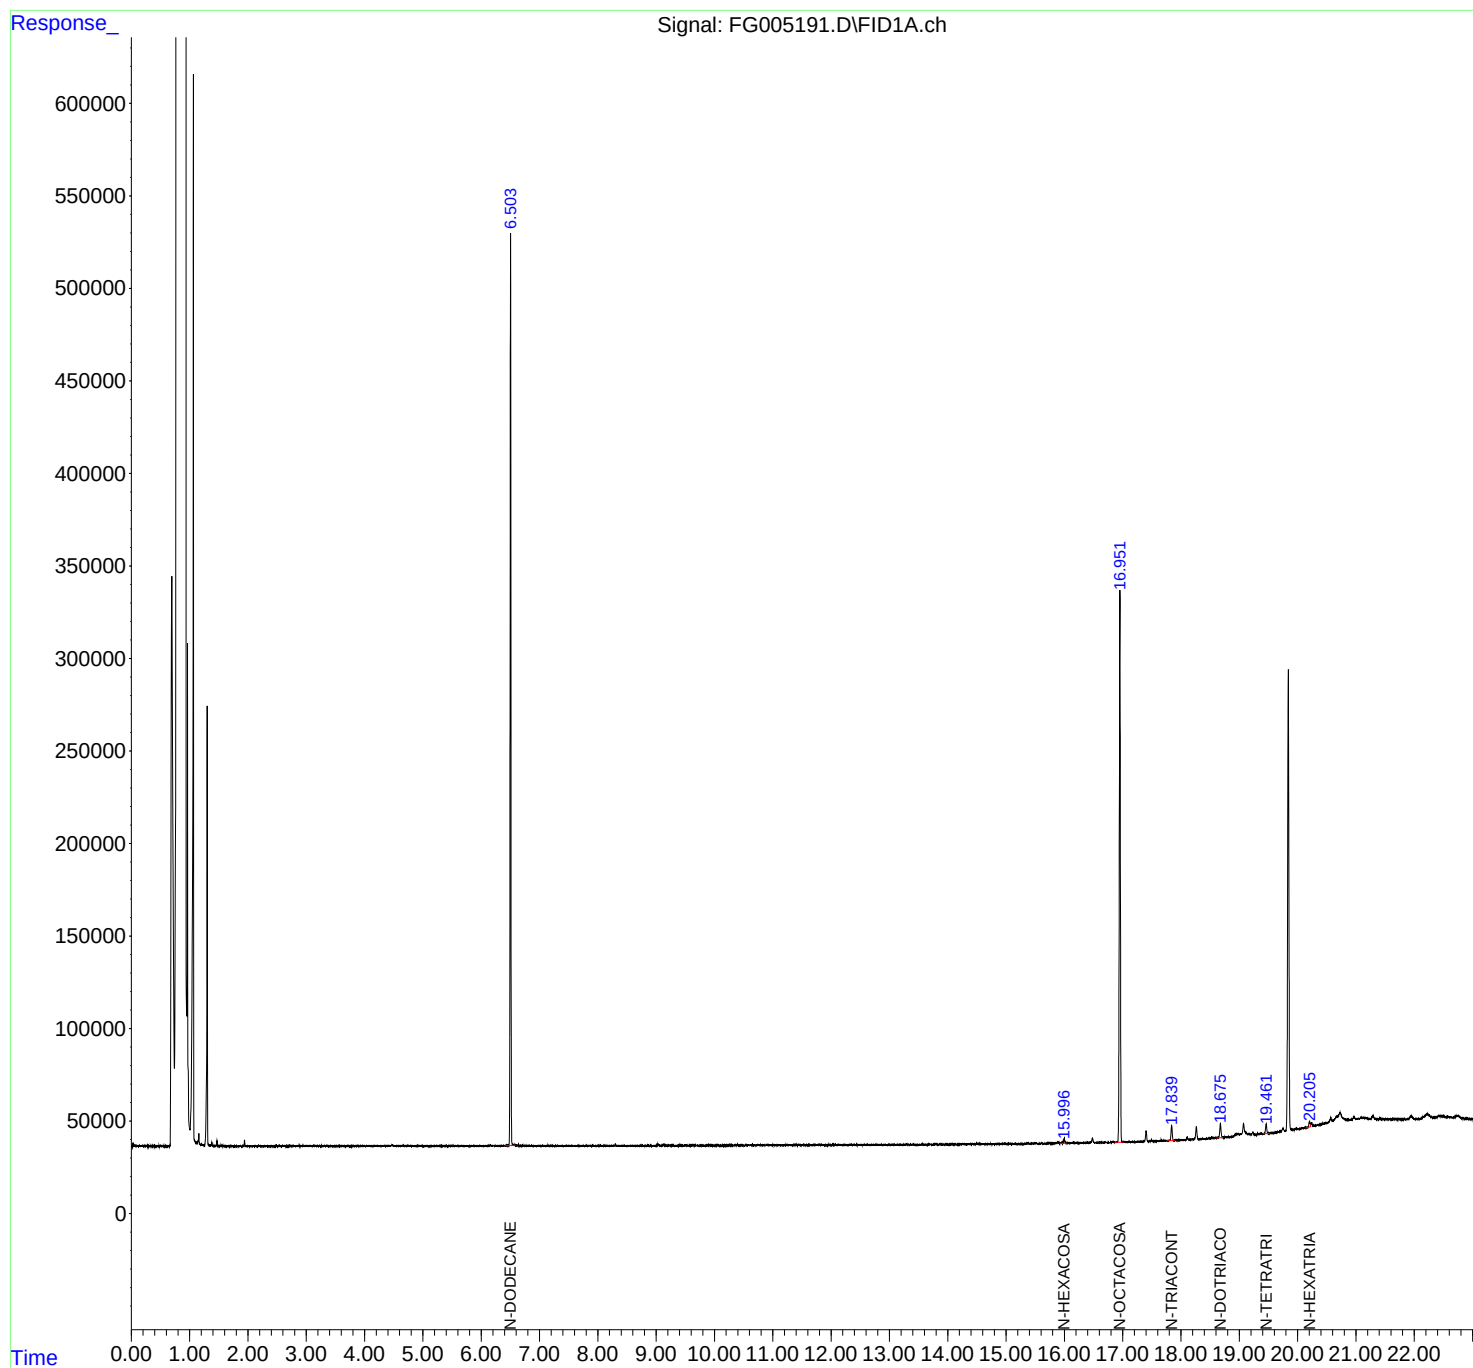

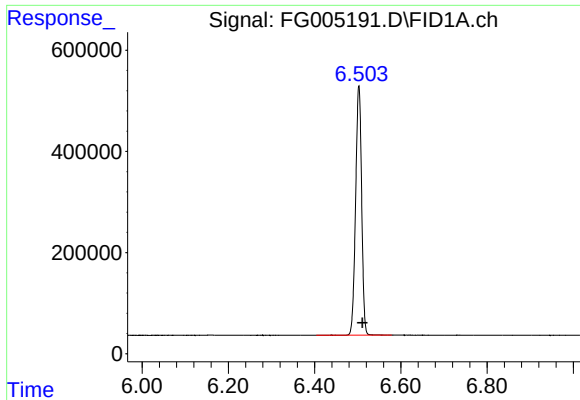


#3 N-DODECANE

R.T.: 6.503 min
Delta R.T.: -0.008 min
Response: 4784503
Conc: 32.20 ug/ml

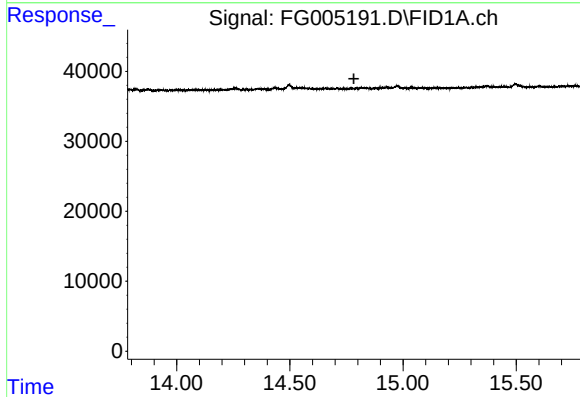


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.783 min
Response: 0
Conc: N.D.

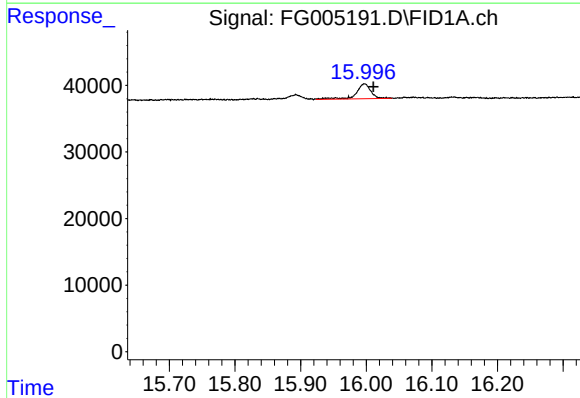


#11 N-HEXACOSANE

R.T.: 15.997 min
Delta R.T.: -0.013 min
Response: 34308
Conc: 0.24 ug/ml

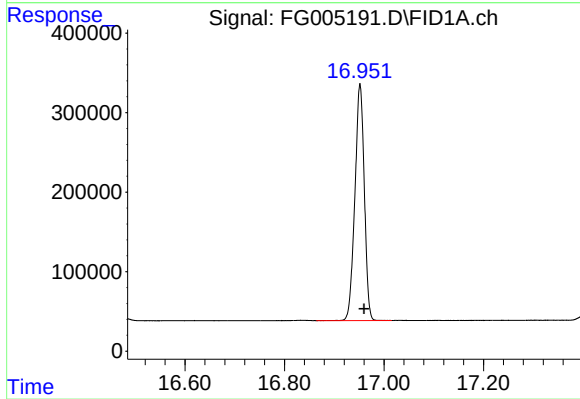


#12 N-OCTACOSANE

R.T.: 16.952 min
Delta R.T.: -0.008 min
Response: 3900982
Conc: 27.43 ug/ml

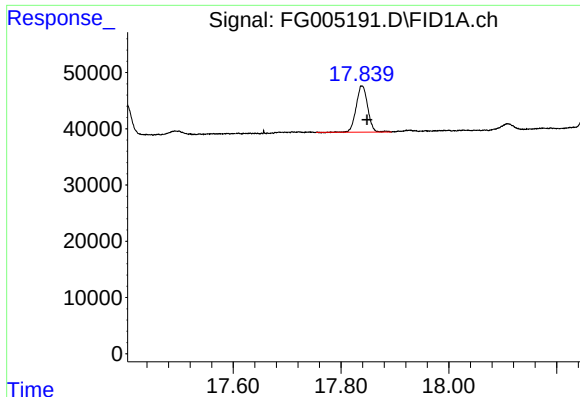


#13 N-TRIACONTANE

R.T.: 17.839 min
Delta R.T.: -0.009 min
Response: 121258
Conc: 0.87 ug/ml

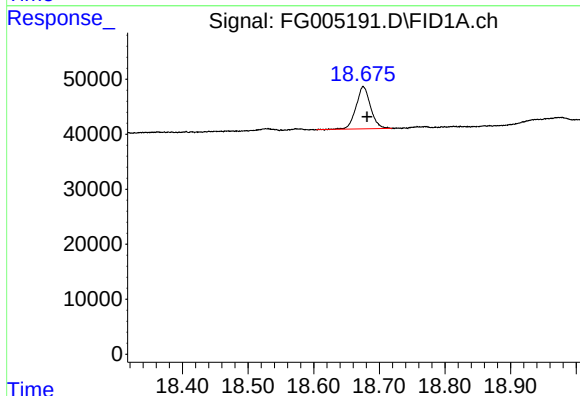


#14 N-DOTRIACONTANE

R.T.: 18.676 min
Delta R.T.: -0.006 min
Response: 117768
Conc: 0.88 ug/ml

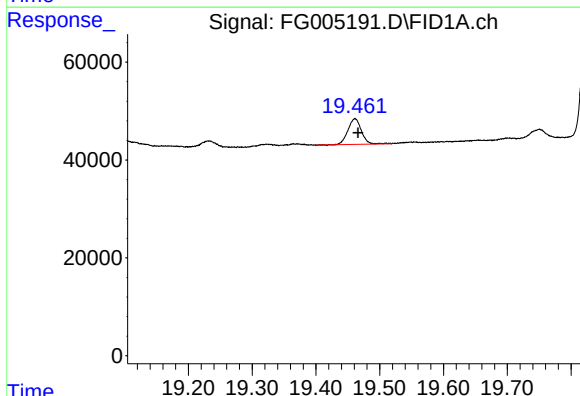

#15 N-TETRATRIACONTANE

R.T.: 19.461 min
Delta R.T.: -0.005 min
Response: 78007
Conc: 0.61 ug/ml

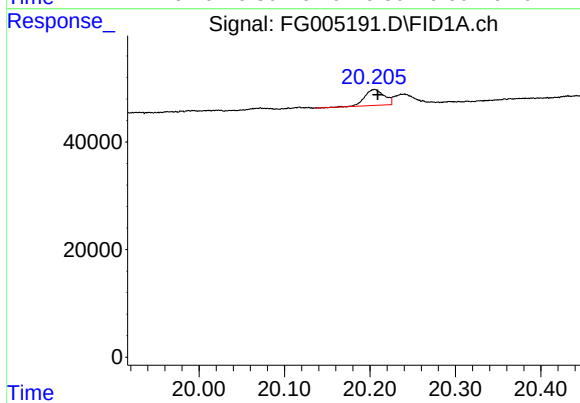

#16 N-HEXATRIACONTANE

R.T.: 20.205 min
Delta R.T.: -0.004 min
Response: 47469
Conc: 0.40 ug/ml