

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062521\
 Data File : FG008427.D
 Signal(s) : FID1A.ch
 Acq On : 25 Jun 2021 21:49
 Operator : DD\AJ
 Sample : M2831-01 20X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 23:34:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062421.M
 Quant Title :
 QLast Update : Thu Jun 24 09:09:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

4)	N-TETRADECANE	8.290	471066	3.189 ug/ml
5)	N-HEXADECANE	9.919	3689640	25.074 ug/ml
6)	N-OCTADECANE	11.342	7492842	49.123 ug/ml
7)	N-EICOSANE	12.674	8028766	52.829 ug/ml
8)	N-DOCOSANE	13.859	986247	6.566 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062521\
Data File : FG008427.D
Signal(s) : FID1A.ch
Acq On : 25 Jun 2021 21:49
Operator : DD\AJ
Sample : M2831-01 20X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 23:34:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062421.M
Quant Title :
QLast Update : Thu Jun 24 09:09:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

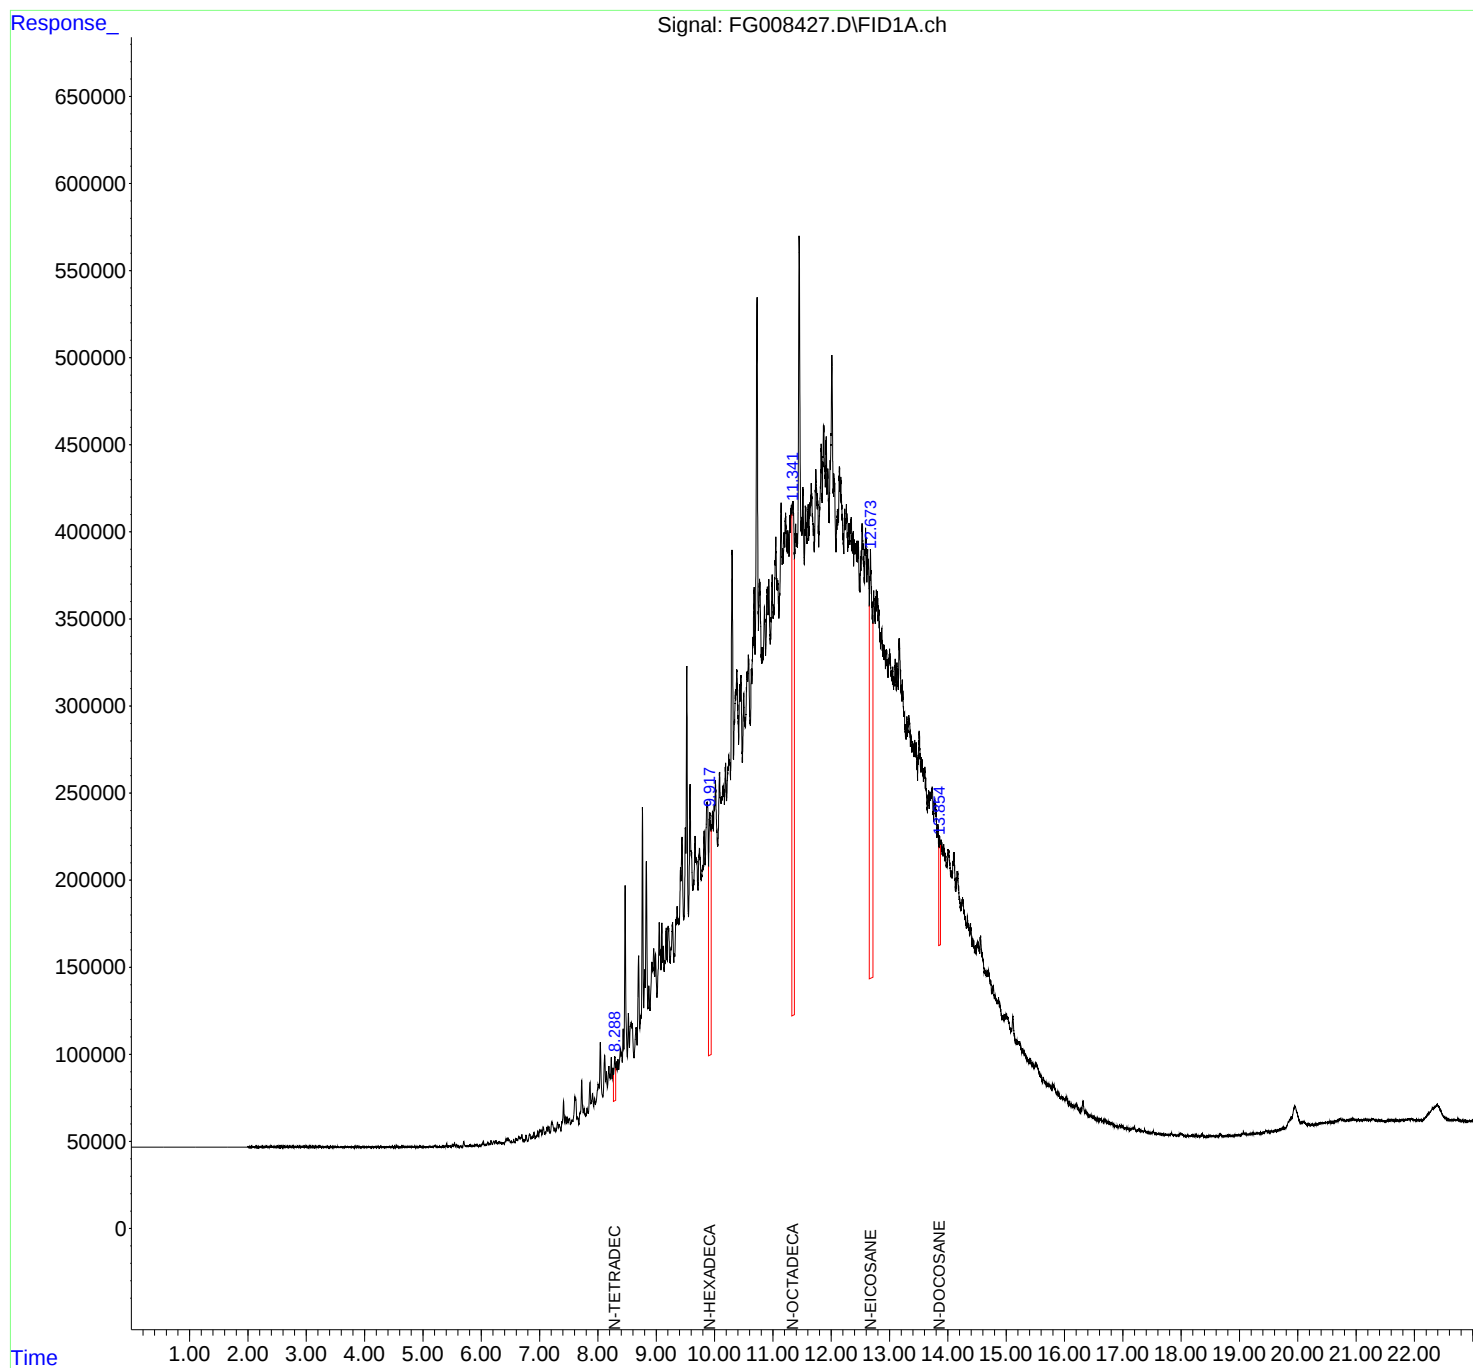


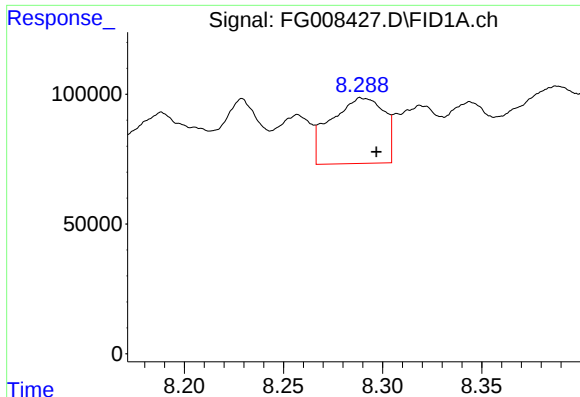

#4 N-TETRADECANE


R.T.: 8.290 min
Delta R.T.: -0.007 min
Response: 471066
Conc: 3.19 ug/ml

Instrument :
FID_G
ClientSampleId :

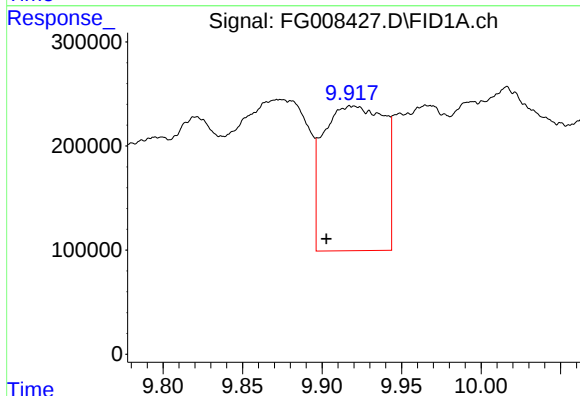


#5 N-HEXADECANE

R.T.: 9.919 min
Delta R.T.: 0.016 min
Response: 3689640
Conc: 25.07 ug/ml

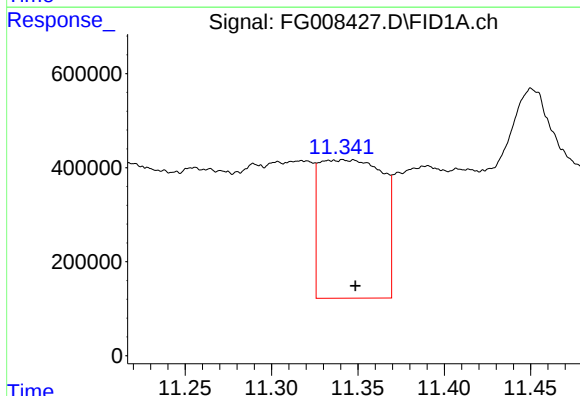


#6 N-OCTADECANE

R.T.: 11.342 min
Delta R.T.: -0.007 min
Response: 7492842
Conc: 49.12 ug/ml

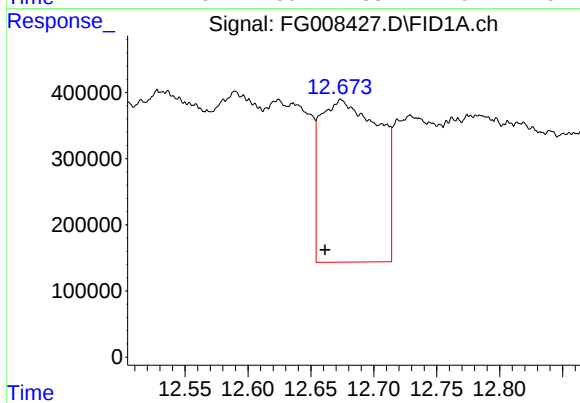

#7 N-EICOSANE


R.T.: 12.674 min
Delta R.T.: 0.013 min
Response: 8028766
Conc: 52.83 ug/ml

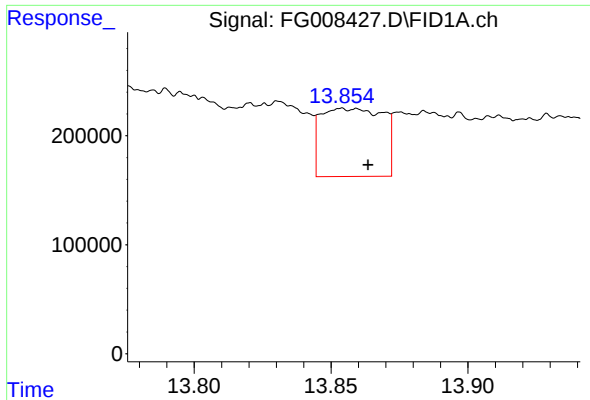

#8 N-DOCOSANE

R.T.: 13.859 min
Delta R.T.: -0.004 min
Response: 986247
Conc: 6.57 ug/ml

Instrument :
FID_G
ClientSampleId :

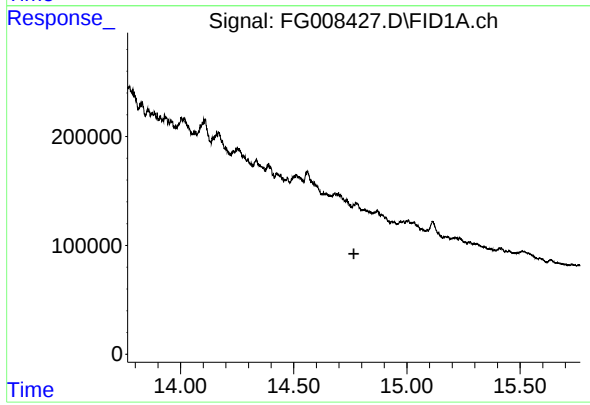

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.766 min
Response: 0
Conc: N.D.