

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062521\
 Data File : FG008428.D
 Signal(s) : FID1A.ch
 Acq On : 25 Jun 2021 23:22
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 25 23:36:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062421.M
 Quant Title :
 QLast Update : Thu Jun 24 09:09:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.766	2360887	18.045 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.683	312138	2.332 ug/ml
16) N-HEXATRIACONTANE	20.238	788307	7.135 ug/ml
18) N-TETRACONTANE	21.953f	1175542	12.317 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062521\
Data File : FG008428.D
Signal(s) : FID1A.ch
Acq On : 25 Jun 2021 23:22
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 25 23:36:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062421.M
Quant Title :
QLast Update : Thu Jun 24 09:09:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

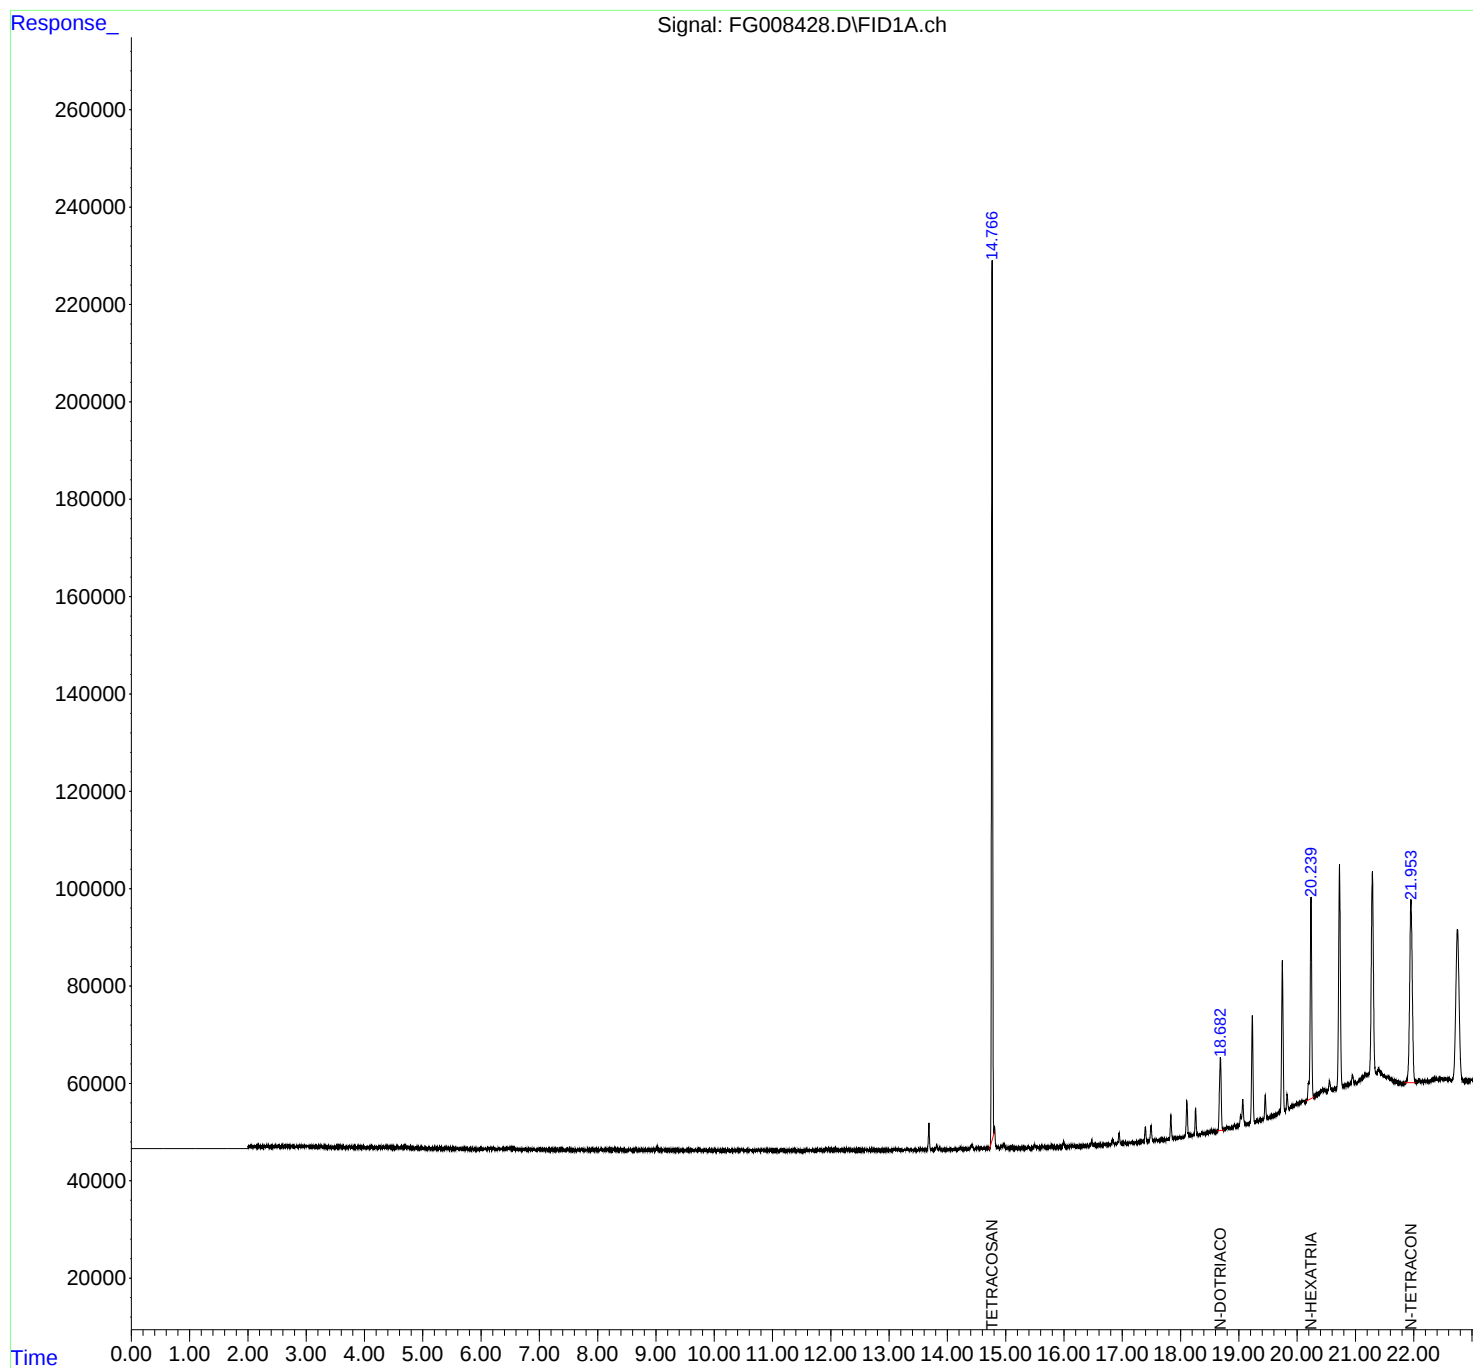


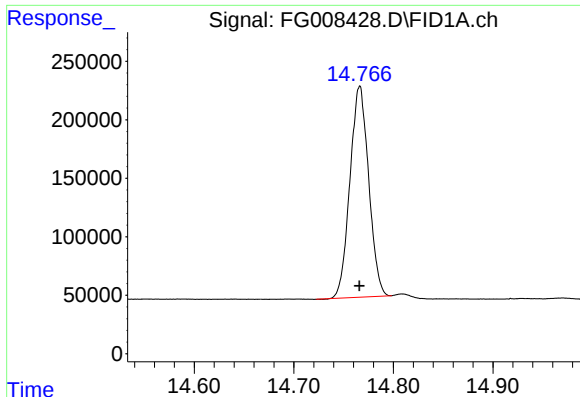

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.766 min
Delta R.T.: 0.000 min
Response: 2360887
Conc: 18.04 ug/ml

Instrument :
FID_G
ClientSampleId :

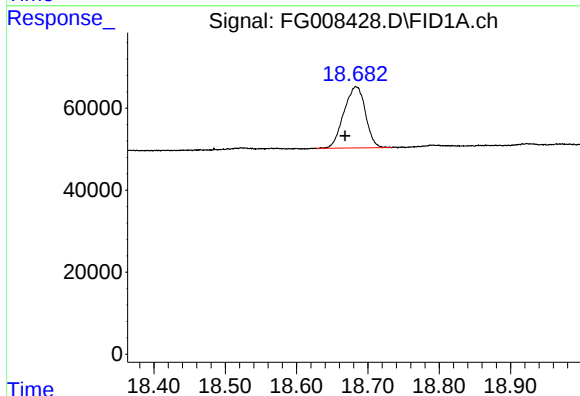


#14 N-DOTRIACONTANE

R.T.: 18.683 min
Delta R.T.: 0.015 min
Response: 312138
Conc: 2.33 ug/ml

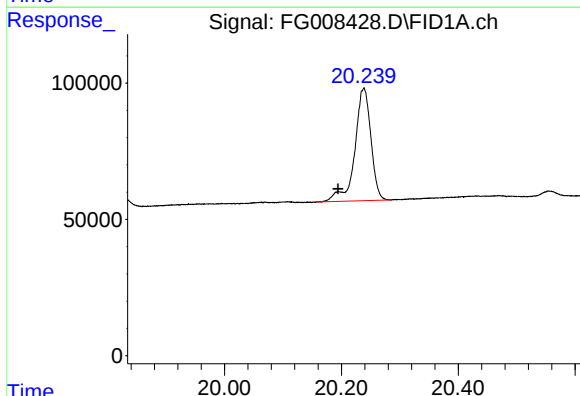

#16 N-HEXATRIACONTANE

R.T.: 20.238 min
Delta R.T.: 0.044 min
Response: 788307
Conc: 7.14 ug/ml

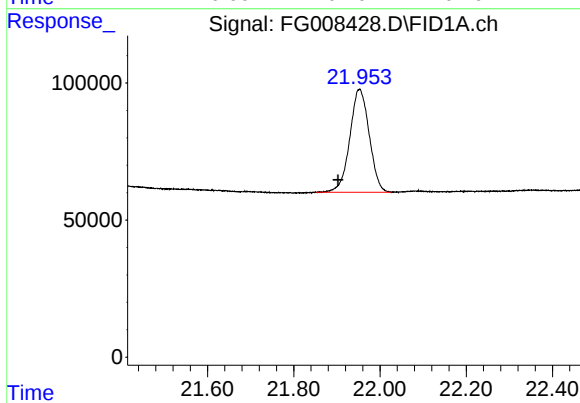

#18 N-TETRACONTANE

R.T.: 21.953 min
Delta R.T.: 0.050 min
Response: 1175542
Conc: 12.32 ug/ml