

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062521\
Data File : FG008421.D
Signal(s) : FID1A.ch
Acq On : 25 Jun 2021 17:40
Operator : DD\AJ
Sample : M2829-06 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
15B-DUP-01

Integration File: autoint1.e
Quant Time: Jun 25 23:33:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062421.M
Quant Title :
QLast Update : Thu Jun 24 09:09:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.768	431646	3.299 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062521\
Data File : FG008421.D
Signal(s) : FID1A.ch
Acq On : 25 Jun 2021 17:40
Operator : DD\AJ
Sample : M2829-06 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
15B-DUP-01

Integration File: autoint1.e
Quant Time: Jun 25 23:33:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062421.M
Quant Title :
QLast Update : Thu Jun 24 09:09:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

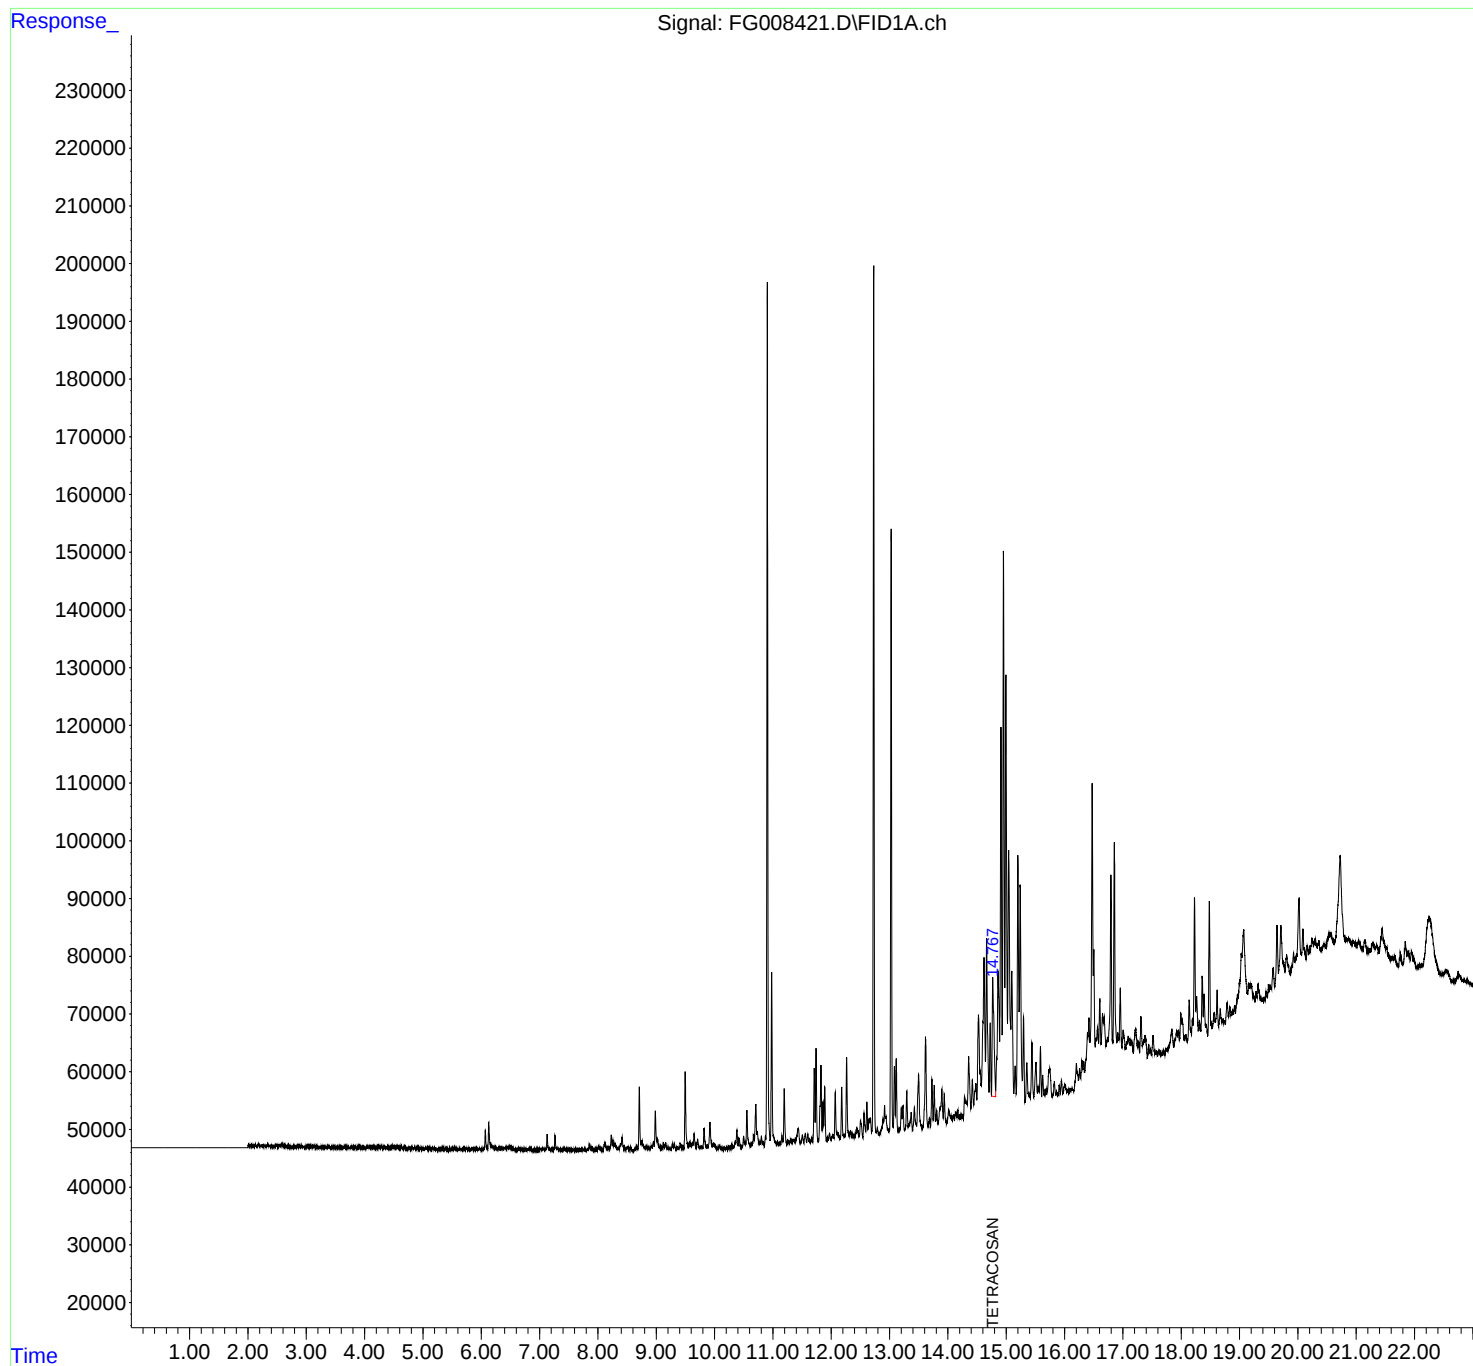

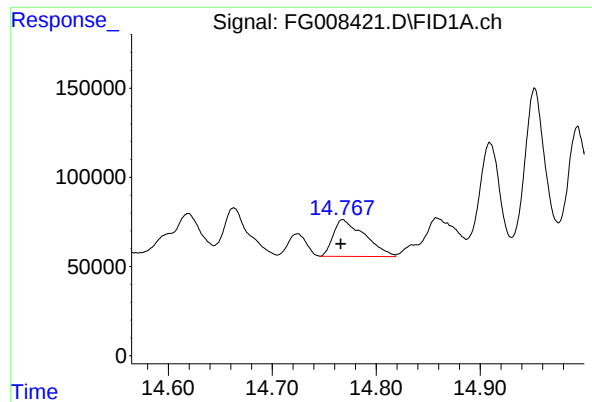

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.768 min
Delta R.T.: 0.002 min
Response: 431646
Conc: 3.30 ug/ml

Instrument :
FID_G
ClientSampleId :
15B-DUP-01