

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062718\
Data File : FG001491.D
Signal(s) : FID1A.ch
Acq On : 27 Jun 2018 18:45
Operator : UA\AJ
Sample : J3048-05 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:38:16 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.531	378161	3.093 ug/ml
Target Compounds			
7) N-EICOSANE	12.482	2482838	17.632 ug/ml
8) N-DOCOSANE	13.645	408761	2.917 ug/ml
10) N-TETRACOSANE	14.701	1468129	10.558 ug/ml
12) N-OCTACOSANE	16.704	443273	3.213 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062718\
Data File : FG001491.D
Signal(s) : FID1A.ch
Acq On : 27 Jun 2018 18:45
Operator : UA\AJ
Sample : J3048-05 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:38:16 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

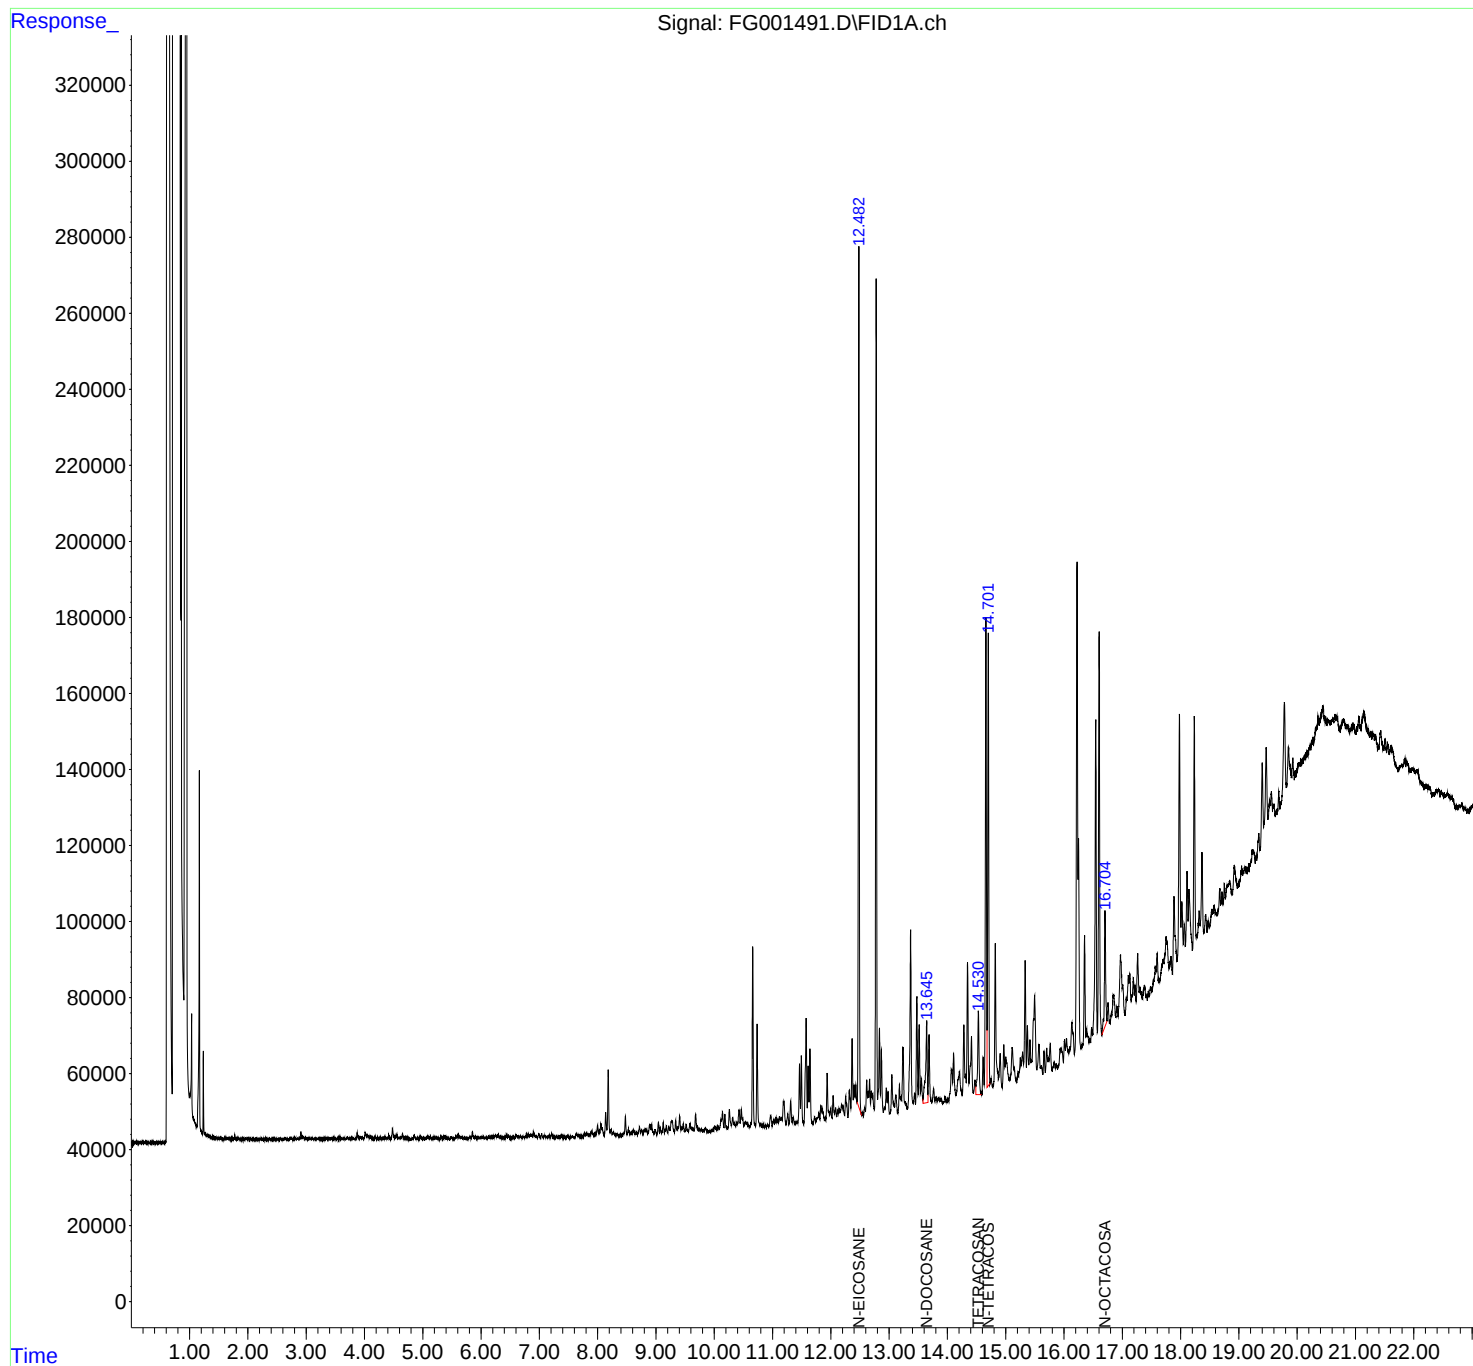


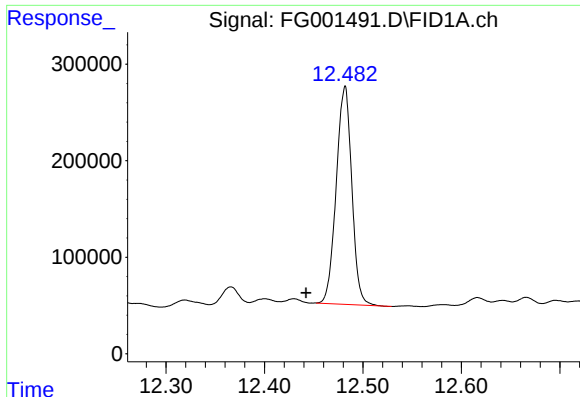

#7 N-EICOSANE


R.T.: 12.482 min
Delta R.T.: 0.039 min
Response: 2482838
Conc: 17.63 ug/ml

Instrument :
FID_G
ClientSampleId :

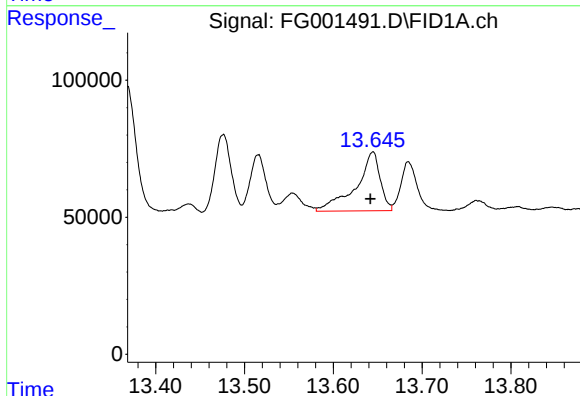


#8 N-DOCOSANE

R.T.: 13.645 min
Delta R.T.: 0.003 min
Response: 408761
Conc: 2.92 ug/ml

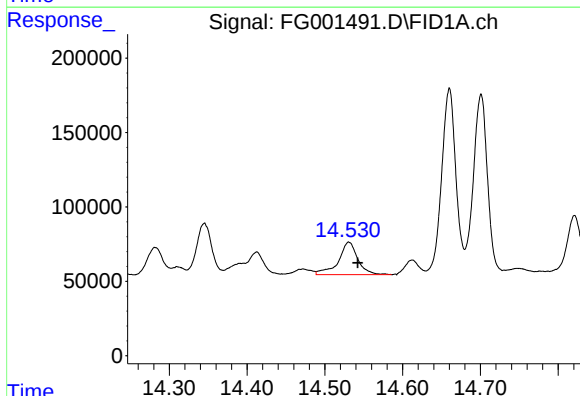


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.531 min
Delta R.T.: -0.011 min
Response: 378161
Conc: 3.09 ug/ml

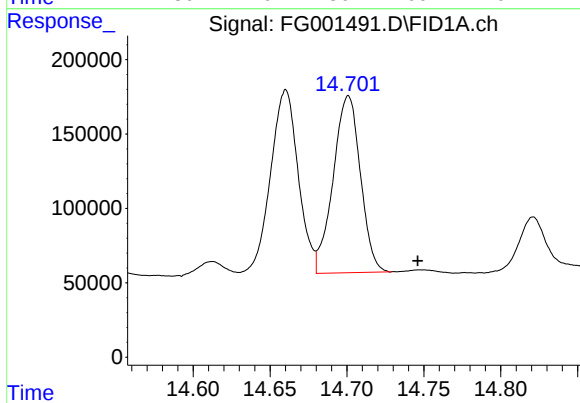

#10 N-TETRACOSANE

R.T.: 14.701 min
Delta R.T.: -0.045 min
Response: 1468129
Conc: 10.56 ug/ml

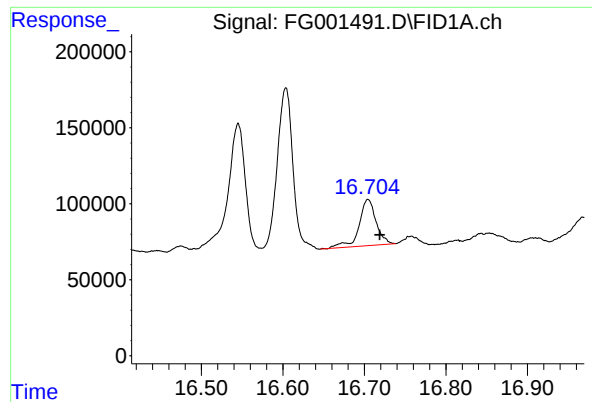

#12 N-OCTACOSANE

R.T.: 16.704 min
Delta R.T.: -0.014 min
Response: 443273
Conc: 3.21 ug/ml

Instrument :
FID_G
ClientSampleId :