

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062718\
 Data File : FG001492.D
 Signal(s) : FID1A.ch
 Acq On : 27 Jun 2018 19:15
 Operator : UA\AJ
 Sample : J3242-07 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 28 01:38:29 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.532	211772	1.732 ug/ml
Target Compounds			
4) N-TETRADECANE	8.081	625874	4.479 ug/ml
5) N-HEXADECANE	9.682	834724	5.932 ug/ml
6) N-OCTADECANE	11.122	704720	4.971 ug/ml
7) N-EICOSANE	12.435	501963	3.565 ug/ml
8) N-DOCOSANE	13.636	133743	0.954 ug/ml
10) N-TETRACOSANE	14.729	648077	4.661 ug/ml
13) N-TRIACONTANE	17.597	250269	1.824 ug/ml
16) N-HEXATRIACONTANE	19.969	186768	1.486 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062718\
Data File : FG001492.D
Signal(s) : FID1A.ch
Acq On : 27 Jun 2018 19:15
Operator : UA\AJ
Sample : J3242-07 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:38:29 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

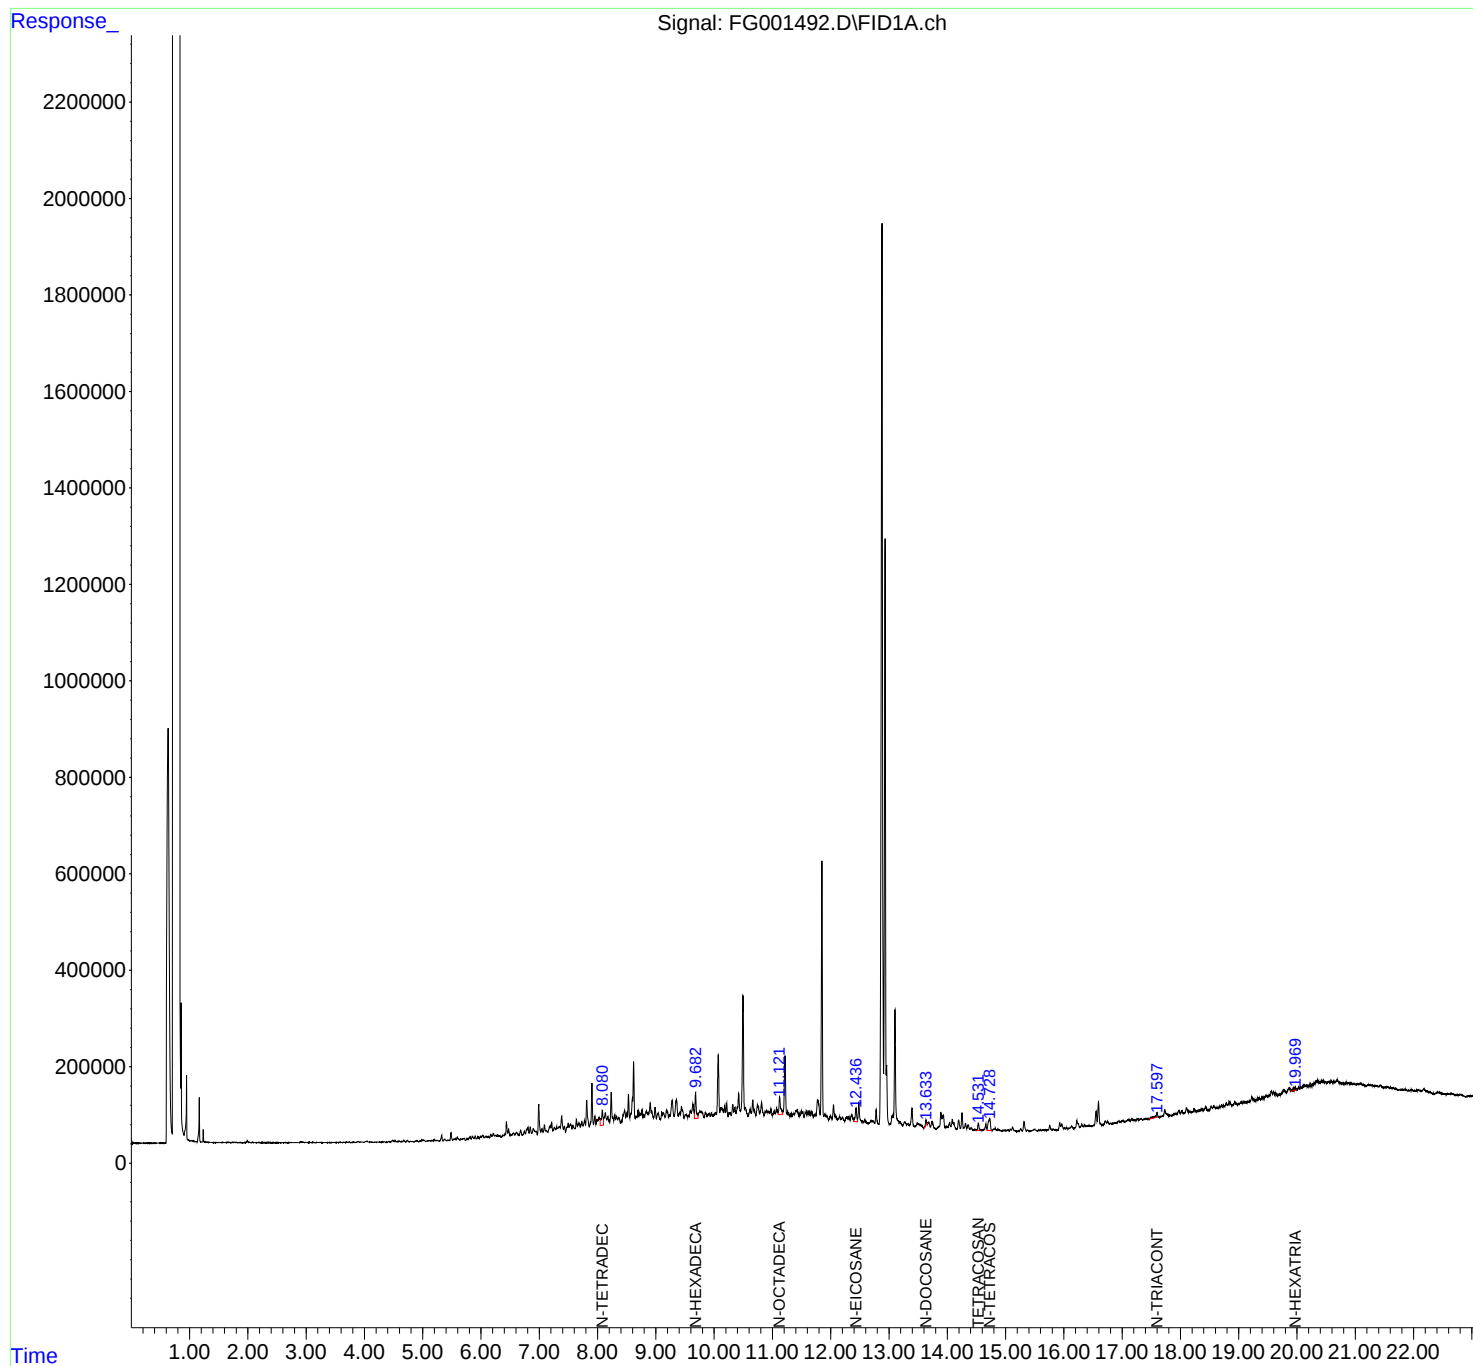


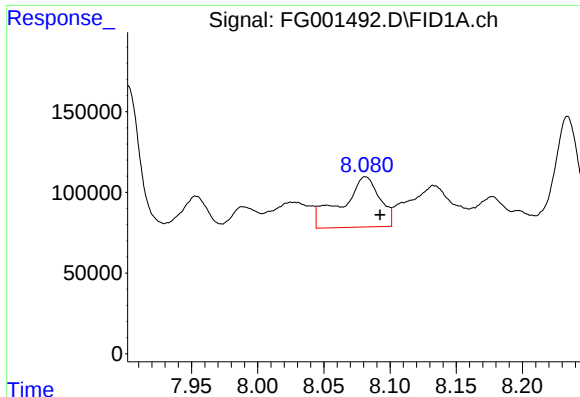

#4 N-TETRADECANE


R.T.: 8.081 min
Delta R.T.: -0.011 min
Response: 625874
Conc: 4.48 ug/ml

Instrument :
FID_G
ClientSampleId :

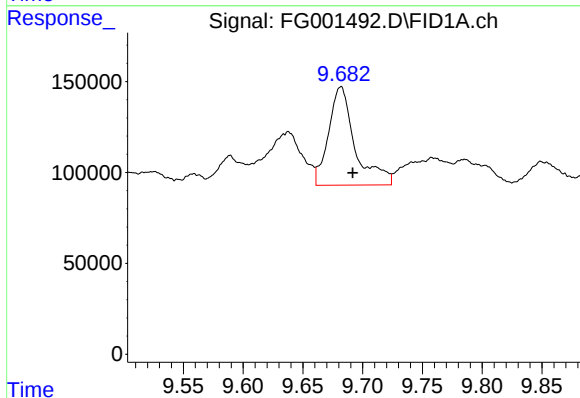


#5 N-HEXADECANE

R.T.: 9.682 min
Delta R.T.: -0.010 min
Response: 834724
Conc: 5.93 ug/ml

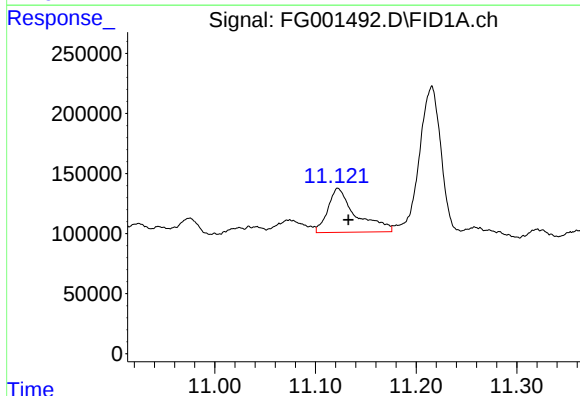


#6 N-OCTADECANE

R.T.: 11.122 min
Delta R.T.: -0.010 min
Response: 704720
Conc: 4.97 ug/ml

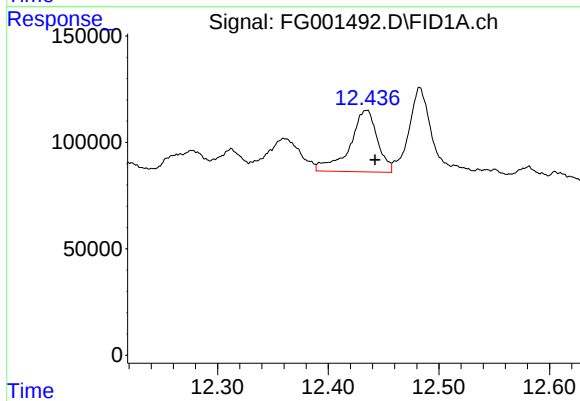

#7 N-EICOSANE


R.T.: 12.435 min
Delta R.T.: -0.008 min
Response: 501963
Conc: 3.56 ug/ml

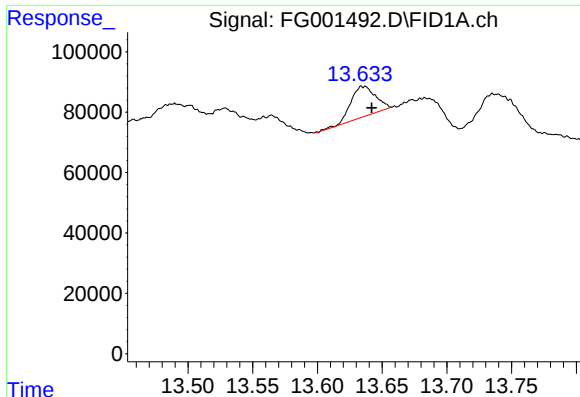

#8 N-DOCOSANE


R.T.: 13.636 min
Delta R.T.: -0.006 min
Response: 133743
Conc: 0.95 ug/ml

Instrument :
FID_G
ClientSampleId :

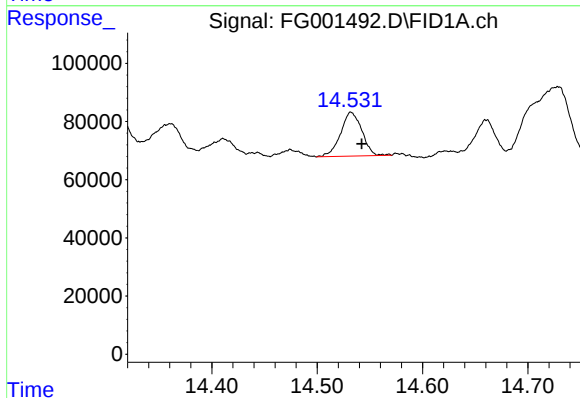


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.532 min
Delta R.T.: -0.010 min
Response: 211772
Conc: 1.73 ug/ml

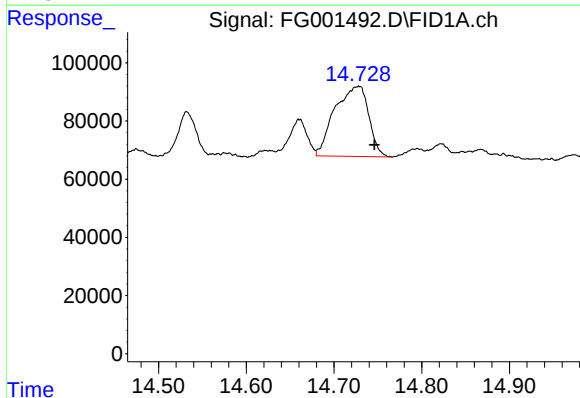


#10 N-TETRACOSANE

R.T.: 14.729 min
Delta R.T.: -0.018 min
Response: 648077
Conc: 4.66 ug/ml

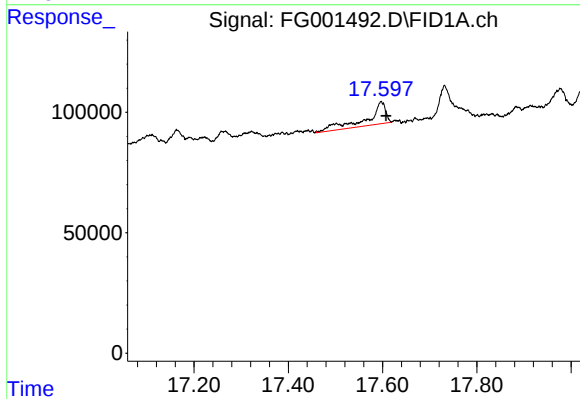

#13 N-TRIACONTANE

R.T.: 17.597 min
Delta R.T.: -0.011 min
Response: 250269
Conc: 1.82 ug/ml

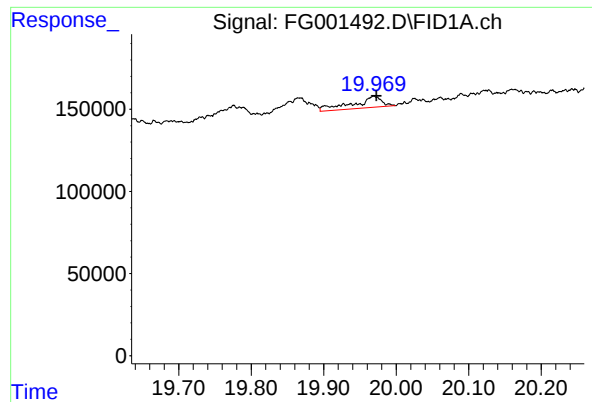

#16 N-HEXATRIACONTANE

R.T.: 19.969 min
Delta R.T.: -0.003 min
Response: 186768
Conc: 1.49 ug/ml

Instrument :
FID_G
ClientSampleId :