

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062718\
 Data File : FG001493.D
 Signal(s) : FID1A.ch
 Acq On : 27 Jun 2018 19:44
 Operator : UA\AJ
 Sample : J3242-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 28 01:38:45 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.532	157370	1.287 ug/ml
Target Compounds			
3) N-DODECANE	6.288	203691	1.469 ug/ml
4) N-TETRADECANE	8.081	390129	2.792 ug/ml
5) N-HEXADECANE	9.681	490141	3.483 ug/ml
6) N-OCTADECANE	11.123	369650	2.608 ug/ml
7) N-EICOSANE	12.432	375272	2.665 ug/ml
8) N-DOCOSANE	13.634	125508	0.896 ug/ml
10) N-TETRACOSANE	14.727	445645	3.205 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062718\
Data File : FG001493.D
Signal(s) : FID1A.ch
Acq On : 27 Jun 2018 19:44
Operator : UA\AJ
Sample : J3242-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:38:45 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

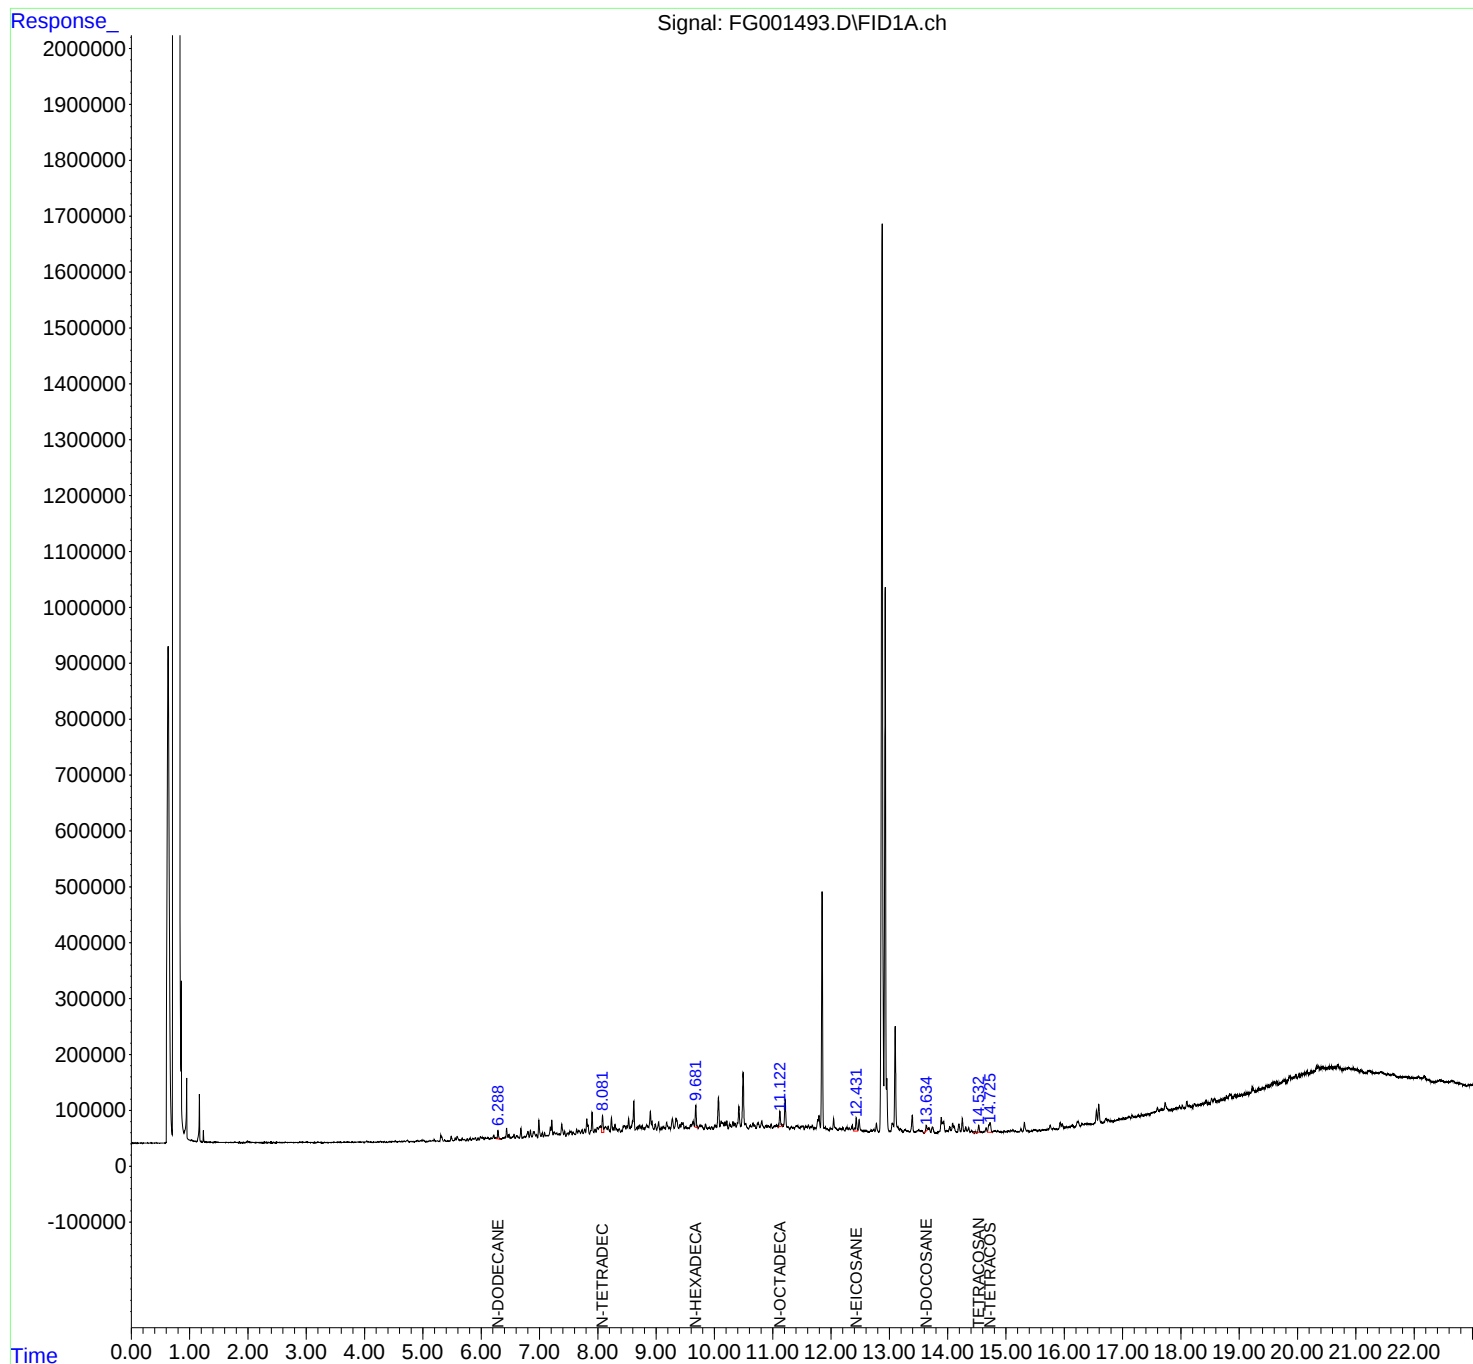


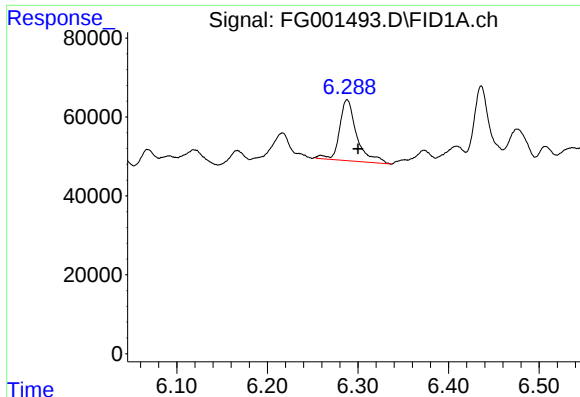

#3 N-DODECANE


R.T.: 6.288 min
Delta R.T.: -0.012 min
Response: 203691
Conc: 1.47 ug/ml

Instrument :
FID_G
ClientSampleId :

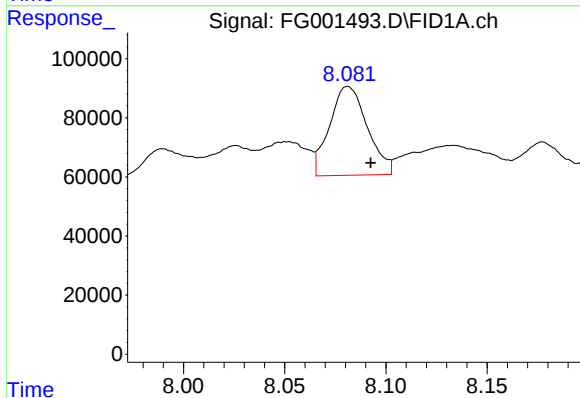


#4 N-TETRADECANE

R.T.: 8.081 min
Delta R.T.: -0.011 min
Response: 390129
Conc: 2.79 ug/ml

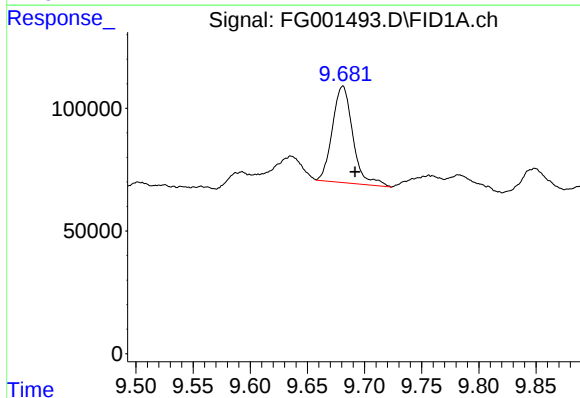


#5 N-HEXADECANE

R.T.: 9.681 min
Delta R.T.: -0.011 min
Response: 490141
Conc: 3.48 ug/ml

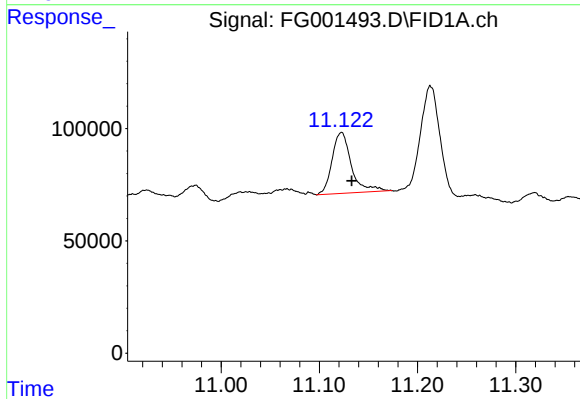

#6 N-OCTADECANE


R.T.: 11.123 min
Delta R.T.: -0.010 min
Response: 369650
Conc: 2.61 ug/ml

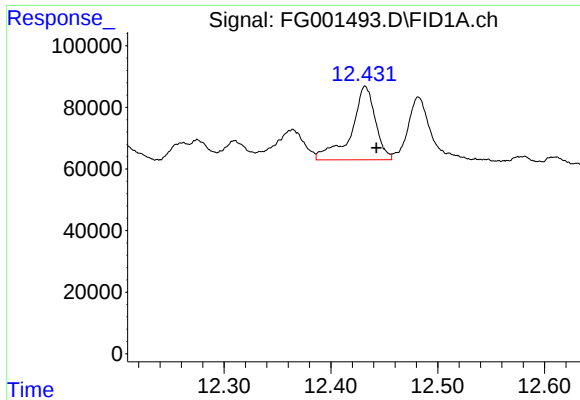

#7 N-EICOSANE


R.T.: 12.432 min
Delta R.T.: -0.010 min
Response: 375272
Conc: 2.66 ug/ml

Instrument :
FID_G
ClientSampleId :

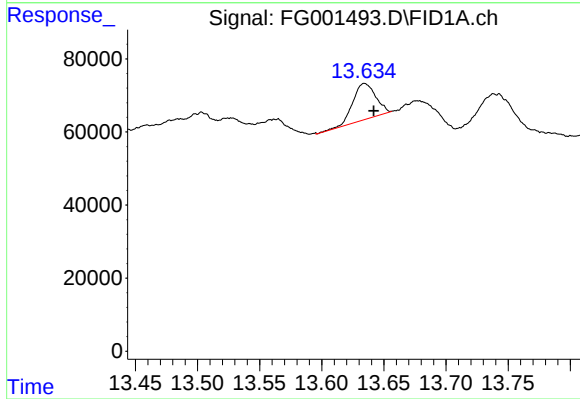


#8 N-DOCOSANE

R.T.: 13.634 min
Delta R.T.: -0.007 min
Response: 125508
Conc: 0.90 ug/ml

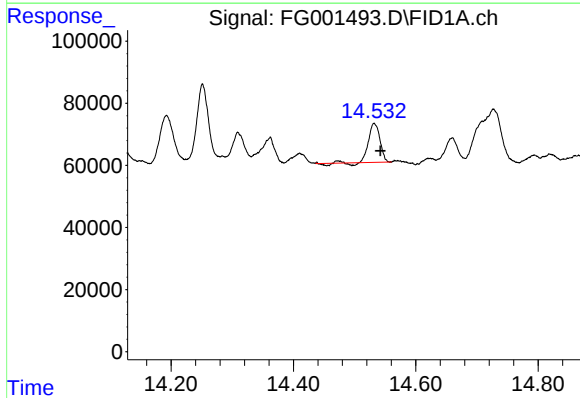

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.532 min
Delta R.T.: -0.010 min
Response: 157370
Conc: 1.29 ug/ml

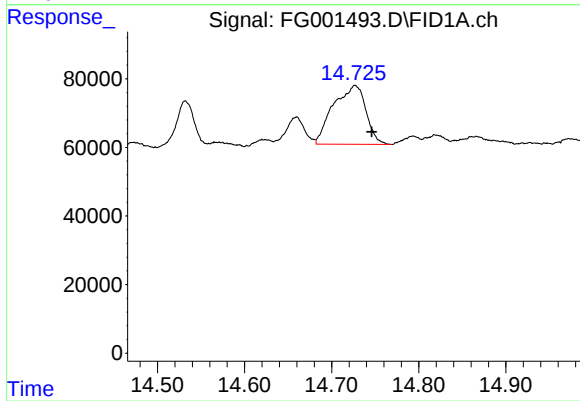

#10 N-TETRACOSANE

R.T.: 14.727 min
Delta R.T.: -0.019 min
Response: 445645
Conc: 3.20 ug/ml