

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062718\
 Data File : FG001494.D
 Signal(s) : FID1A.ch
 Acq On : 27 Jun 2018 20:14
 Operator : UA\AJ
 Sample : J3242-03 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 28 01:38:59 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.533	186745	1.528 ug/ml
Target Compounds			
4) N-TETRADECANE	8.082	439633	3.146 ug/ml
5) N-HEXADECANE	9.682	486745	3.459 ug/ml
6) N-OCTADECANE	11.123	671126	4.735 ug/ml
7) N-EICOSANE	12.434	375897	2.669 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062718\
Data File : FG001494.D
Signal(s) : FID1A.ch
Acq On : 27 Jun 2018 20:14
Operator : UA\AJ
Sample : J3242-03 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:38:59 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

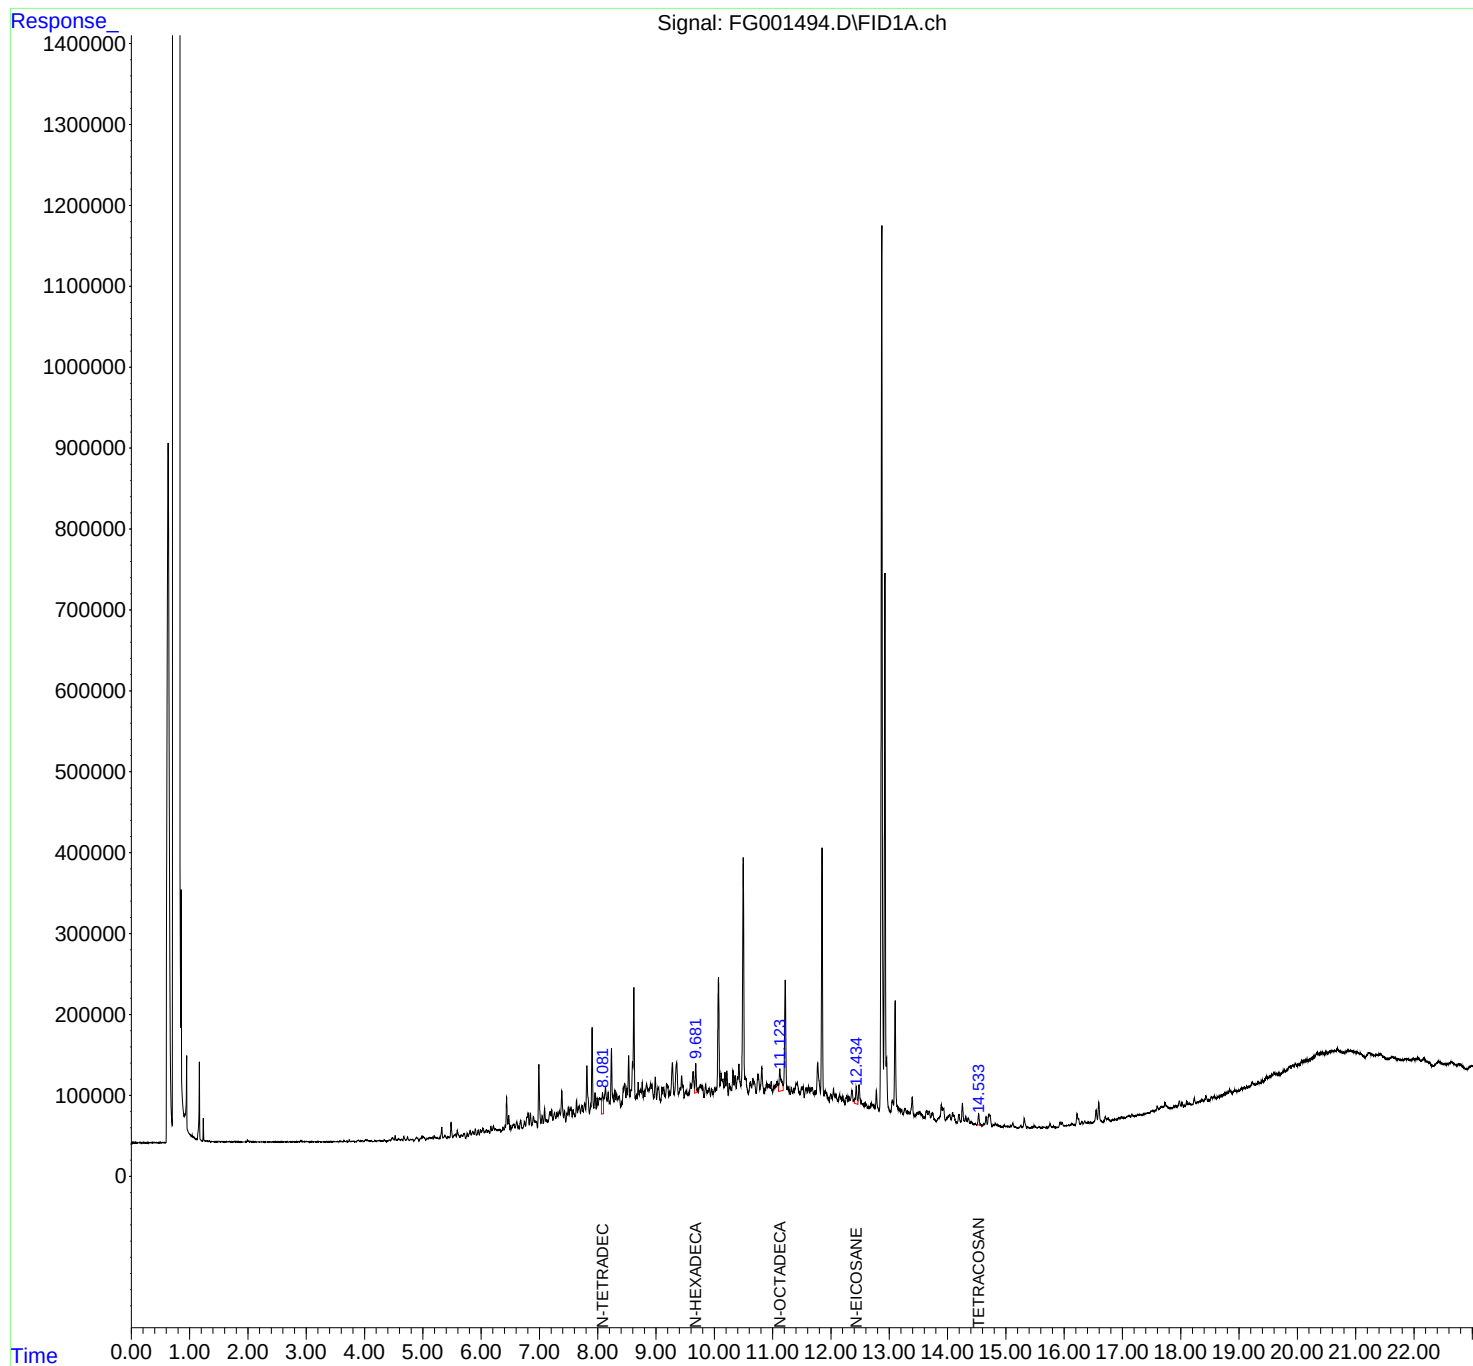


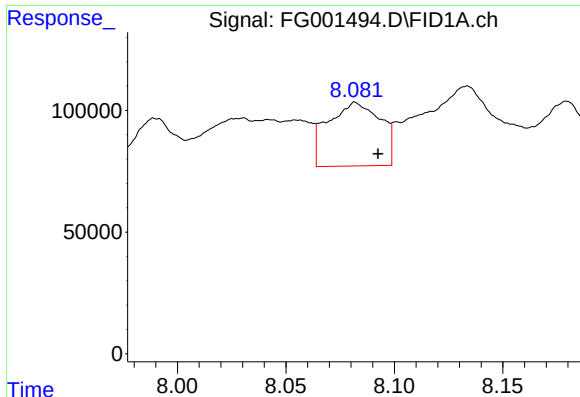

#4 N-TETRADECANE


R.T.: 8.082 min
Delta R.T.: -0.010 min
Response: 439633
Conc: 3.15 ug/ml

Instrument :
FID_G
ClientSampleId :

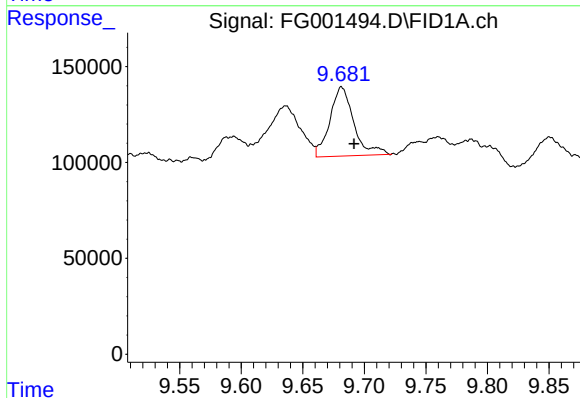


#5 N-HEXADECANE

R.T.: 9.682 min
Delta R.T.: -0.010 min
Response: 486745
Conc: 3.46 ug/ml

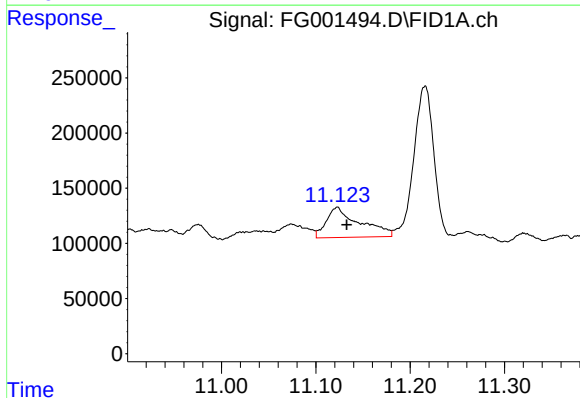


#6 N-OCTADECANE

R.T.: 11.123 min
Delta R.T.: -0.010 min
Response: 671126
Conc: 4.73 ug/ml

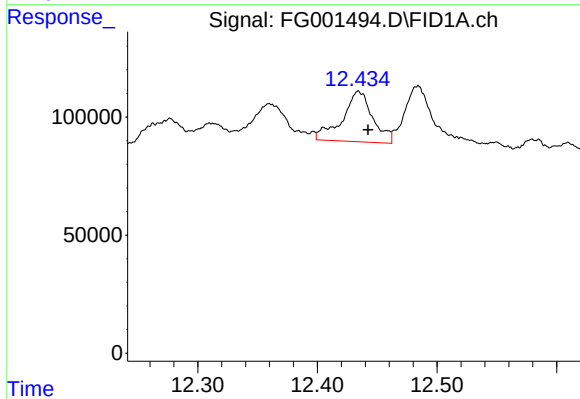

#7 N-EICOSANE

R.T.: 12.434 min
Delta R.T.: -0.008 min
Response: 375897
Conc: 2.67 ug/ml

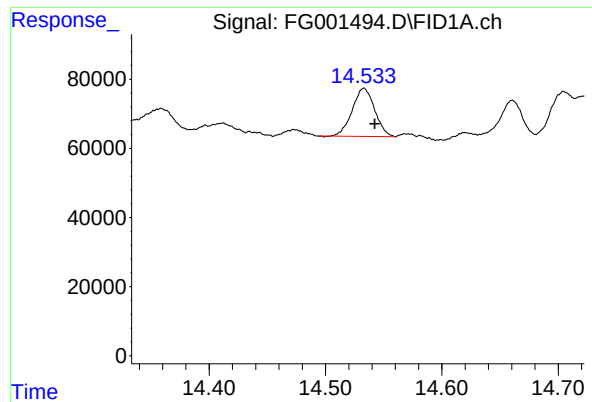

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.533 min
Delta R.T.: -0.009 min
Response: 186745
Conc: 1.53 ug/ml

Instrument :
FID_G
ClientSampleId :