

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062718\
 Data File : FG001495.D
 Signal(s) : FID1A.ch
 Acq On : 27 Jun 2018 20:44
 Operator : UA\AJ
 Sample : J3242-05 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 28 01:39:11 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.532	200568	1.641 ug/ml
Target Compounds			
4) N-TETRADECANE	8.082	984199	7.043 ug/ml
5) N-HEXADECANE	9.681	737155	5.238 ug/ml
6) N-OCTADECANE	11.122	580233	4.093 ug/ml
7) N-EICOSANE	12.433	387229	2.750 ug/ml
10) N-TETRACOSANE	14.703	102942	0.740 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062718\
Data File : FG001495.D
Signal(s) : FID1A.ch
Acq On : 27 Jun 2018 20:44
Operator : UA\AJ
Sample : J3242-05 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:39:11 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

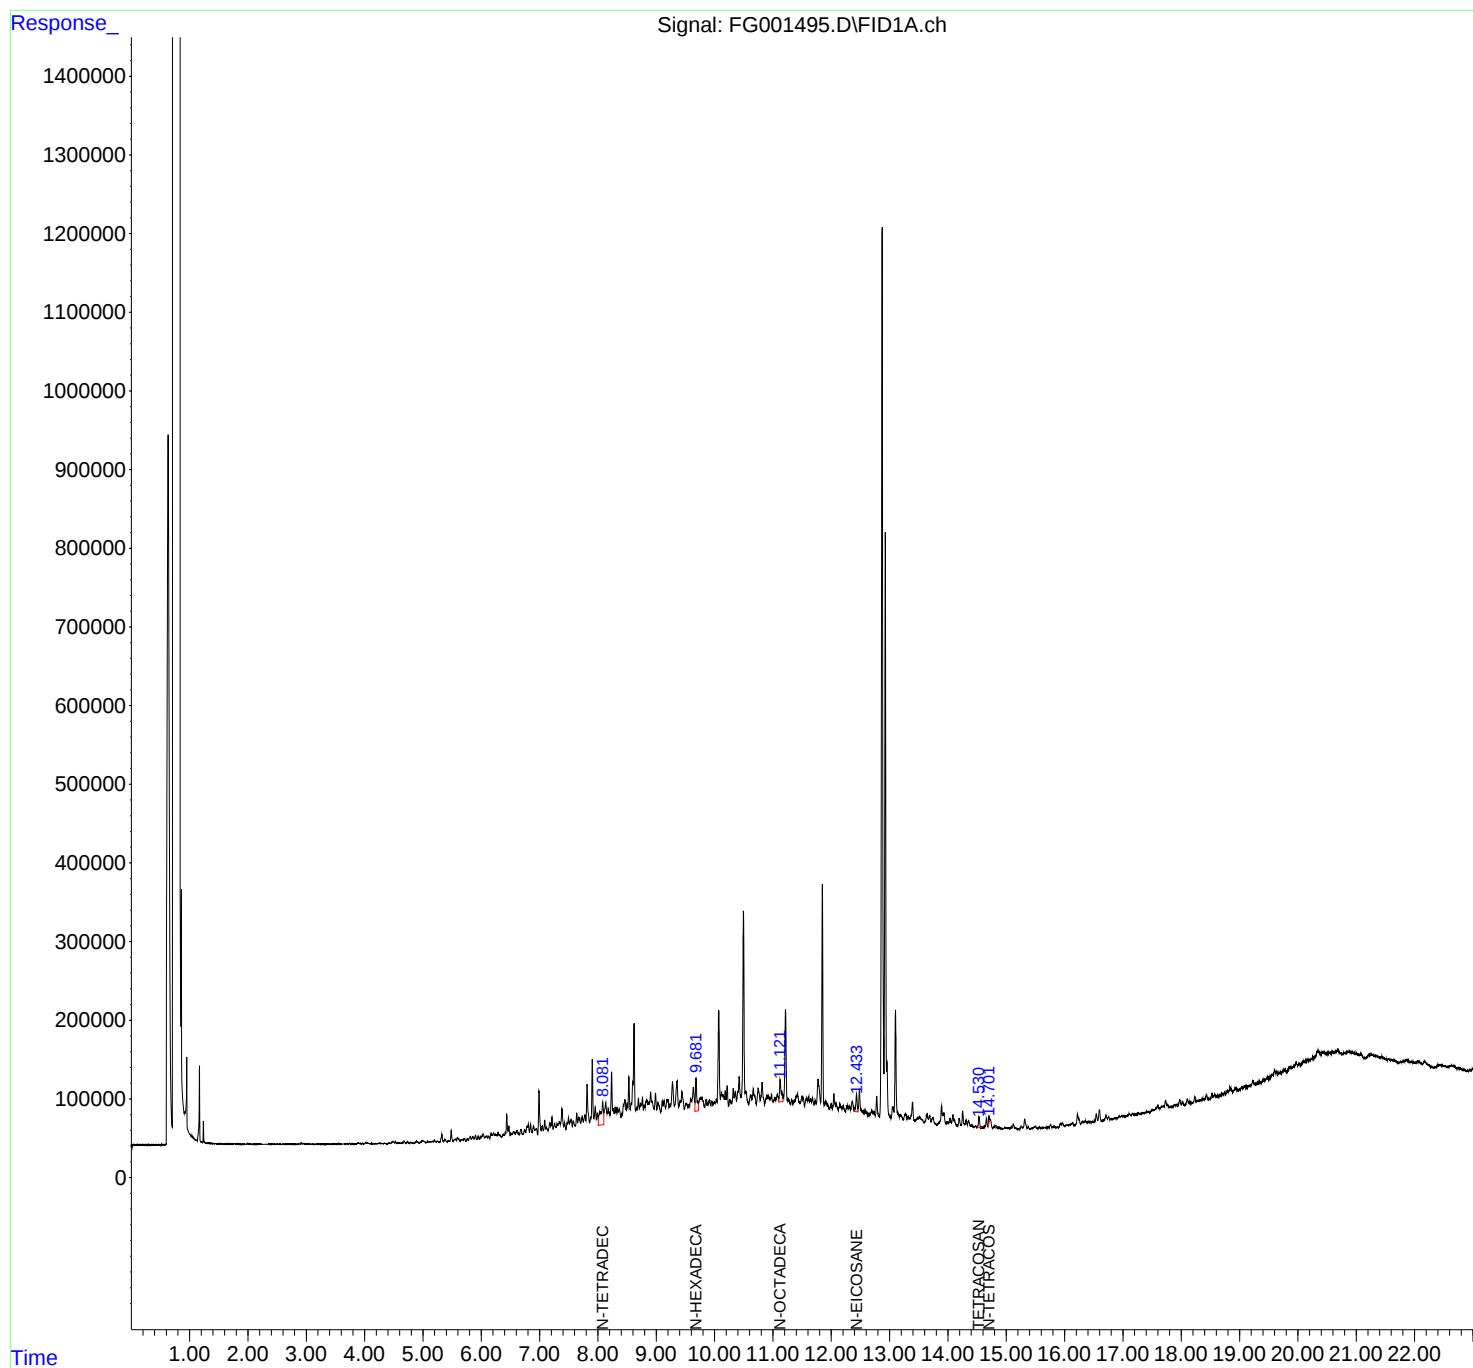


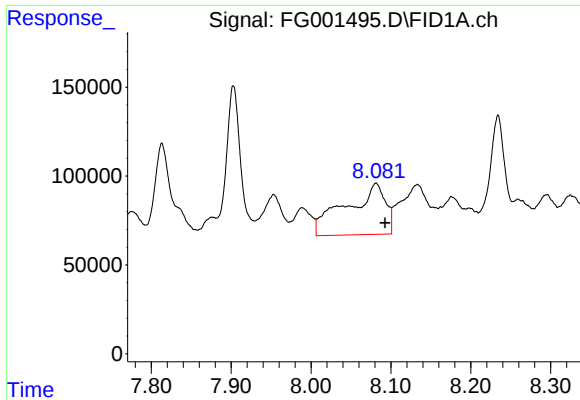

#4 N-TETRADECANE


R.T.: 8.082 min
Delta R.T.: -0.011 min
Response: 984199
Conc: 7.04 ug/ml

Instrument :
FID_G
ClientSampleId :

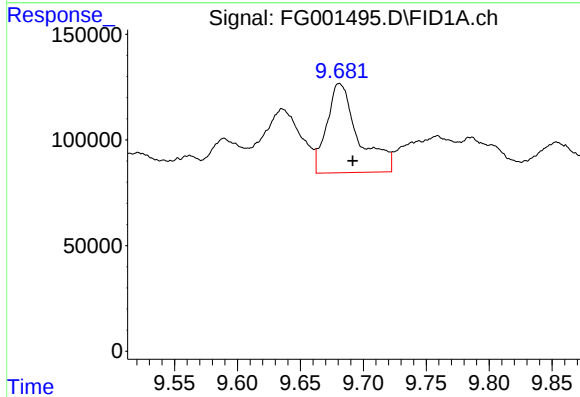


#5 N-HEXADECANE

R.T.: 9.681 min
Delta R.T.: -0.011 min
Response: 737155
Conc: 5.24 ug/ml

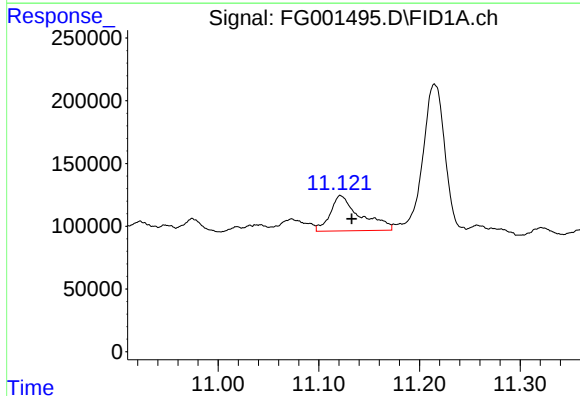


#6 N-OCTADECANE

R.T.: 11.122 min
Delta R.T.: -0.011 min
Response: 580233
Conc: 4.09 ug/ml

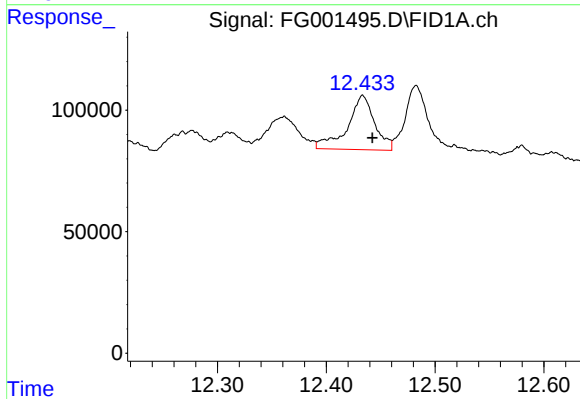

#7 N-EICOSANE


R.T.: 12.433 min
Delta R.T.: -0.009 min
Response: 387229
Conc: 2.75 ug/ml

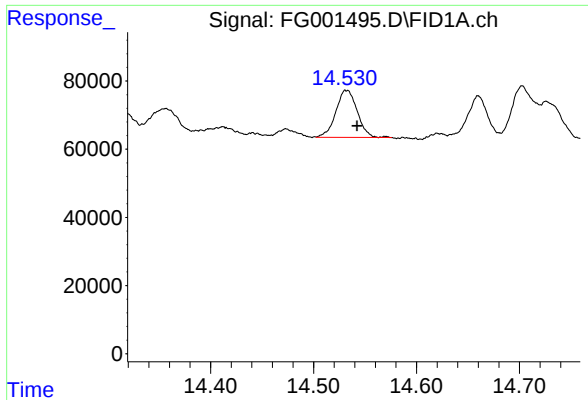

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.532 min
Delta R.T.: -0.010 min
Response: 200568
Conc: 1.64 ug/ml

Instrument :
FID_G
ClientSampleId :

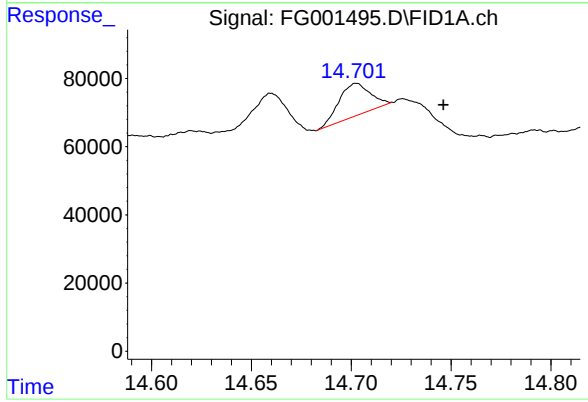

#10 N-TETRACOSANE

R.T.: 14.703 min
Delta R.T.: -0.043 min
Response: 102942
Conc: 0.74 ug/ml