

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062718\
 Data File : FG001498.D
 Signal(s) : FID1A.ch
 Acq On : 27 Jun 2018 22:14
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 28 01:39:44 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.536	5930569	48.512 ug/ml
Target Compounds			
2) N-DECANE	4.273	6783365	49.487 ug/ml
3) N-DODECANE	6.290	6877875	49.614 ug/ml
4) N-TETRADECANE	8.083	6924831	49.557 ug/ml
5) N-HEXADECANE	9.683	6962821	49.478 ug/ml
6) N-OCTADECANE	11.125	6975953	49.212 ug/ml
7) N-EICOSANE	12.435	6888648	48.919 ug/ml
8) N-DOCOSANE	13.635	6789525	48.446 ug/ml
10) N-TETRACOSANE	14.740	6692804	48.133 ug/ml
11) N-HEXACOSANE	15.762	5321956	38.418 ug/mlm
12) N-OCTACOSANE	16.712	6491305	47.046 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062718\
Data File : FG001498.D
Signal(s) : FID1A.ch
Acq On : 27 Jun 2018 22:14
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:39:44 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

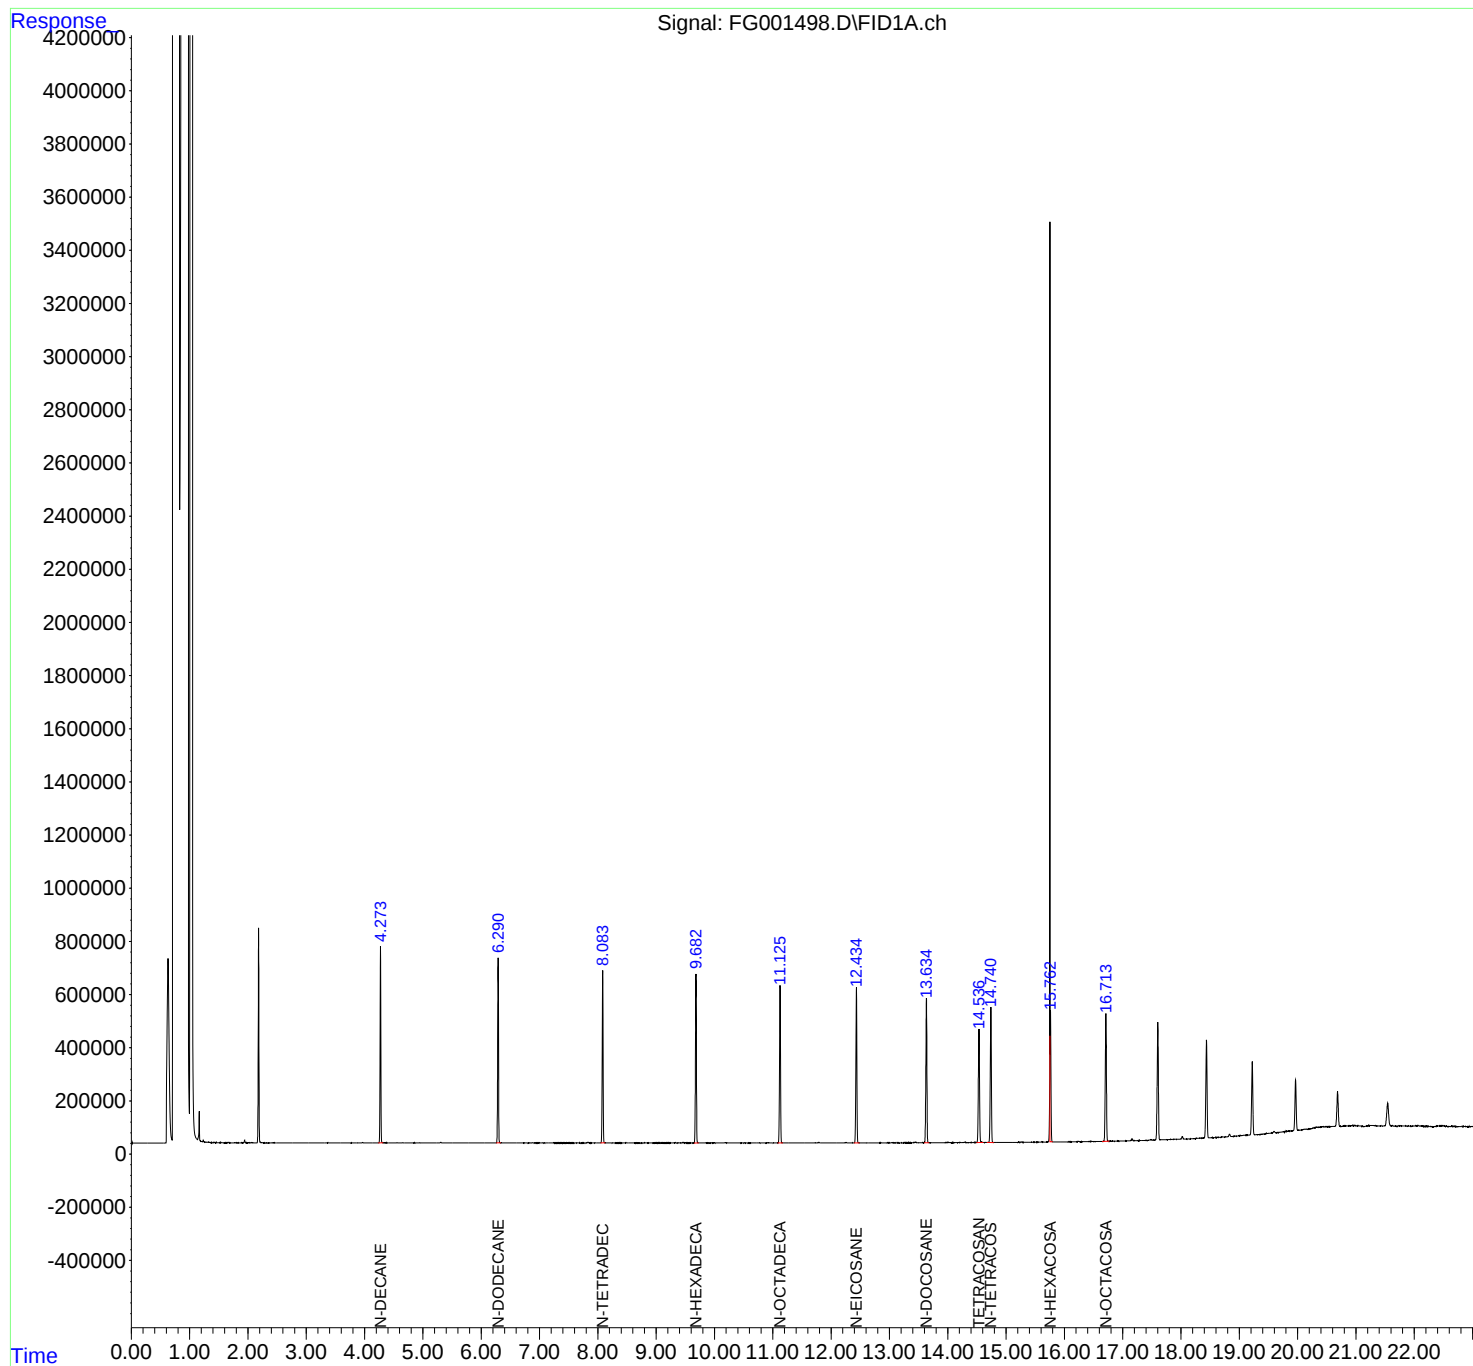


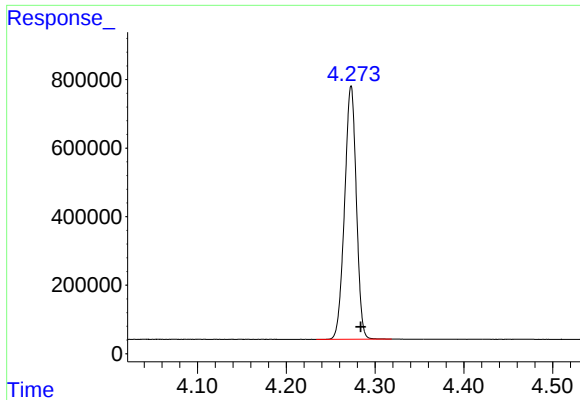

#2 N-DECANE


R.T.: 4.273 min
Delta R.T.: -0.011 min
Response: 6783365
Conc: 49.49 ug/ml

Instrument :
FID_G
ClientSampleId :

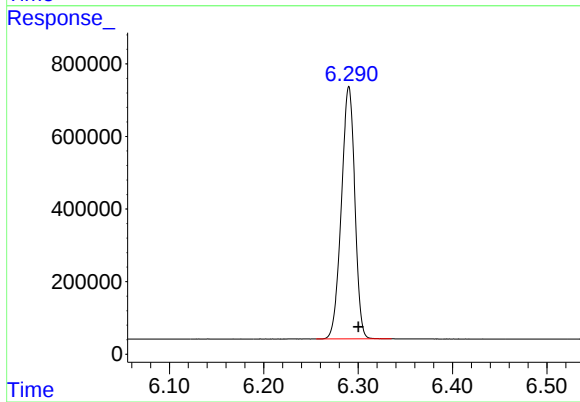


#3 N-DODECANE

R.T.: 6.290 min
Delta R.T.: -0.010 min
Response: 6877875
Conc: 49.61 ug/ml

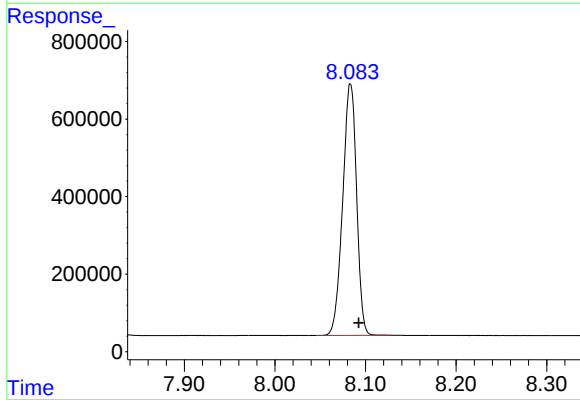


#4 N-TETRADECANE

R.T.: 8.083 min
Delta R.T.: -0.009 min
Response: 6924831
Conc: 49.56 ug/ml

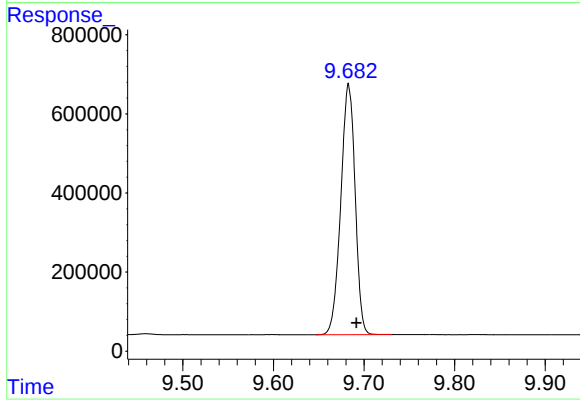

#5 N-HEXADECANE


R.T.: 9.683 min
Delta R.T.: -0.009 min
Response: 6962821
Conc: 49.48 ug/ml

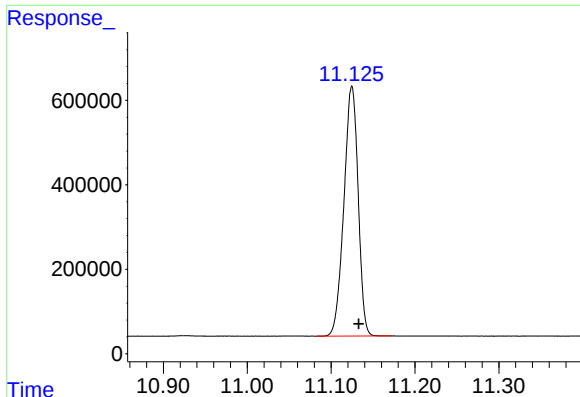

#6 N-OCTADECANE


R.T.: 11.125 min
Delta R.T.: -0.008 min
Response: 6975953
Conc: 49.21 ug/ml

Instrument :
FID_G
ClientSampleId :

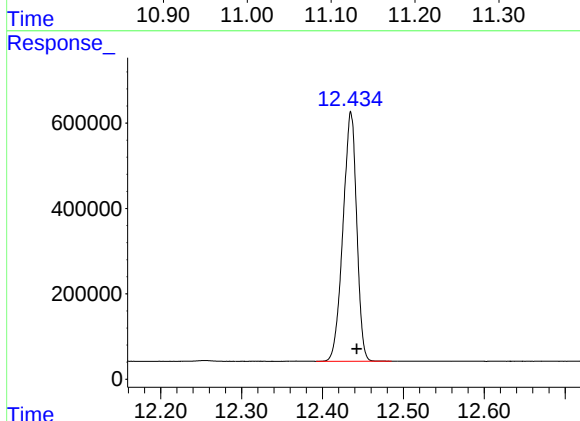


#7 N-EICOSANE

R.T.: 12.435 min
Delta R.T.: -0.007 min
Response: 6888648
Conc: 48.92 ug/ml

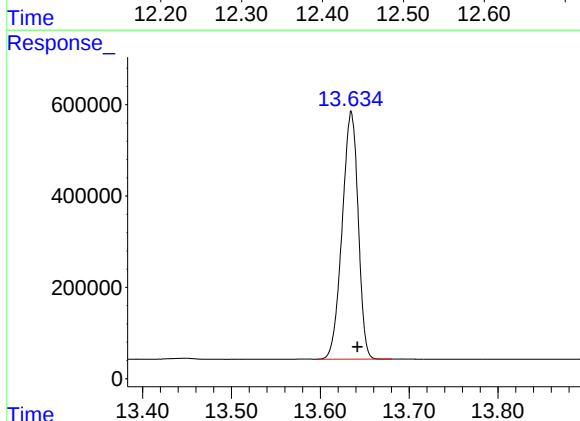


#8 N-DOCOSANE

R.T.: 13.635 min
Delta R.T.: -0.007 min
Response: 6789525
Conc: 48.45 ug/ml

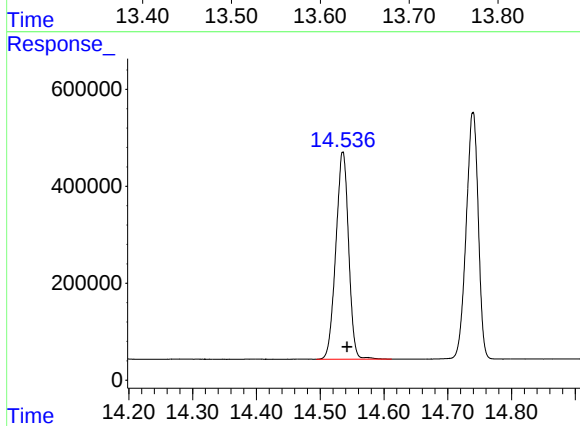

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.536 min
Delta R.T.: -0.007 min
Response: 5930569
Conc: 48.51 ug/ml

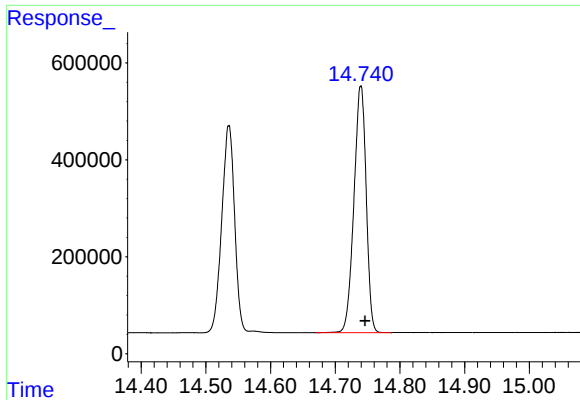

#10 N-TETRACOSANE


R.T.: 14.740 min
Delta R.T.: -0.007 min
Response: 6692804
Conc: 48.13 ug/ml

Instrument :
FID_G
ClientSampleId :

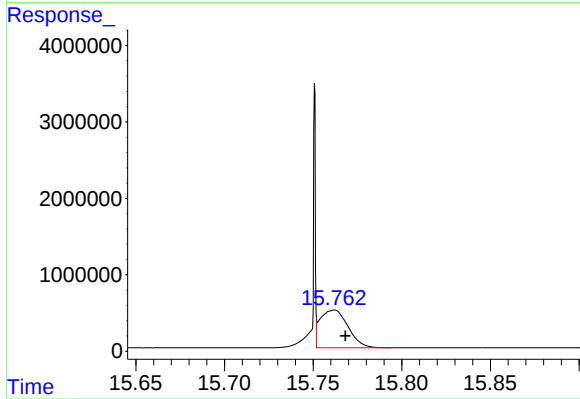

#11 N-HEXACOSANE

R.T.: 15.762 min
Delta R.T.: -0.006 min
Response: 5321956
Conc: 38.42 ug/ml m

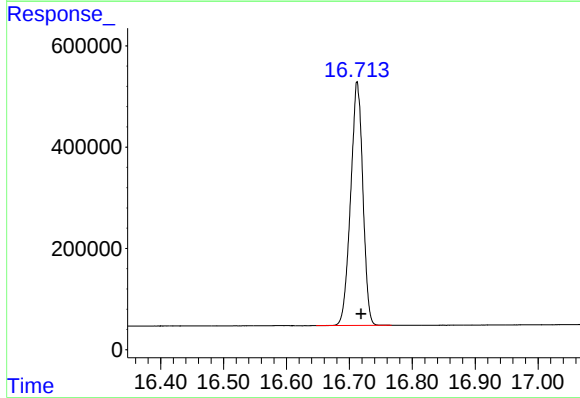

#12 N-OCTACOSANE

R.T.: 16.712 min
Delta R.T.: -0.006 min
Response: 6491305
Conc: 47.05 ug/ml