

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062722\
Data File : FG009997.D
Signal(s) : FID1A.ch
Acq On : 27 Jun 2022 23:10
Operator : AJ\MA
Sample : PB145850BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:26:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.818	2376158	22.575 ug/ml
Target Compounds			
17) N-OCTATRIACONTANE	20.970	536248	7.467 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062722\
Data File : FG009997.D
Signal(s) : FID1A.ch
Acq On : 27 Jun 2022 23:10
Operator : AJ\MA
Sample : PB145850BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 01:26:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

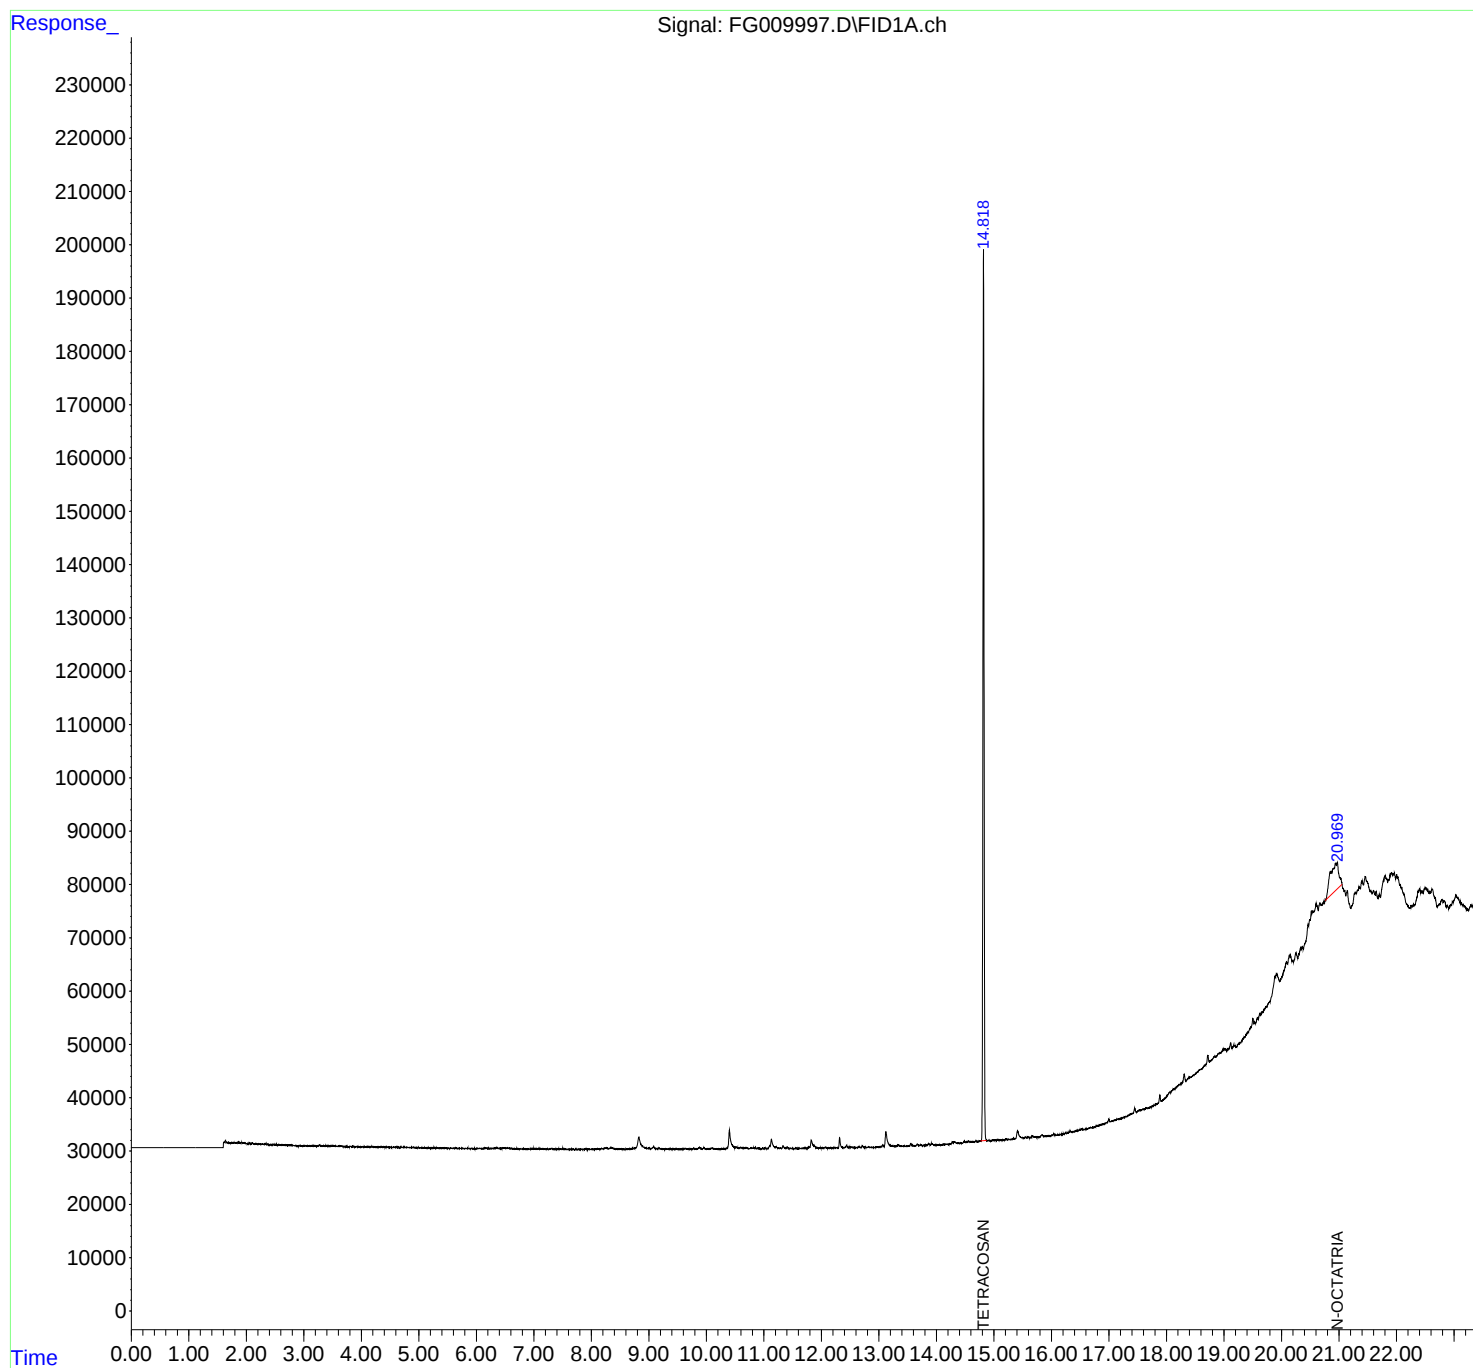


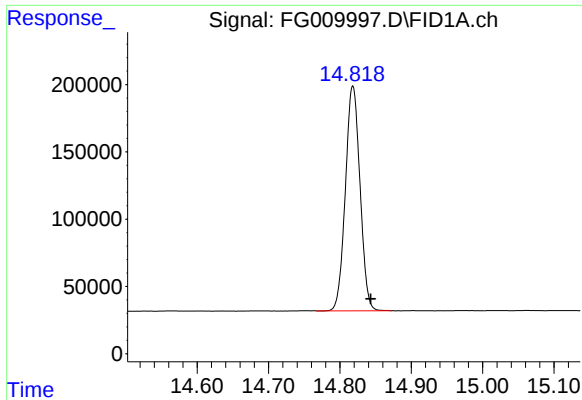

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.818 min
Delta R.T.: -0.025 min
Response: 2376158
Conc: 22.58 ug/ml

Instrument :
FID_G
ClientSampleId :

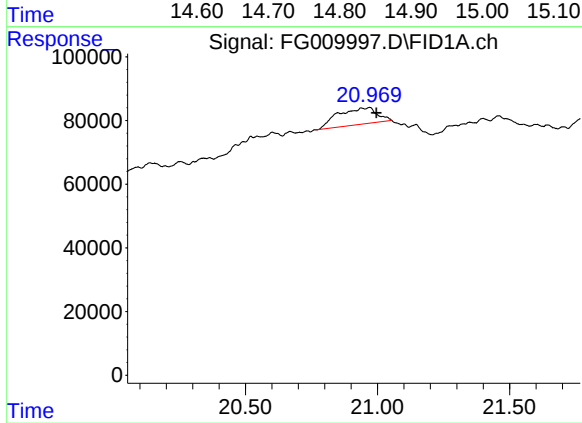

#17 N-OCTATRIACONTANE

R.T.: 20.970 min
Delta R.T.: -0.026 min
Response: 536248
Conc: 7.47 ug/ml