

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062722\
 Data File : FG010005.D
 Signal(s) : FID1A.ch
 Acq On : 28 Jun 2022 03:03
 Operator : AJ\MA
 Sample : N3494-34 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 28 05:14:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
 Quant Title :
 QLast Update : Wed Jun 01 13:06:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.820	203437	1.933 ug/ml
Target Compounds			
3) N-DODECANE	6.590	117091	0.928 ug/ml
7) N-EICOSANE	12.747	246789	2.018 ug/ml
8) N-DOCOSANE	13.915	75312	0.625 ug/ml
12) N-OCTACOSANE	16.999	99112	0.866 ug/ml
13) N-TRIACONTANE	17.889	181942	1.690 ug/ml
14) N-DOTRIACONTANE	18.724	41301	0.392 ug/ml
15) N-TETRATRIACONTANE	19.540	247874	2.582 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062722\
Data File : FG010005.D
Signal(s) : FID1A.ch
Acq On : 28 Jun 2022 03:03
Operator : AJ\MA
Sample : N3494-34 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 05:14:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

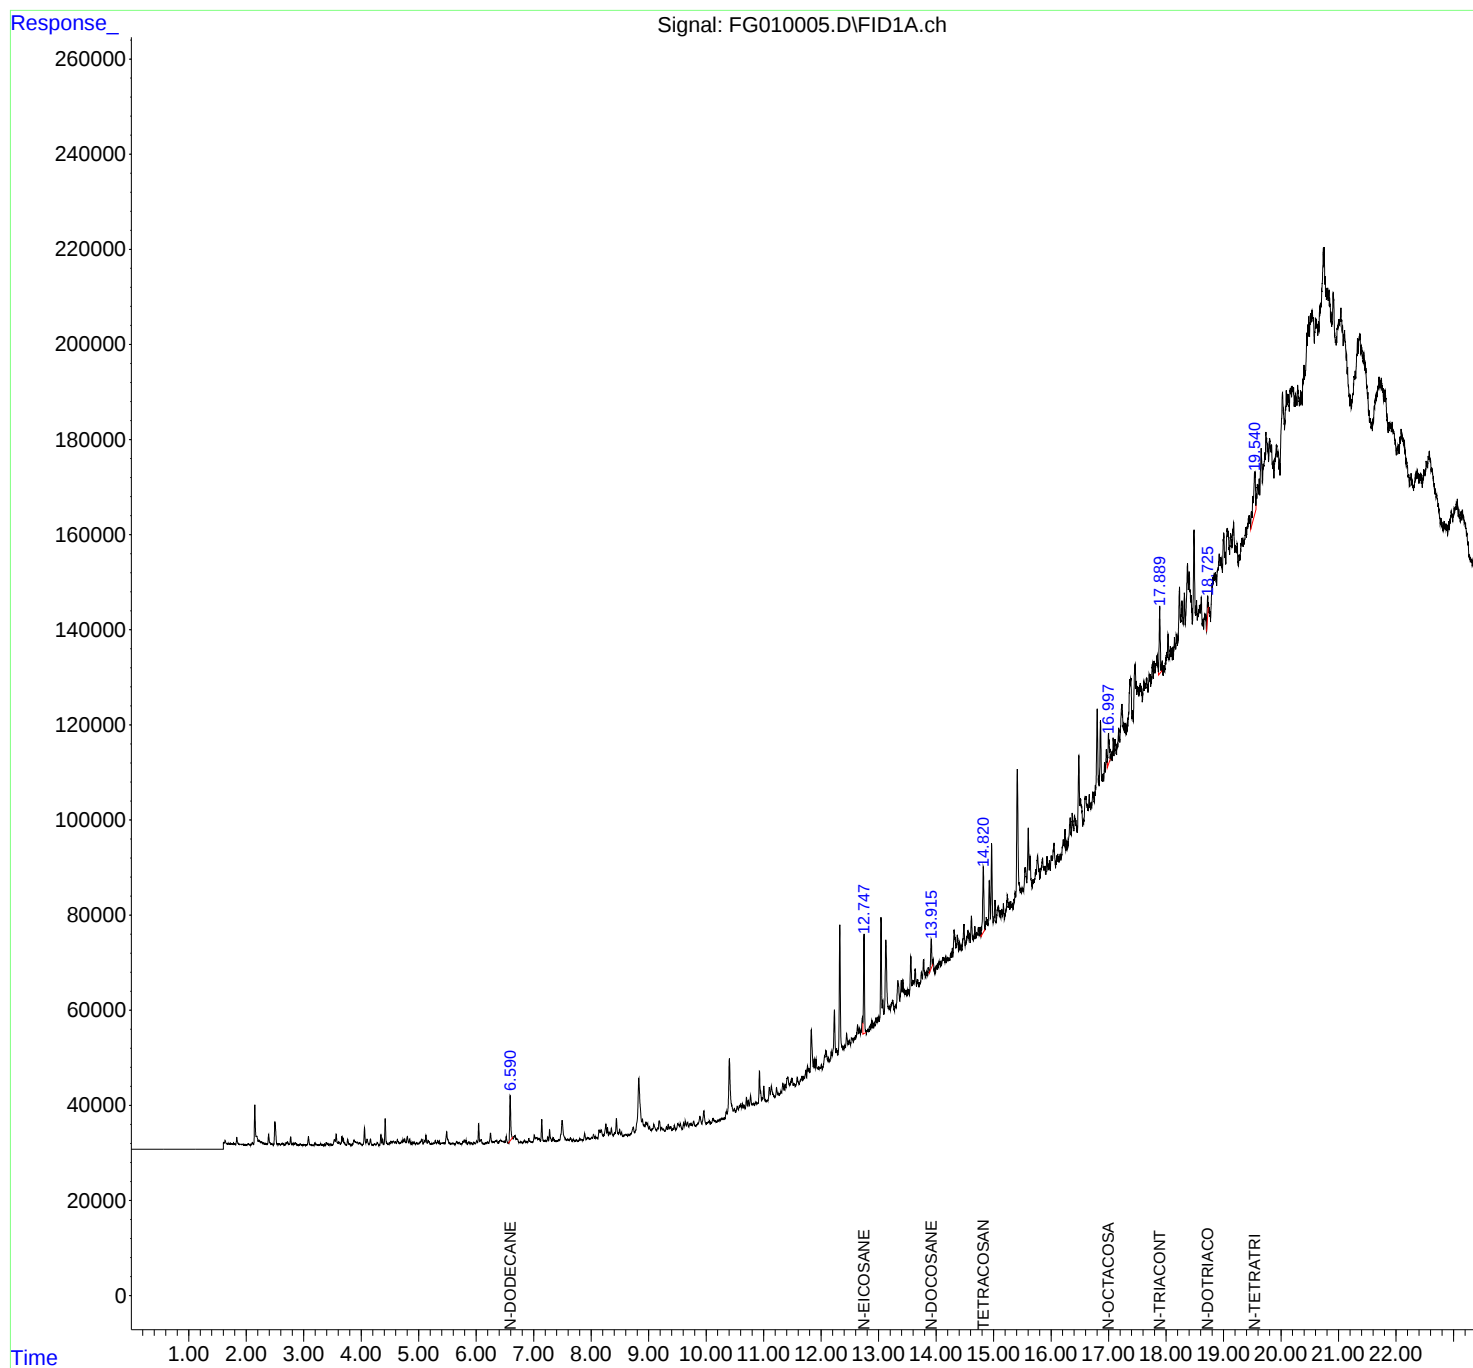


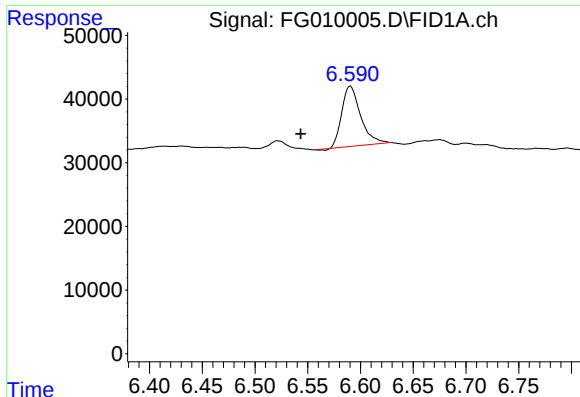

#3 N-DODECANE


R.T.: 6.590 min
Delta R.T.: 0.047 min
Response: 117091
Conc: 0.93 ug/ml

Instrument :
FID_G
ClientSampleId :

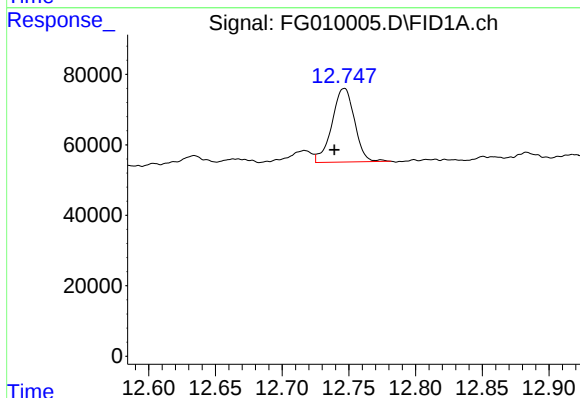


#7 N-EICOSANE

R.T.: 12.747 min
Delta R.T.: 0.007 min
Response: 246789
Conc: 2.02 ug/ml

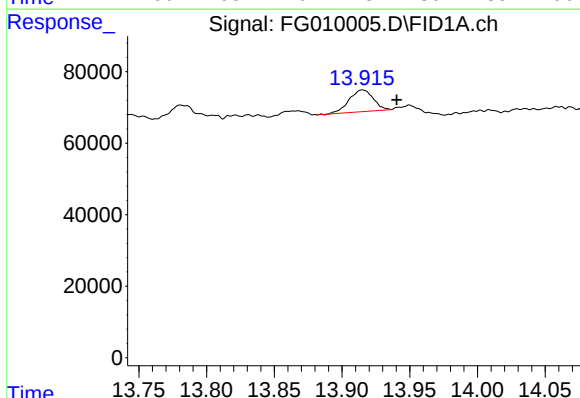


#8 N-DOCOSANE

R.T.: 13.915 min
Delta R.T.: -0.025 min
Response: 75312
Conc: 0.62 ug/ml

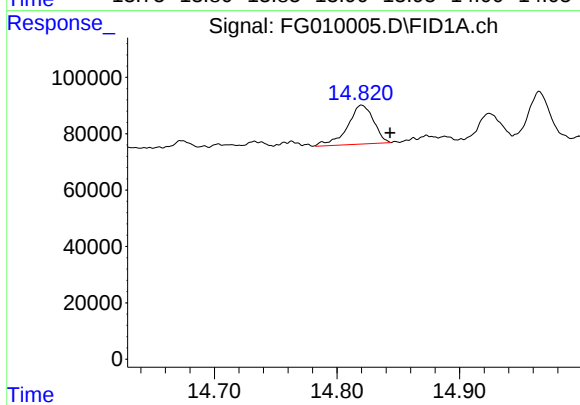

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.820 min
Delta R.T.: -0.023 min
Response: 203437
Conc: 1.93 ug/ml

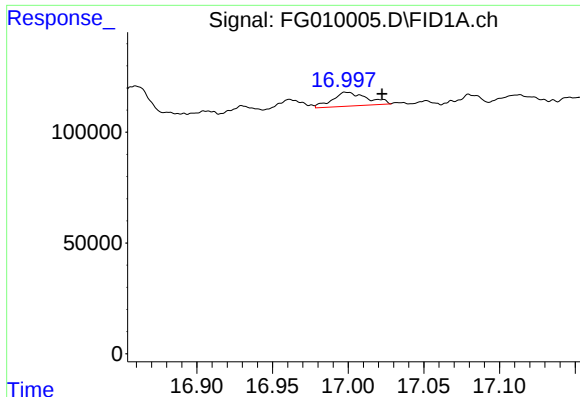

#12 N-OCTACOSANE


R.T.: 16.999 min
Delta R.T.: -0.024 min
Response: 99112
Conc: 0.87 ug/ml

Instrument :
FID_G
ClientSampleId :

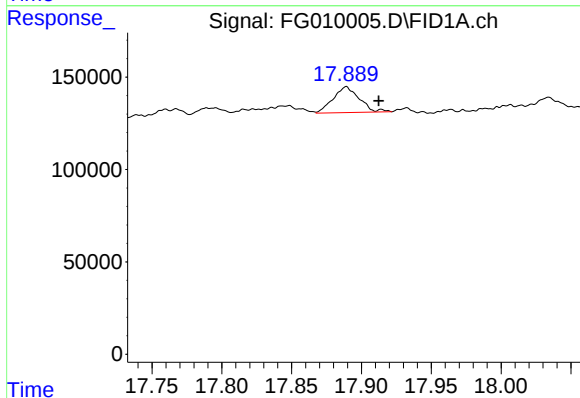


#13 N-TRIACONTANE

R.T.: 17.889 min
Delta R.T.: -0.023 min
Response: 181942
Conc: 1.69 ug/ml

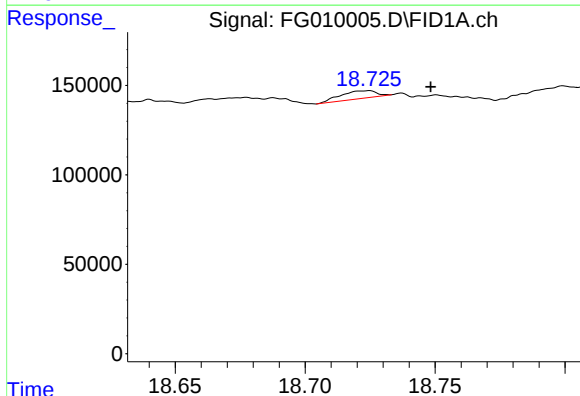

#14 N-DOTRIACONTANE

R.T.: 18.724 min
Delta R.T.: -0.024 min
Response: 41301
Conc: 0.39 ug/ml

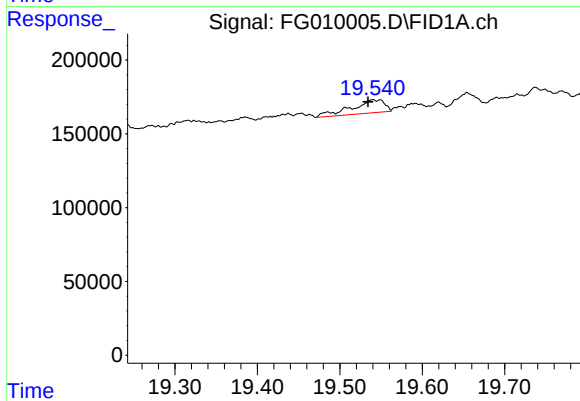

#15 N-TETRATRIACONTANE

R.T.: 19.540 min
Delta R.T.: 0.006 min
Response: 247874
Conc: 2.58 ug/ml