

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062723AL\
 Data File : FG012300.D
 Signal(s) : FID1A.ch
 Acq On : 27 Jun 2023 10:14
 Operator : YP\AJ
 Sample : 03357-14DL2 50X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 27 11:20:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 062023.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 20 14:37:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.332	64734	0.575 ug/ml
Spiked Amount 50.000		Recovery =	1.15%
Target Compounds			
13) T n-Docosane (C22)	13.146f	7858	0.062 ug/ml
14) T n-Tetracosane (C24)	14.167	139253	1.046 ug/ml
15) T n-Hexacosane (C26)	15.250	60157	0.491 ug/ml
16) T n-Octacosane (C28)	16.182	65024	0.538 ug/ml
17) T n-Tricontane (C30)	17.049	64869	0.521 ug/ml
18) T n-Dotriacontane (C32)	17.884	46974	0.379 ug/ml
19) T n-Tetratriacontane (C34)	18.691	157689	1.318 ug/ml
20) T n-Hexatriacontane (C36)	19.414	21029	0.182 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062723AL\
Data File : FG012300.D
Signal(s) : FID1A.ch
Acq On : 27 Jun 2023 10:14
Operator : YP\AJ
Sample : 03357-14DL2 50X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 27 11:20:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 062023.M
Quant Title : GC Extractables
QLast Update : Tue Jun 20 14:37:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

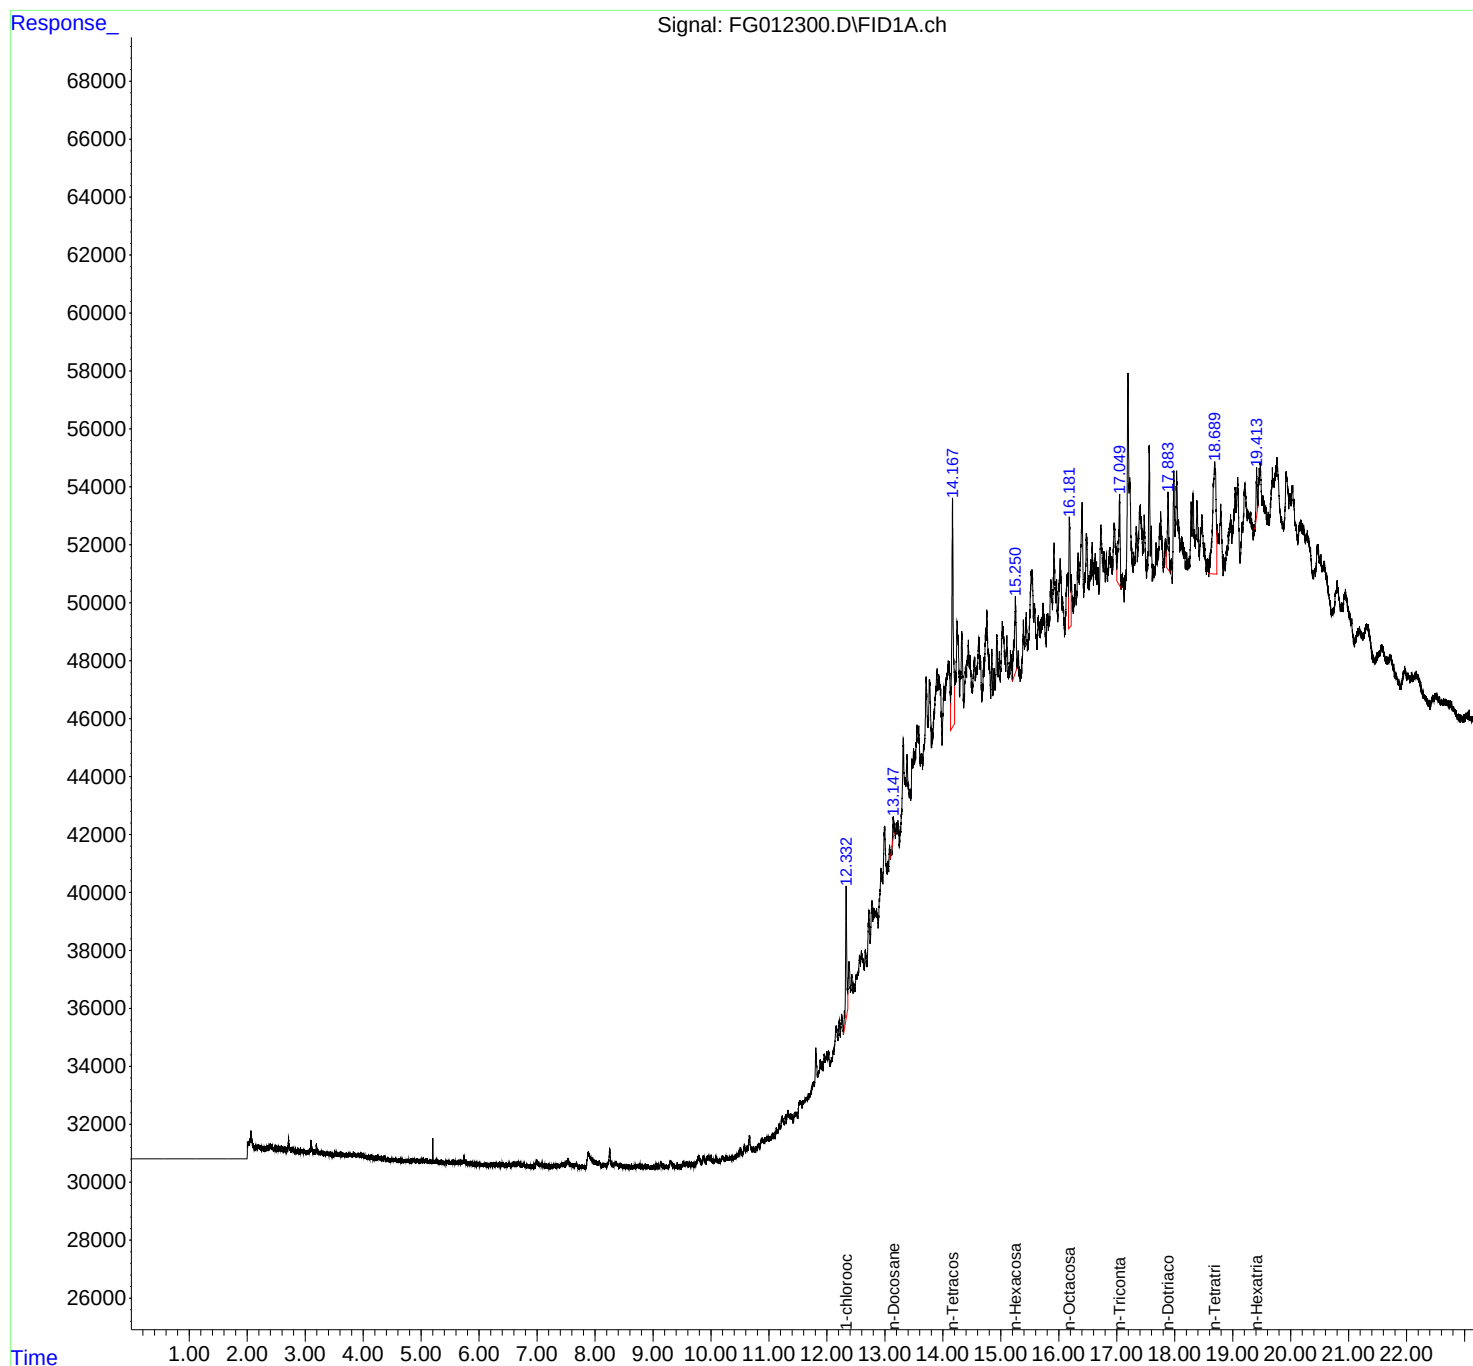


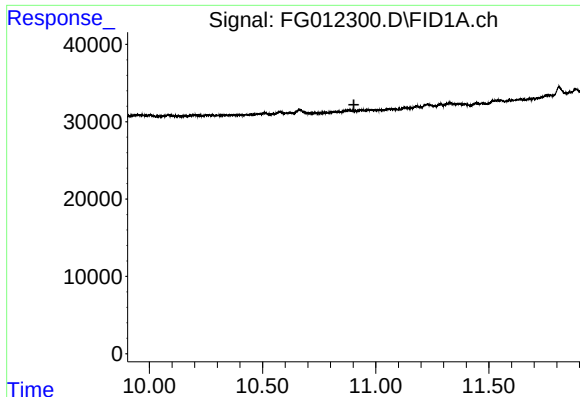

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.903 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

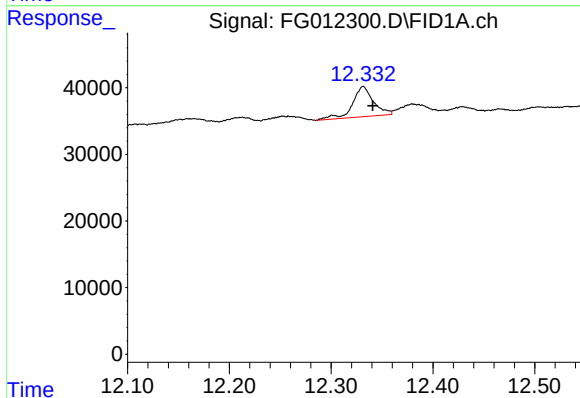


#12 1-chlorooctadecane (SURR)

R.T.: 12.332 min
Delta R.T.: -0.009 min
Response: 64734
Conc: 0.57 ug/ml

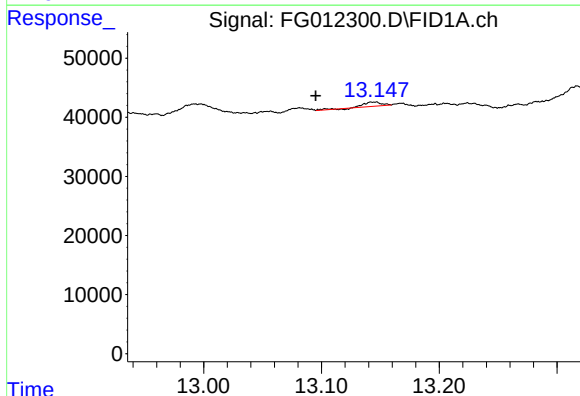


#13 n-Docosane (C22)

R.T.: 13.146 min
Delta R.T.: 0.051 min
Response: 7858
Conc: 0.06 ug/ml

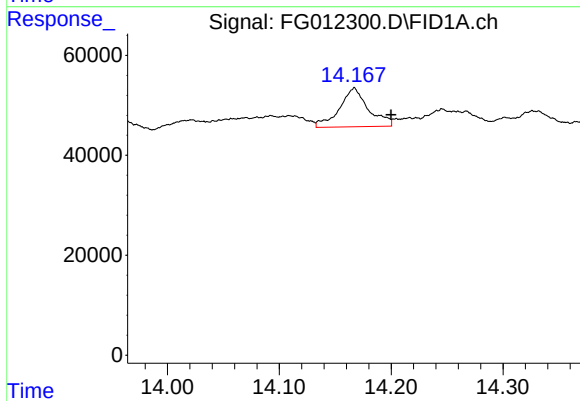

#14 n-Tetracosane (C24)


R.T.: 14.167 min
Delta R.T.: -0.033 min
Response: 139253
Conc: 1.05 ug/ml

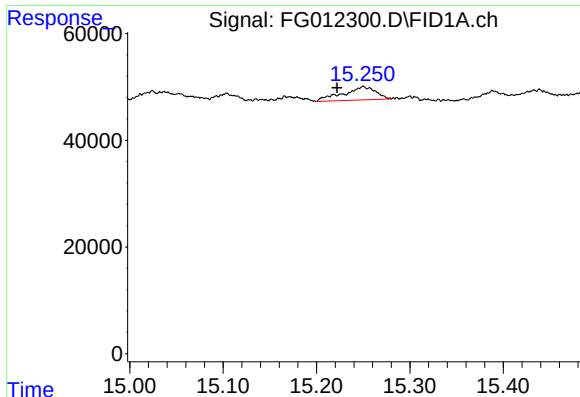

#15 n-Hexacosane (C26)


R.T.: 15.250 min
Delta R.T.: 0.028 min
Response: 60157
Conc: 0.49 ug/ml

Instrument :
FID_G
ClientSampleId :

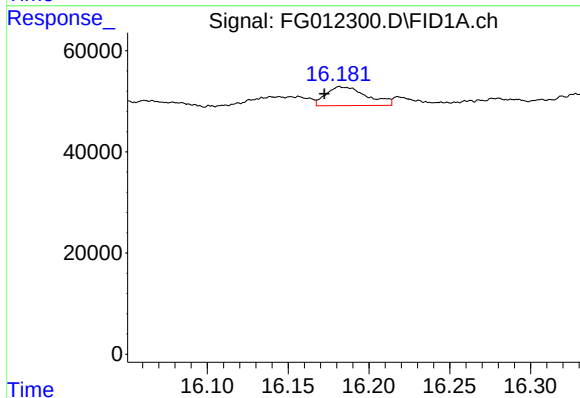


#16 n-Octacosane (C28)

R.T.: 16.182 min
Delta R.T.: 0.010 min
Response: 65024
Conc: 0.54 ug/ml

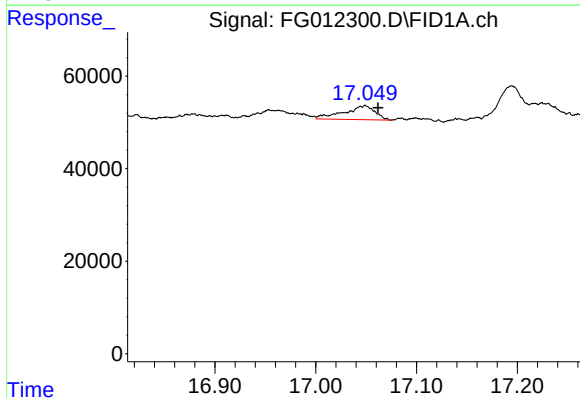


#17 n-Tricontane (C30)

R.T.: 17.049 min
Delta R.T.: -0.013 min
Response: 64869
Conc: 0.52 ug/ml

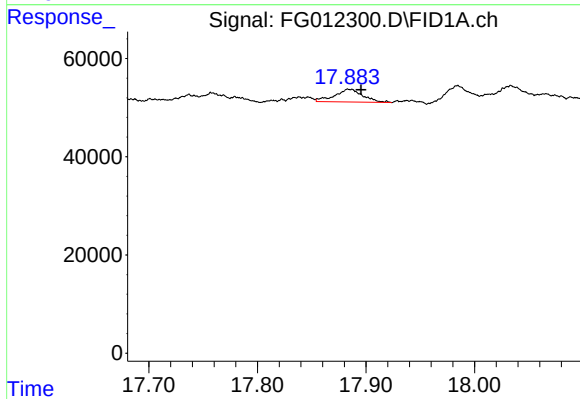

#18 n-Dotriacontane (C32)


R.T.: 17.884 min
Delta R.T.: -0.011 min
Response: 46974
Conc: 0.38 ug/ml

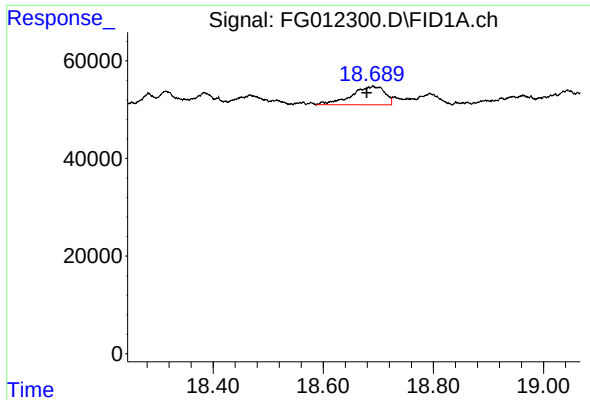

#19 n-Tetratriacontane (C34)

R.T.: 18.691 min
Delta R.T.: 0.011 min
Response: 157689
Conc: 1.32 ug/ml

Instrument :
FID_G
ClientSampleId :

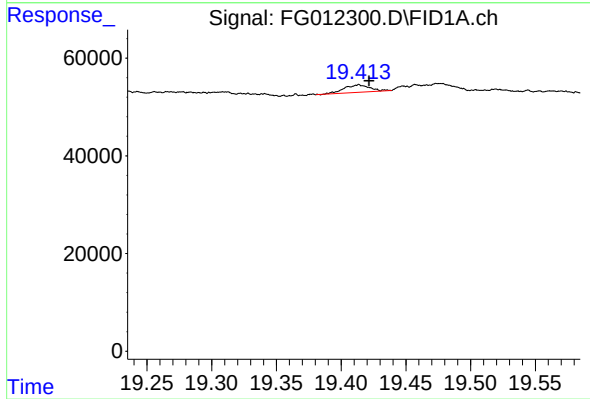

#20 n-Hexatriacontane (C36)

R.T.: 19.414 min
Delta R.T.: -0.008 min
Response: 21029
Conc: 0.18 ug/ml