

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062723AL\
 Data File : FG012304.D
 Signal(s) : FID1A.ch
 Acq On : 27 Jun 2023 12:11
 Operator : YP\AJ
 Sample : 03357-27DL2 100X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 27 13:42:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 062023.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 20 14:37:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	12.332	67637	0.600 ug/ml
Spiked Amount 50.000		Recovery =	1.20%
Target Compounds			
11) T n-Heneicosane (C21)	12.562f	11642	0.091 ug/ml
13) T n-Docosane (C22)	13.082	6078	0.048 ug/ml
14) T n-Tetracosane (C24)	14.166	134005	1.007 ug/ml
15) T n-Hexacosane (C26)	15.246	99831	0.814 ug/ml
16) T n-Octacosane (C28)	16.185	43064	0.356 ug/ml
17) T n-Tricontane (C30)	17.045	37903	0.305 ug/ml
19) T n-Tetratriacontane (C34)	18.692	176196	1.473 ug/ml
20) T n-Hexatriacontane (C36)	19.420	24757	0.215 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062723AL\
Data File : FG012304.D
Signal(s) : FID1A.ch
Acq On : 27 Jun 2023 12:11
Operator : YP\AJ
Sample : 03357-27DL2 100X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 27 13:42:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 062023.M
Quant Title : GC Extractables
QLast Update : Tue Jun 20 14:37:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

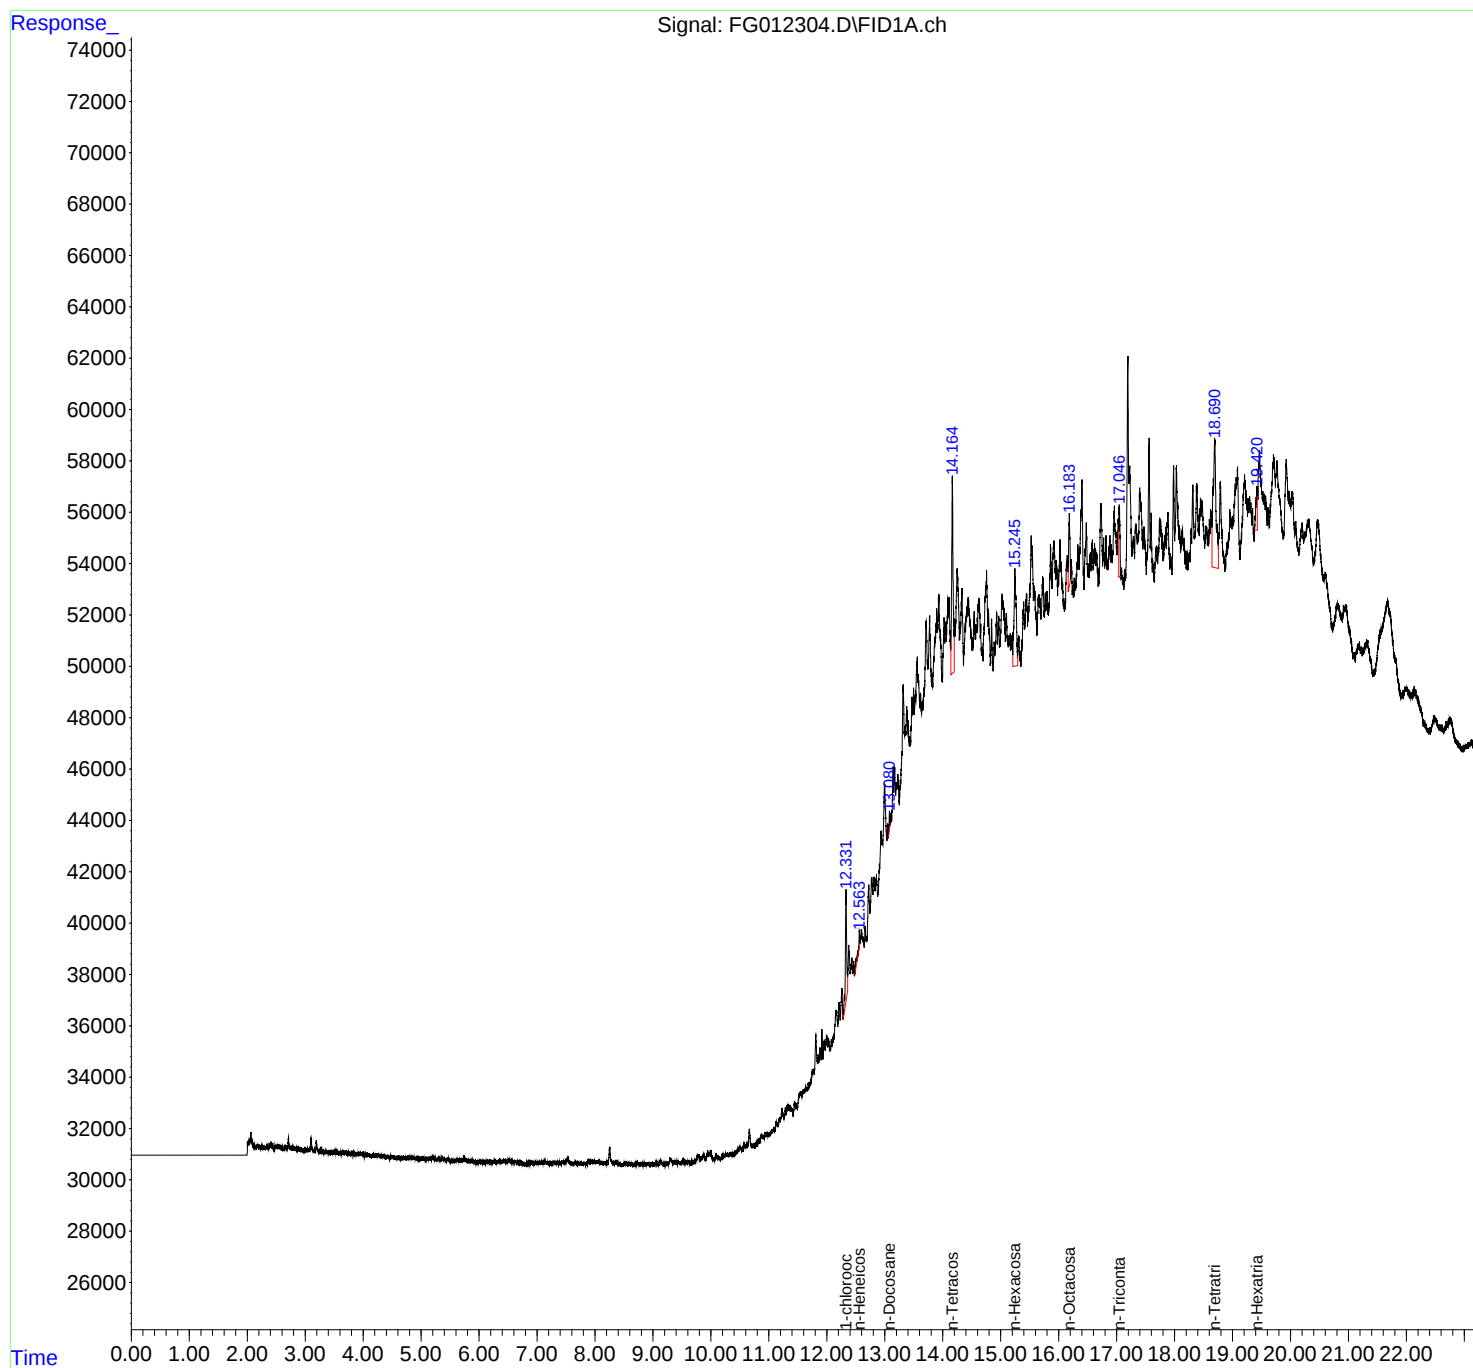


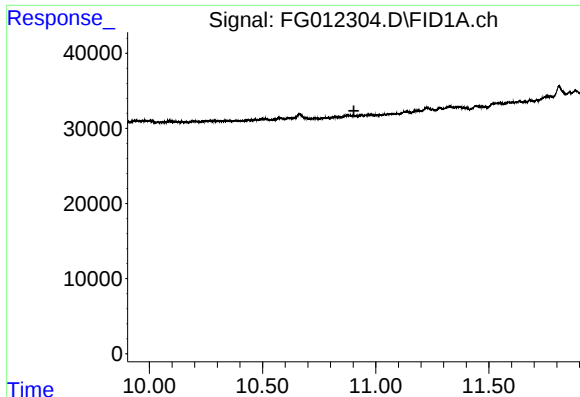

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 10.903 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

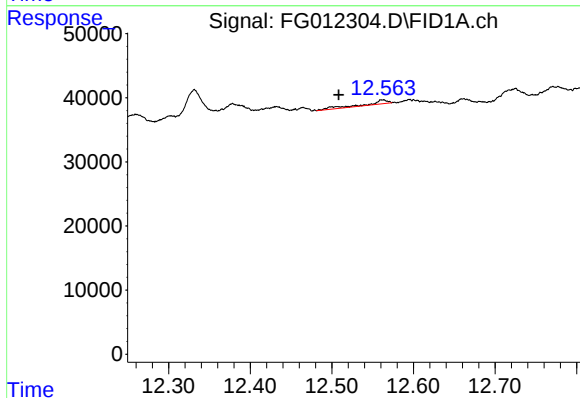


#11 n-Heneicosane (C21)

R.T.: 12.562 min
Delta R.T.: 0.054 min
Response: 11642
Conc: 0.09 ug/ml

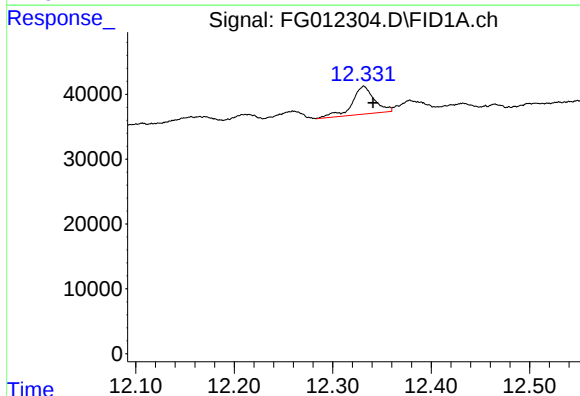


#12 1-chlorooctadecane (SURR)

R.T.: 12.332 min
Delta R.T.: -0.009 min
Response: 67637
Conc: 0.60 ug/ml

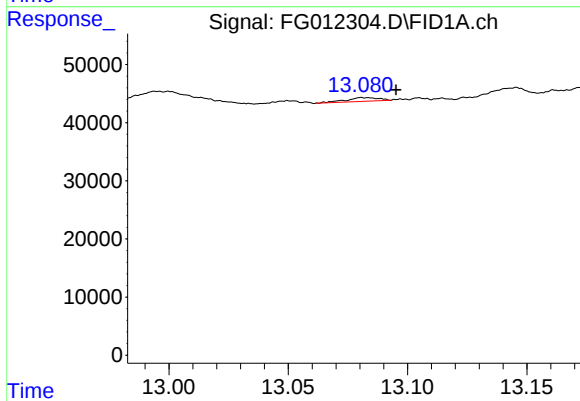

#13 n-Docosane (C22)


R.T.: 13.082 min
Delta R.T.: -0.014 min
Response: 6078
Conc: 0.05 ug/ml

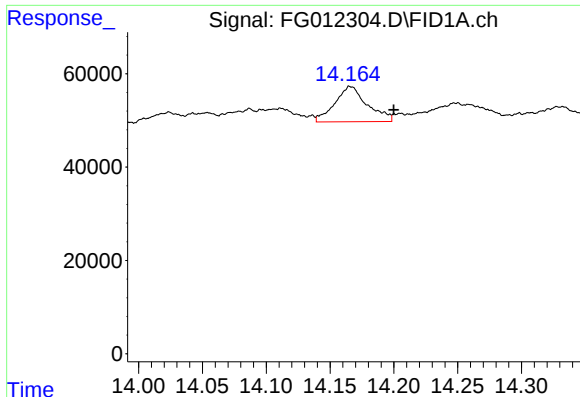

#14 n-Tetracosane (C24)


R.T.: 14.166 min
Delta R.T.: -0.034 min
Response: 134005
Conc: 1.01 ug/ml

Instrument :
FID_G
ClientSampleId :

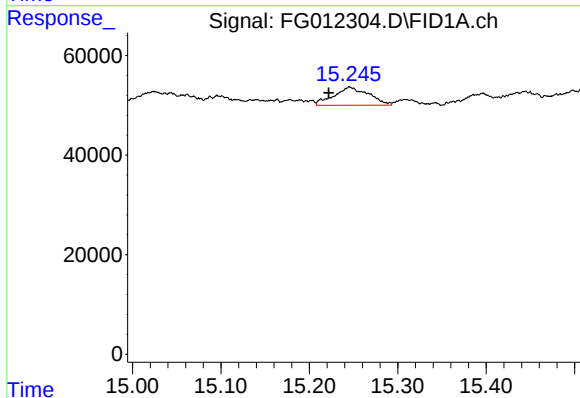


#15 n-Hexacosane (C26)

R.T.: 15.246 min
Delta R.T.: 0.024 min
Response: 99831
Conc: 0.81 ug/ml

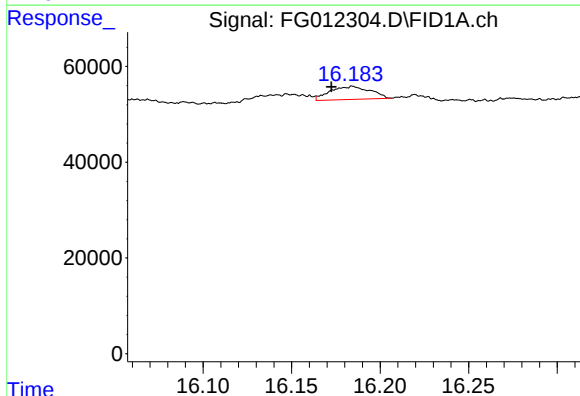


#16 n-Octacosane (C28)

R.T.: 16.185 min
Delta R.T.: 0.012 min
Response: 43064
Conc: 0.36 ug/ml

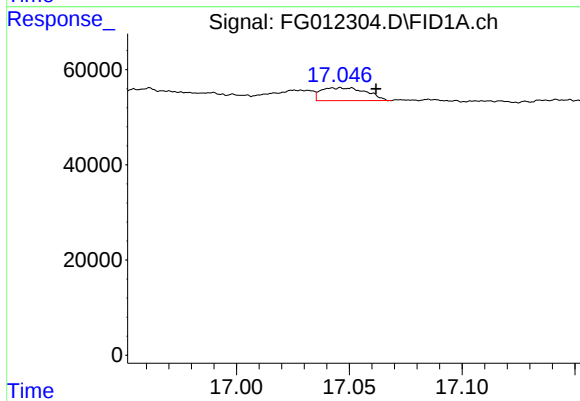

#17 n-Tricontane (C30)


R.T.: 17.045 min
Delta R.T.: -0.016 min
Response: 37903
Conc: 0.30 ug/ml

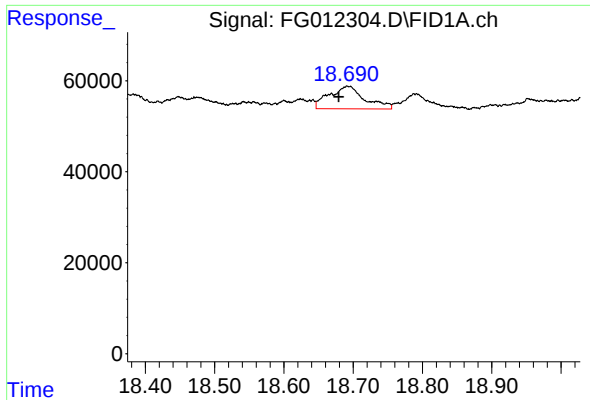

#19 n-Tetratriacontane (C34)

R.T.: 18.692 min
Delta R.T.: 0.012 min
Response: 176196
Conc: 1.47 ug/ml

Instrument :
FID_G
ClientSampleId :

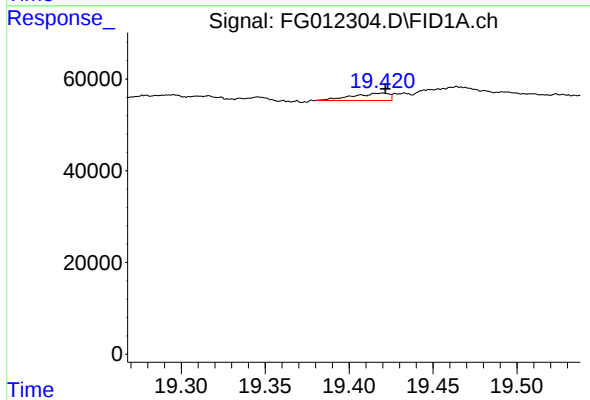

#20 n-Hexatriacontane (C36)

R.T.: 19.420 min
Delta R.T.: -0.001 min
Response: 24757
Conc: 0.21 ug/ml