

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062818\
 Data File : FG001508.D
 Signal(s) : FID1A.ch
 Acq On : 28 Jun 2018 14:52
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 28 15:17:51 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
 Quant Title :
 QLast Update : Fri Jun 01 15:28:31 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.535	6127454	50.122 ug/ml
Target Compounds			
2) N-DECANE	4.273	7602732	55.465 ug/ml
3) N-DODECANE	6.290	7638266	55.099 ug/ml
4) N-TETRADECANE	8.083	7617277	54.512 ug/ml
5) N-HEXADECANE	9.683	7578570	53.853 ug/ml
6) N-OCTADECANE	11.124	7518358	53.039 ug/ml
7) N-EICOSANE	12.435	7351846	52.209 ug/ml
8) N-DOCOSANE	13.635	7187304	51.284 ug/ml
10) N-TETRACOSANE	14.739	7032052	50.572 ug/ml
11) N-HEXACOSANE	15.761	6908223	49.868 ug/ml
12) N-OCTACOSANE	16.712	6819106	49.422 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062818\
Data File : FG001508.D
Signal(s) : FID1A.ch
Acq On : 28 Jun 2018 14:52
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 28 15:17:51 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_G\Method\FG060118.M
Quant Title :
QLast Update : Fri Jun 01 15:28:31 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

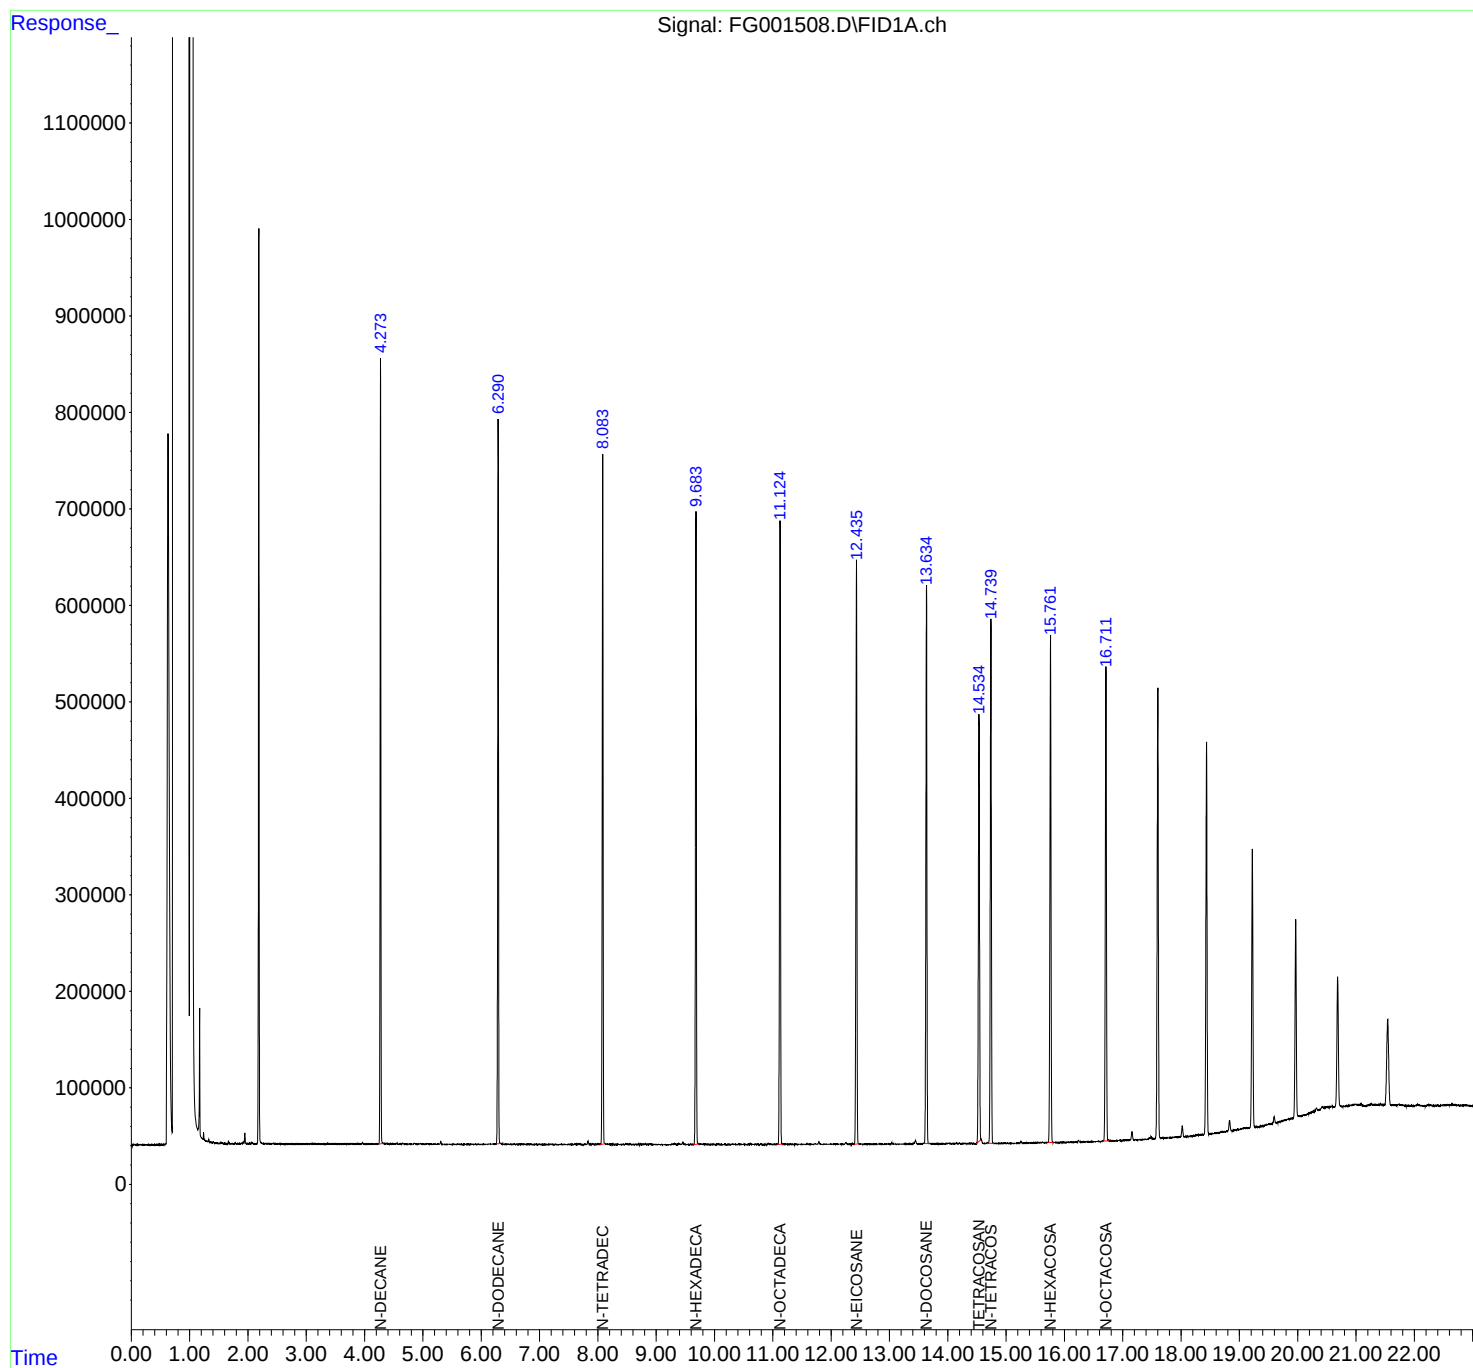

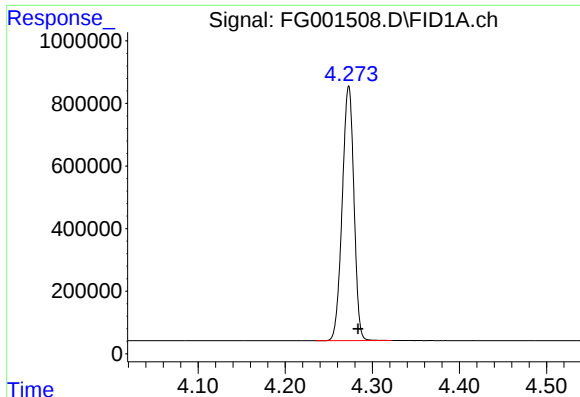


#2 N-DECANE

R.T.: 4.273 min
Delta R.T.: -0.011 min
Response: 7602732
Conc: 55.46 ug/ml

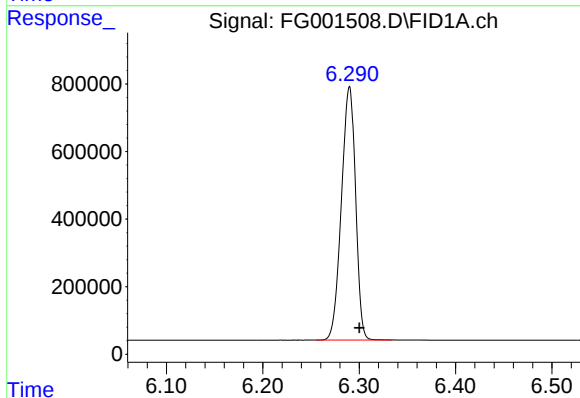


#3 N-DODECANE

R.T.: 6.290 min
Delta R.T.: -0.010 min
Response: 7638266
Conc: 55.10 ug/ml

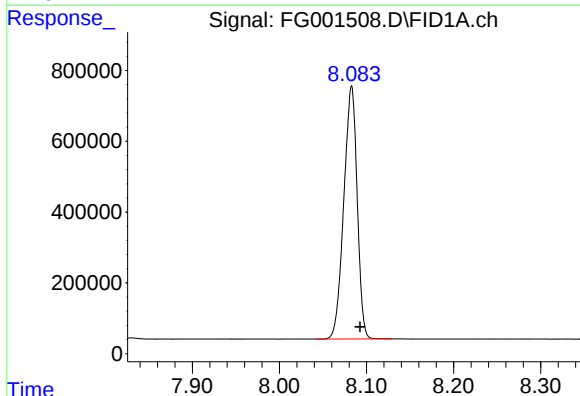


#4 N-TETRADECANE

R.T.: 8.083 min
Delta R.T.: -0.010 min
Response: 7617277
Conc: 54.51 ug/ml

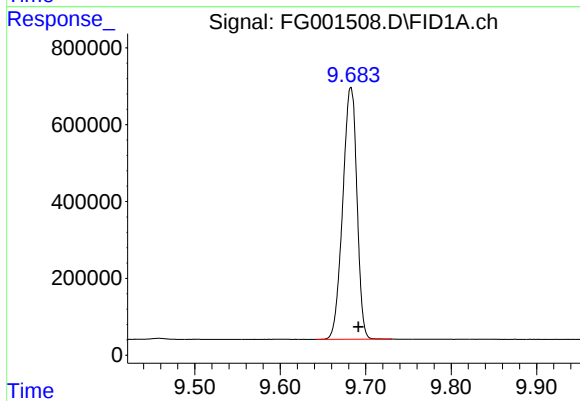


#5 N-HEXADECANE

R.T.: 9.683 min
Delta R.T.: -0.009 min
Response: 7578570
Conc: 53.85 ug/ml

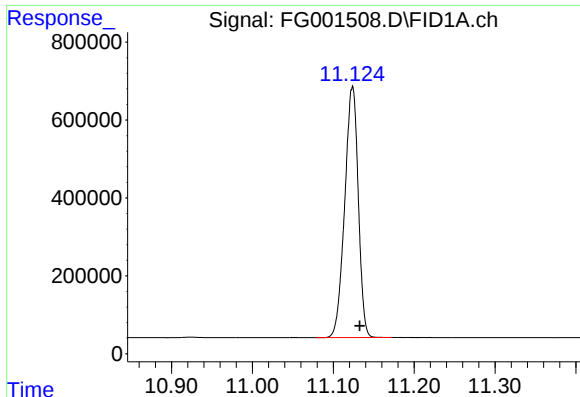


#6 N-OCTADECANE

R.T.: 11.124 min
Delta R.T.: -0.009 min
Response: 7518358
Conc: 53.04 ug/ml

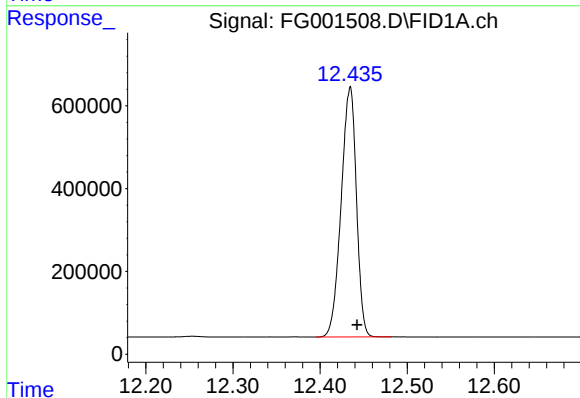


#7 N-EICOSANE

R.T.: 12.435 min
Delta R.T.: -0.008 min
Response: 7351846
Conc: 52.21 ug/ml

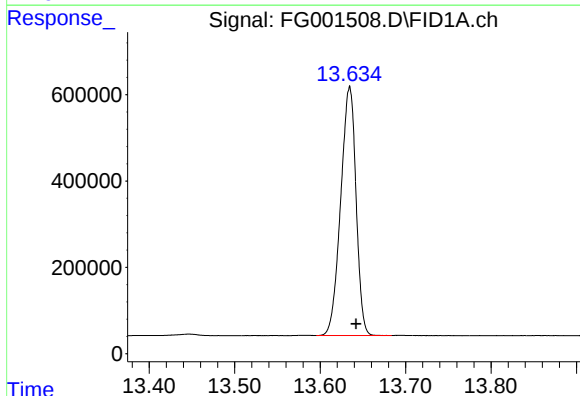


#8 N-DOCOSANE

R.T.: 13.635 min
Delta R.T.: -0.007 min
Response: 7187304
Conc: 51.28 ug/ml

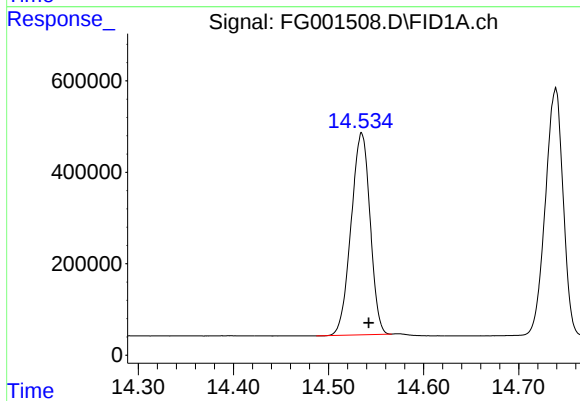


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.535 min
Delta R.T.: -0.007 min
Response: 6127454
Conc: 50.12 ug/ml

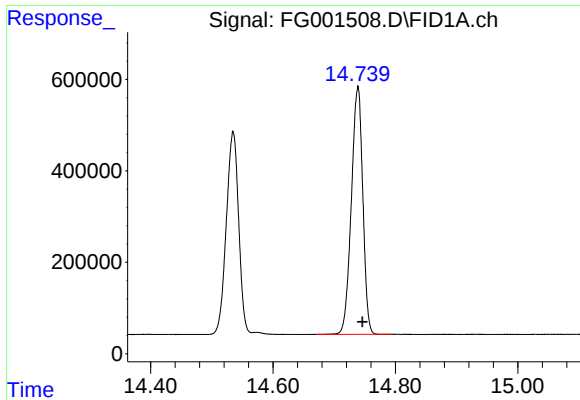


#10 N-TETRACOSANE

R.T.: 14.739 min
Delta R.T.: -0.007 min
Response: 7032052
Conc: 50.57 ug/ml

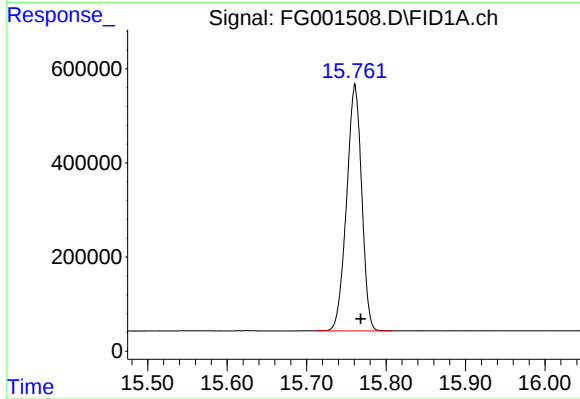

#11 N-HEXACOSANE

R.T.: 15.761 min
Delta R.T.: -0.007 min
Response: 6908223
Conc: 49.87 ug/ml

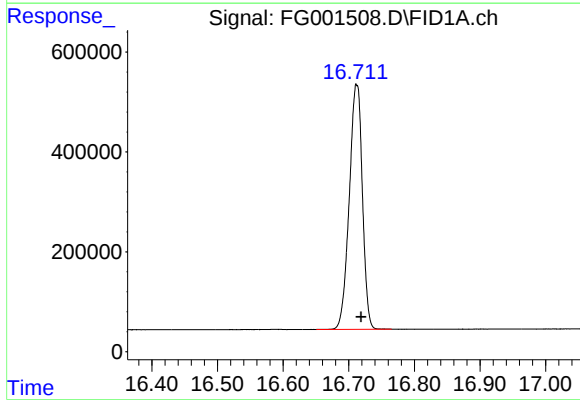

#12 N-OCTACOSANE

R.T.: 16.712 min
Delta R.T.: -0.007 min
Response: 6819106
Conc: 49.42 ug/ml