

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062821\
 Data File : FG008430.D
 Signal(s) : FID1A.ch
 Acq On : 28 Jun 2021 09:05
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 MECL2

Integration File: autoint1.e
 Quant Time: Jun 29 02:29:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062421.M
 Quant Title :
 QLast Update : Thu Jun 24 09:09:15 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) N-TETRACOSANE	14.948	255506	1.704 ug/ml
14) N-DOTRIACONTANE	18.685	260914	1.950 ug/ml
16) N-HEXATRIACONTANE	20.240	340536	3.082 ug/ml
18) N-TETRACONTANE	21.952	388973	4.075 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062821\
Data File : FG008430.D
Signal(s) : FID1A.ch
Acq On : 28 Jun 2021 09:05
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jun 29 02:29:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062421.M
Quant Title :
QLast Update : Thu Jun 24 09:09:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

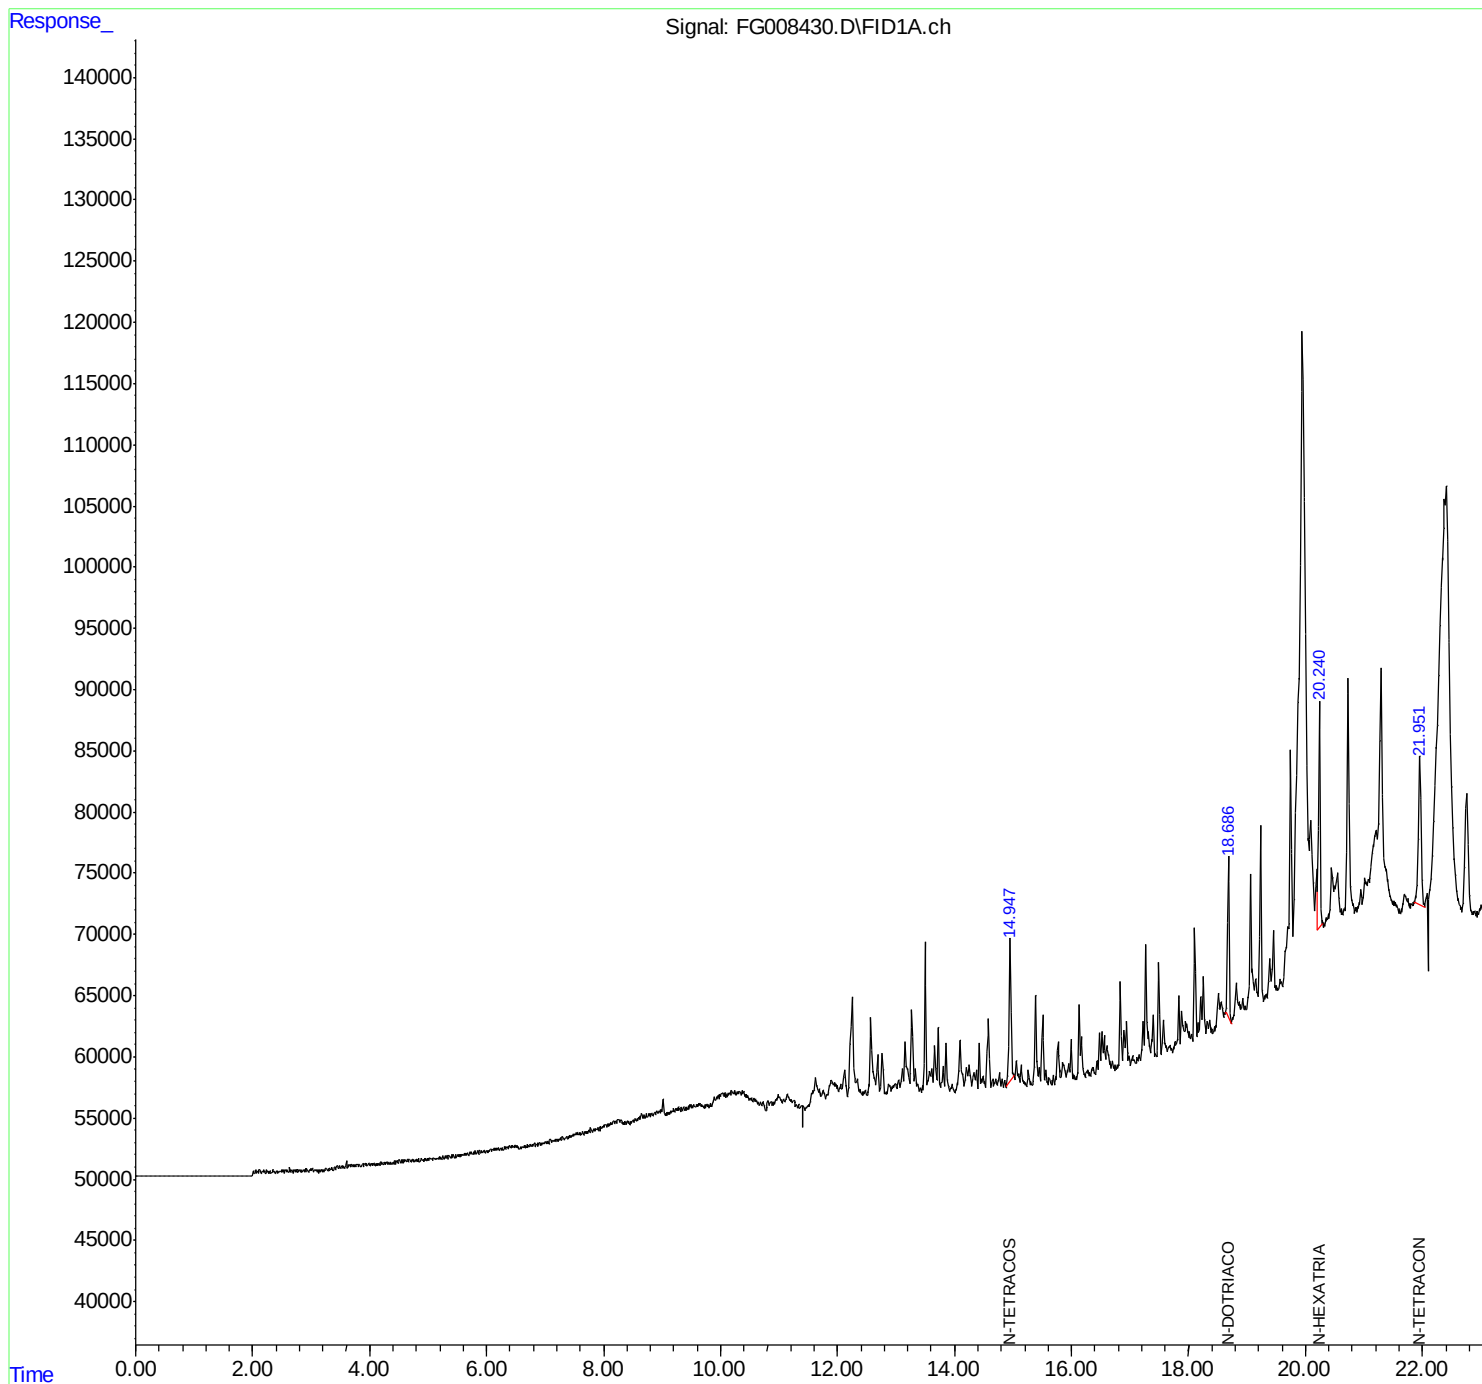


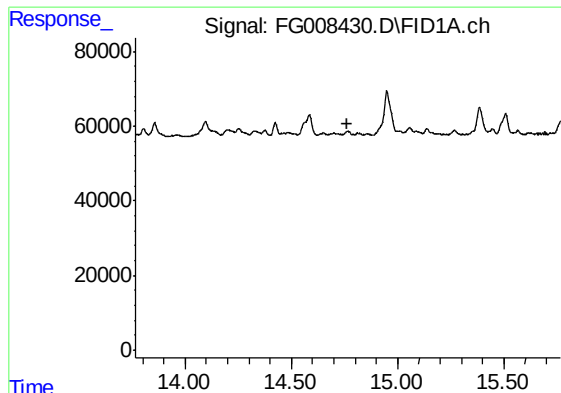

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.766 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :
MECL2

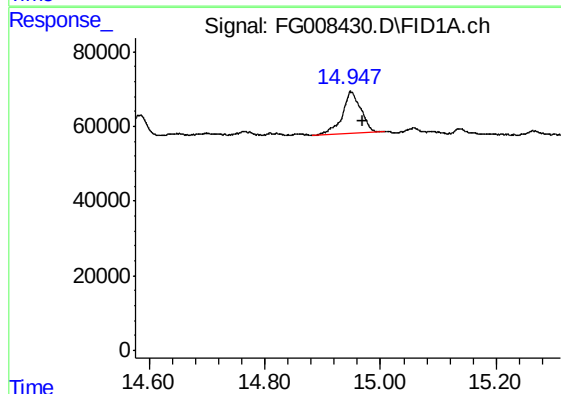


#10 N-TETRACOSANE

R.T.: 14.948 min
Delta R.T.: -0.021 min
Response: 255506
Conc: 1.70 ug/ml

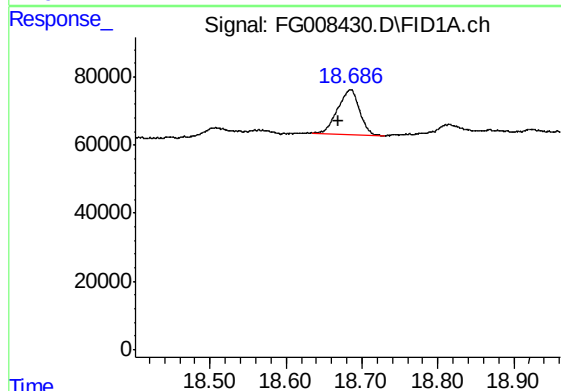


#14 N-DOTRIACONTANE

R.T.: 18.685 min
Delta R.T.: 0.017 min
Response: 260914
Conc: 1.95 ug/ml

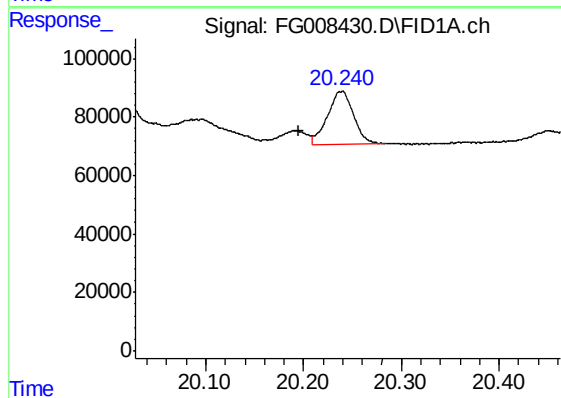

#16 N-HEXATRIACONTANE

R.T.: 20.240 min
Delta R.T.: 0.045 min
Response: 340536
Conc: 3.08 ug/ml

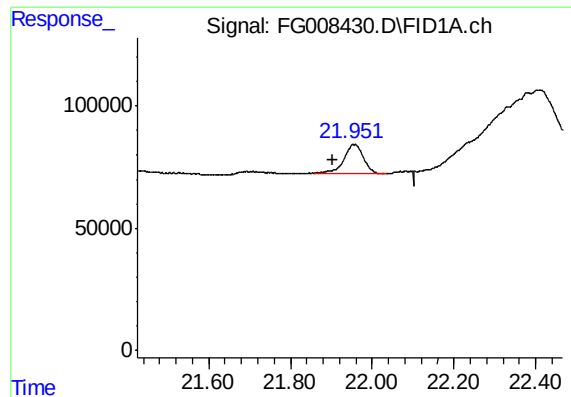

#18 N-TETRACONTANE

R.T.: 21.952 min
Delta R.T.: 0.050 min
Response: 388973
Conc: 4.08 ug/ml

Instrument :
FID_G
ClientSampleId :
MECL2