

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062821\
Data File : FG008454.D
Signal(s) : FID1A.ch
Acq On : 28 Jun 2021 22:42
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 29 02:34:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062421.M
Quant Title :
QLast Update : Thu Jun 24 09:09:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.768	2306847	17.632 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.670	104427	0.780 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062821\
Data File : FG008454.D
Signal(s) : FID1A.ch
Acq On : 28 Jun 2021 22:42
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 29 02:34:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062421.M
Quant Title :
QLast Update : Thu Jun 24 09:09:15 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

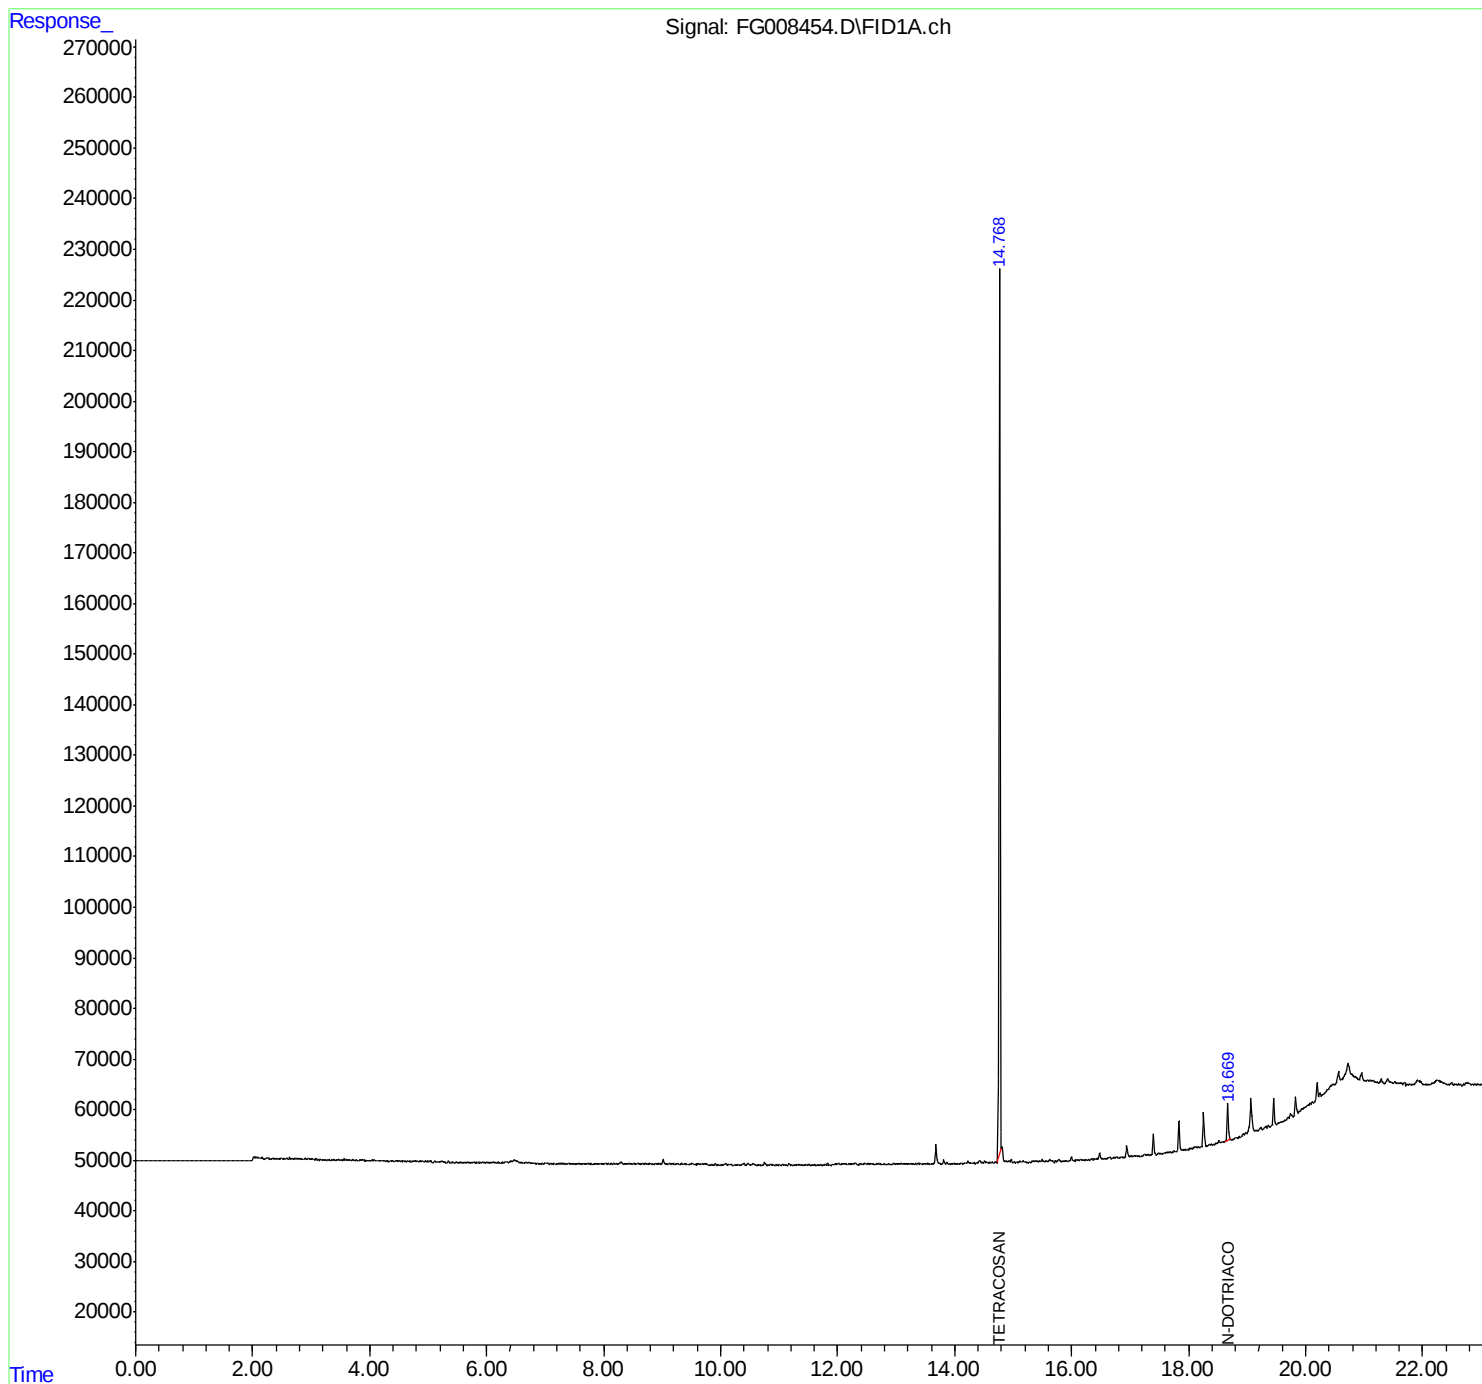


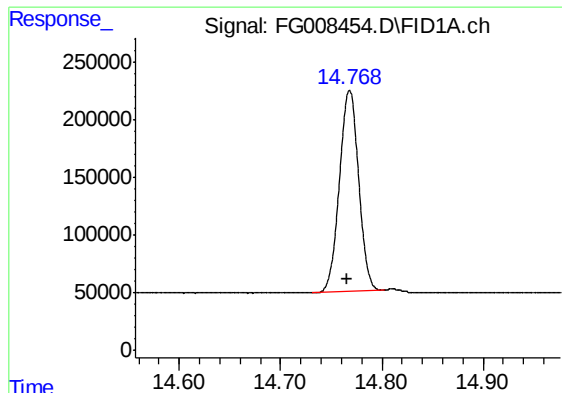

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.768 min
Delta R.T.: 0.002 min
Response: 2306847
Conc: 17.63 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK

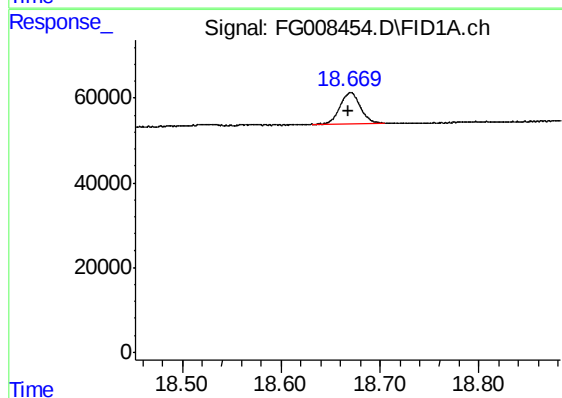

#14 N-DOTRIACONTANE

R.T.: 18.670 min
Delta R.T.: 0.002 min
Response: 104427
Conc: 0.78 ug/ml