

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062822\
Data File : FG010011.D
Signal(s) : FID1A.ch
Acq On : 28 Jun 2022 06:27
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Jun 29 01:25:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.521	3760067	29.805 ug/ml
12) N-OCTACOSANE	16.996	3510413	30.677 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG062822\
Data File : FG010011.D
Signal(s) : FID1A.ch
Acq On : 28 Jun 2022 06:27
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Jun 29 01:25:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060122.M
Quant Title :
QLast Update : Wed Jun 01 13:06:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

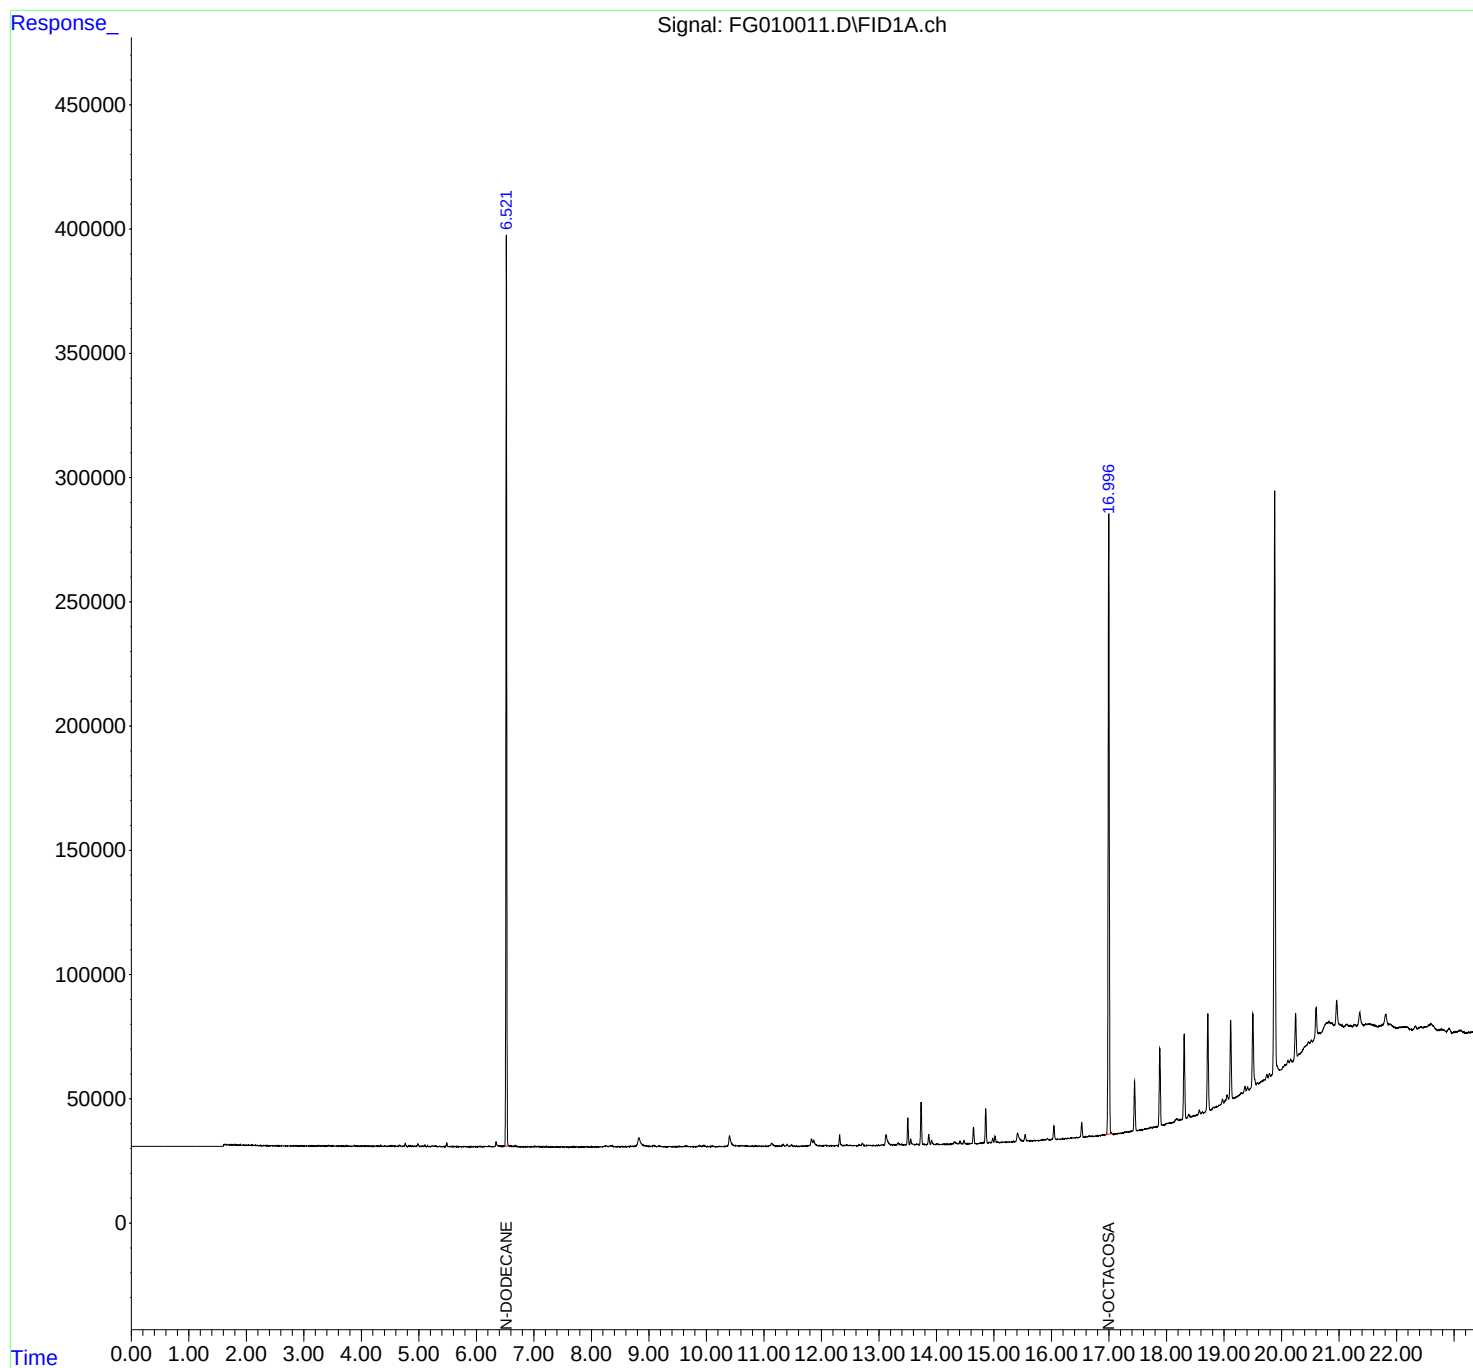


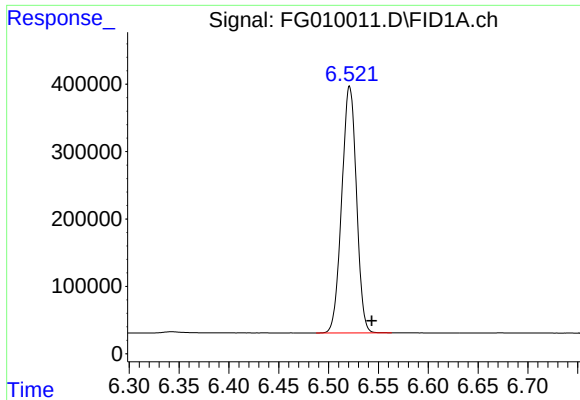

#3 N-DODECANE


R.T.: 6.521 min
Delta R.T.: -0.022 min
Response: 3760067
Conc: 29.80 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

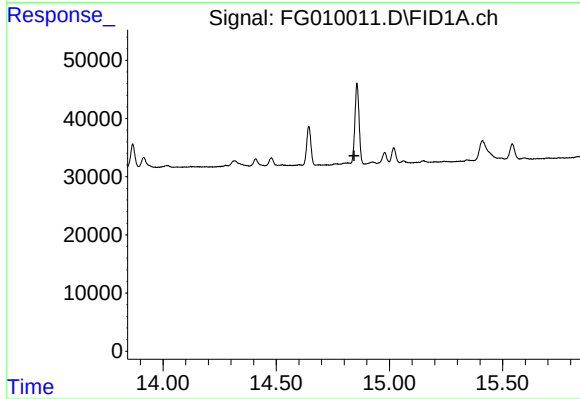

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.843 min
Response: 0
Conc: N.D.

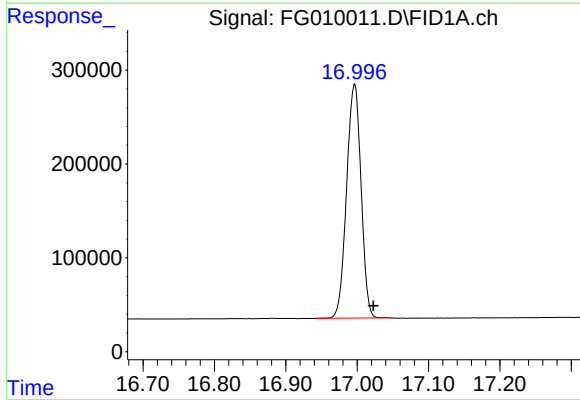

#12 N-OCTACOSANE

R.T.: 16.996 min
Delta R.T.: -0.026 min
Response: 3510413
Conc: 30.68 ug/ml