

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG063020\
Data File : FG006993.D
Signal(s) : FID1A.ch
Acq On : 30 Jun 2020 19:04
Operator : DD\AJ
Sample : L3157-03 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CB-D35

Integration File: autoint1.e
Quant Time: Jul 01 01:30:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG061520.M
Quant Title :
QLast Update : Tue Jun 16 03:44:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.781	437821	3.392 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG063020\
Data File : FG006993.D
Signal(s) : FID1A.ch
Acq On : 30 Jun 2020 19:04
Operator : DD\AJ
Sample : L3157-03 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
CB-D35

Integration File: autoint1.e
Quant Time: Jul 01 01:30:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG061520.M
Quant Title :
QLast Update : Tue Jun 16 03:44:57 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

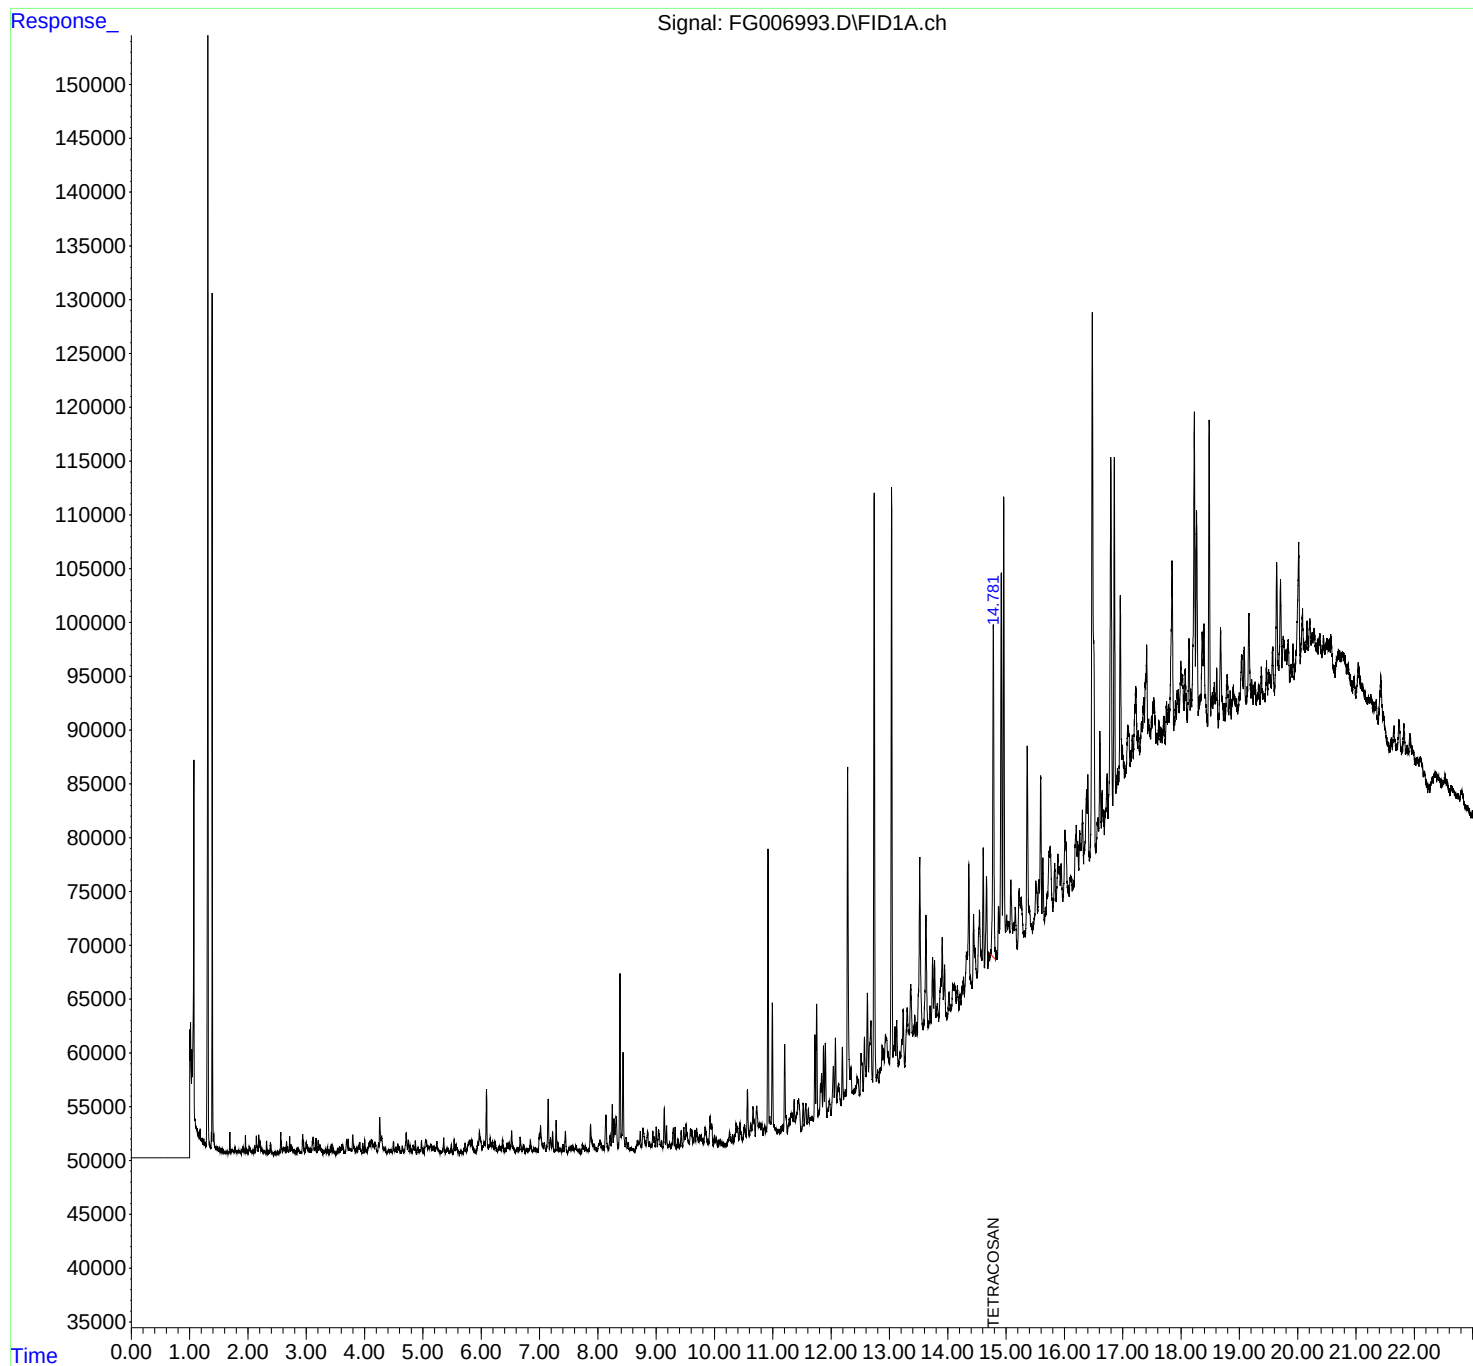

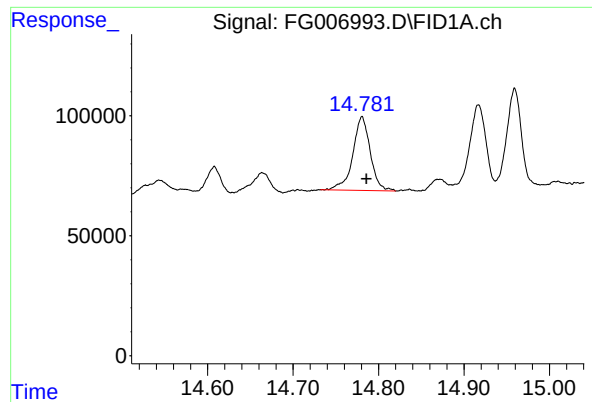

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.781 min
Delta R.T.: -0.005 min
Response: 437821
Conc: 3.39 ug/ml

Instrument :
FID_G
ClientSampleId :
CB-D35