

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG063022\
Data File : FG010045.D
Signal(s) : FID1A.ch
Acq On : 30 Jun 2022 16:20
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 01 02:07:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.812	2346917	19.738 ug/ml
Target Compounds			


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG063022\
Data File : FG010045.D
Signal(s) : FID1A.ch
Acq On : 30 Jun 2022 16:20
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 01 02:07:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

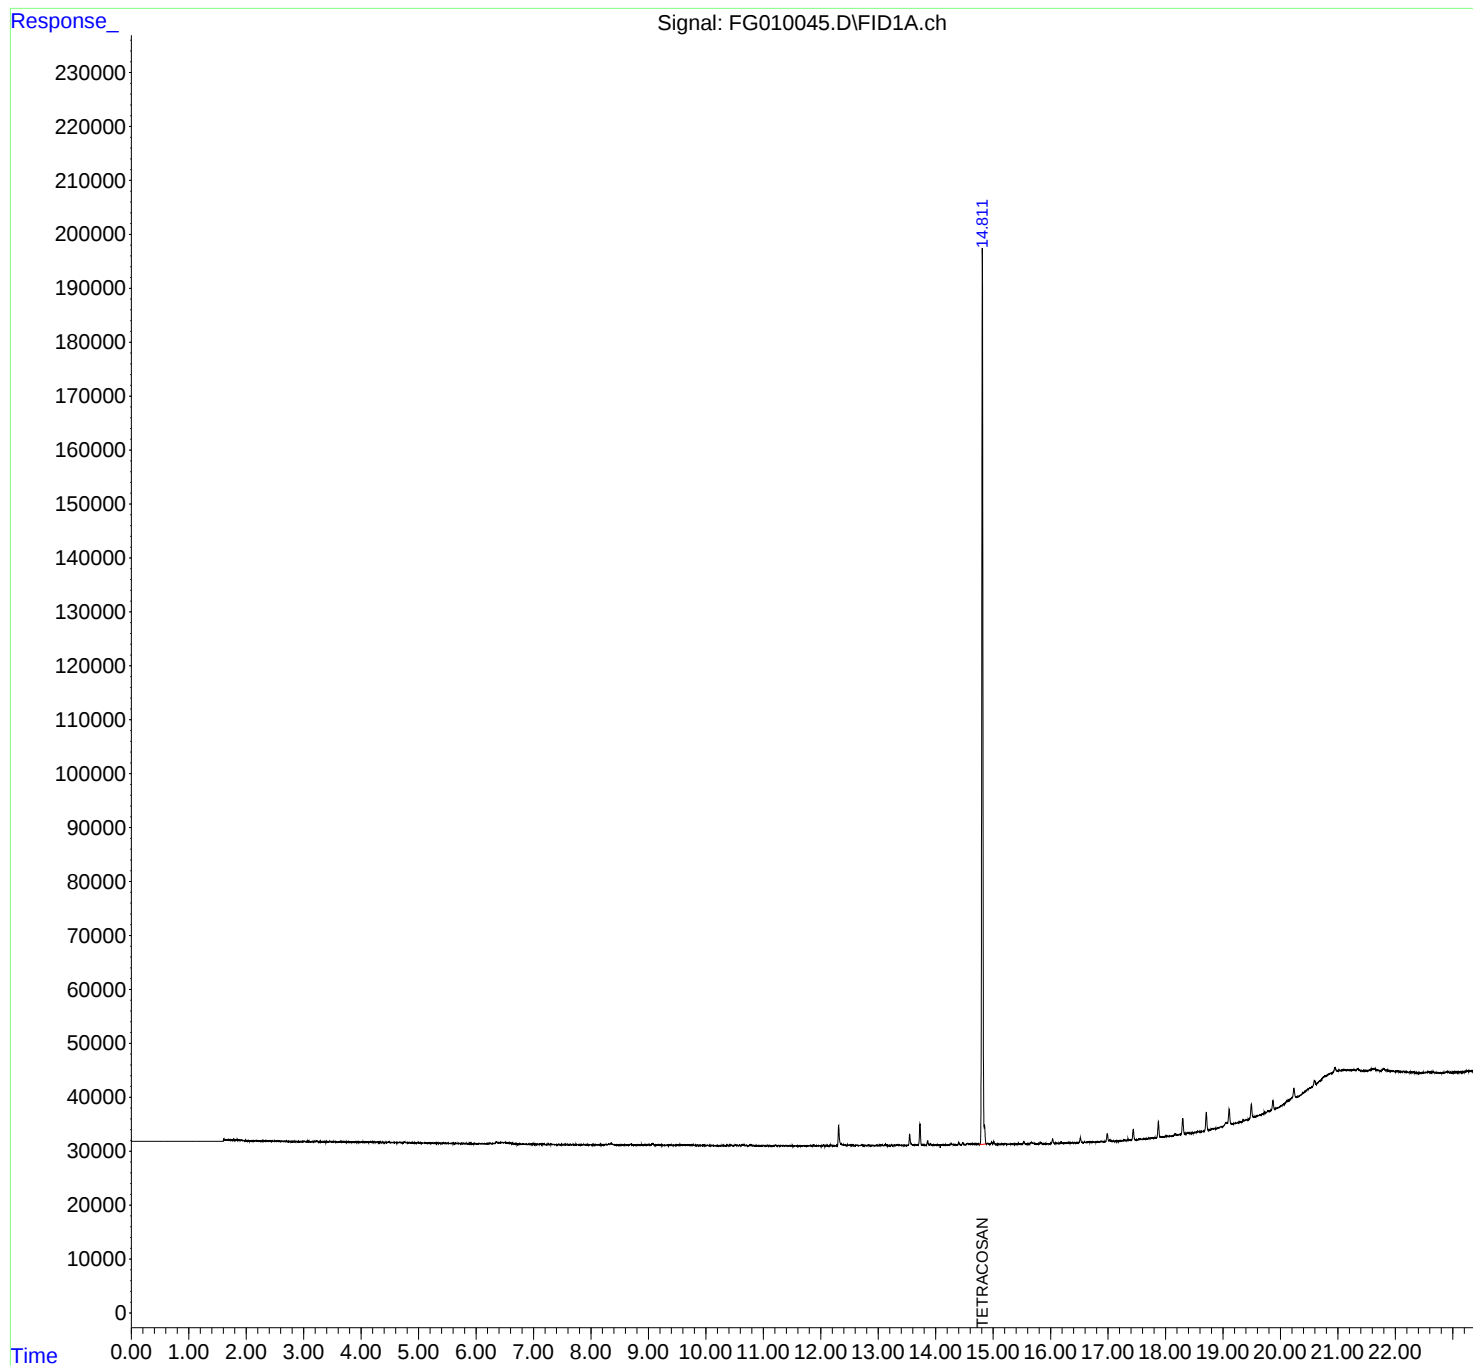

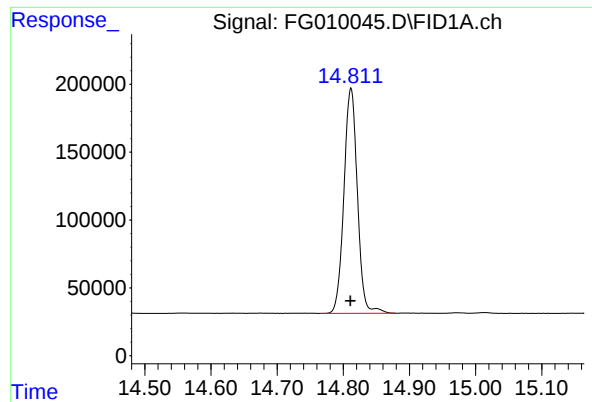

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.812 min
Delta R.T.: 0.000 min
Response: 2346917
Conc: 19.74 ug/ml