

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070119\
 Data File : FG005297.D
 Signal(s) : FID1A.ch
 Acq On : 02 Jul 2019 02:01
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Jul 02 05:57:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
 Quant Title :
 QLast Update : Mon Jun 10 08:32:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	1957381	14.851 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.962	34749	0.244 ug/ml
13) N-TRIACONTANE	17.851	59503	0.425 ug/ml
14) N-DOTRIACONTANE	18.684	64207	0.477 ug/ml
15) N-TETRATRIACONTANE	19.474	45188	0.352 ug/ml
17) N-OCTATRIACONTANE	20.978	50105	0.473 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070119\
Data File : FG005297.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2019 02:01
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jul 02 05:57:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

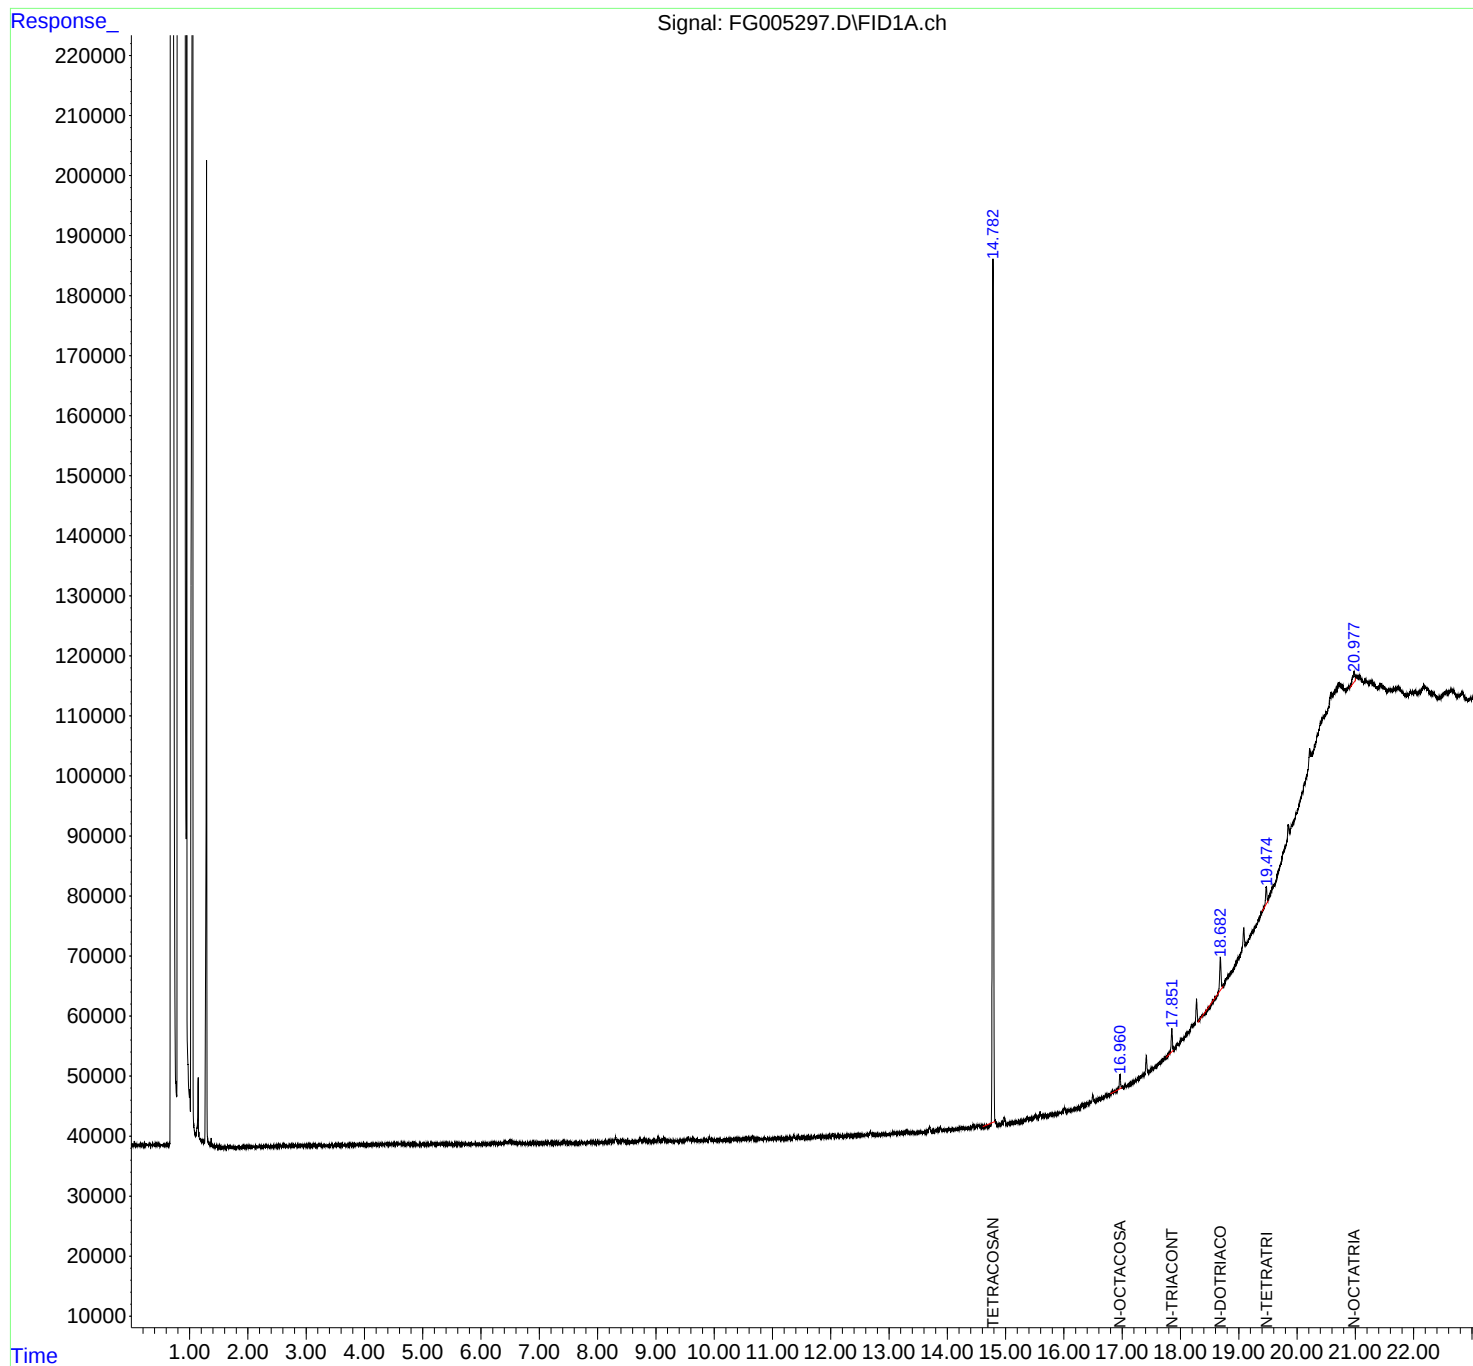


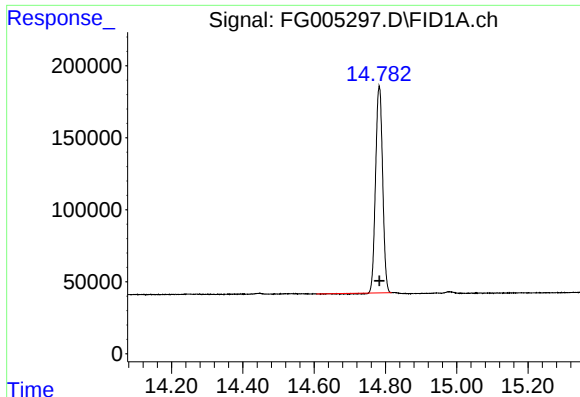

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.783 min
Delta R.T.: 0.000 min
Response: 1957381
Conc: 14.85 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK

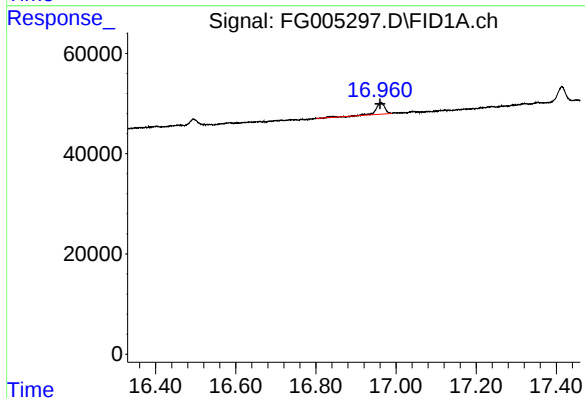


#12 N-OCTACOSANE

R.T.: 16.962 min
Delta R.T.: 0.002 min
Response: 34749
Conc: 0.24 ug/ml

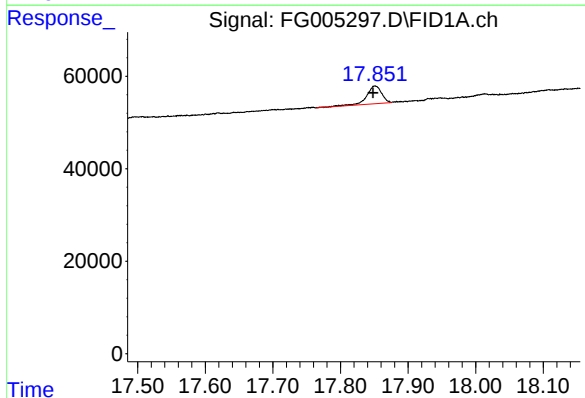


#13 N-TRIACONTANE

R.T.: 17.851 min
Delta R.T.: 0.003 min
Response: 59503
Conc: 0.43 ug/ml

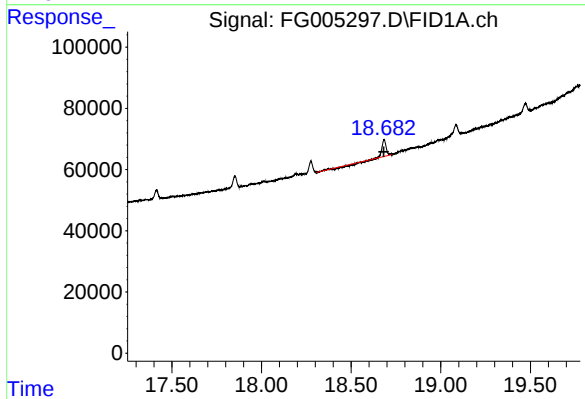

#14 N-DOTRIACONTANE


R.T.: 18.684 min
Delta R.T.: 0.002 min
Response: 64207
Conc: 0.48 ug/ml

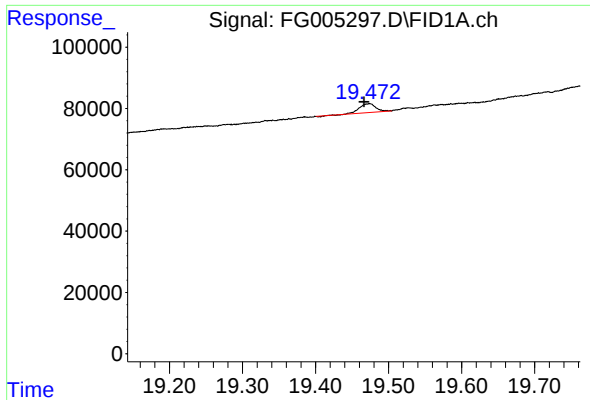

#15 N-TETRATRIACONTANE

R.T.: 19.474 min
Delta R.T.: 0.008 min
Response: 45188
Conc: 0.35 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK

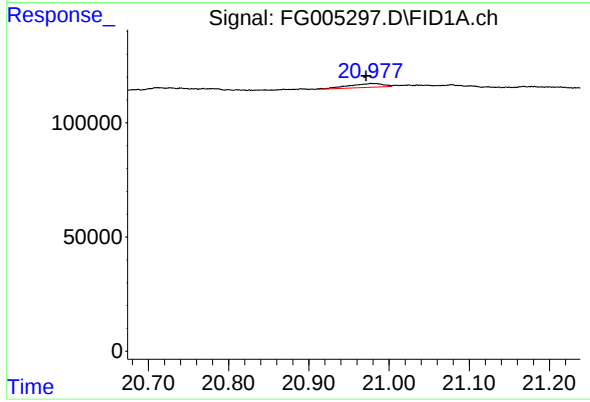

#17 N-OCTATRIACONTANE

R.T.: 20.978 min
Delta R.T.: 0.007 min
Response: 50105
Conc: 0.47 ug/ml