

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070119\
Data File : FG005301.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2019 03:59
Operator : DD\AJ
Sample : PB121047BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB121047BL

Integration File: autoint1.e
Quant Time: Jul 02 05:58:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.781	1990255	15.101 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.961	33450	0.235 ug/ml
13) N-TRIACONTANE	17.849	73644	0.526 ug/ml
14) N-DOTRIACONTANE	18.683	96750	0.719 ug/ml
15) N-TETRATRIACONTANE	19.470	72261	0.564 ug/ml
17) N-OCTATRIACONTANE	20.980	63216	0.596 ug/ml
18) N-TETRACONTANE	21.940	75319	0.721 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070119\
Data File : FG005301.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2019 03:59
Operator : DD\AJ
Sample : PB121047BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB121047BL

Integration File: autoint1.e
Quant Time: Jul 02 05:58:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

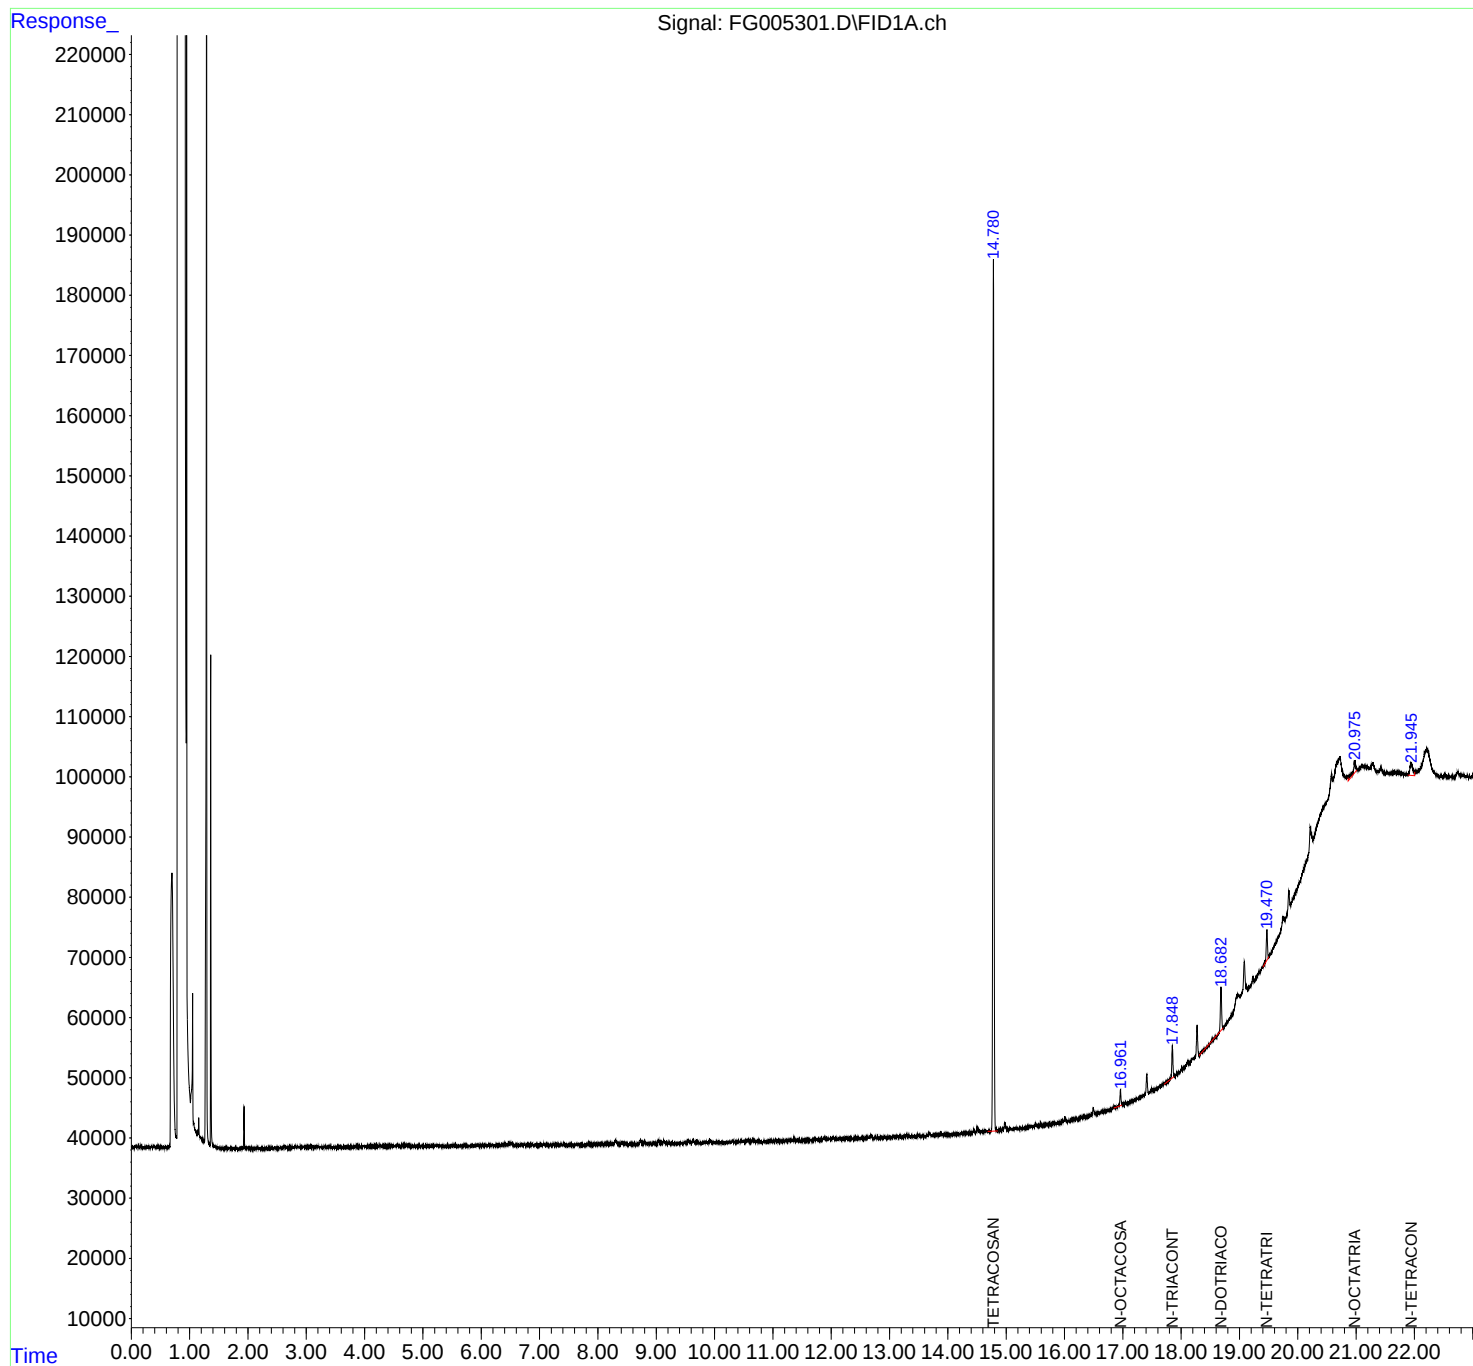


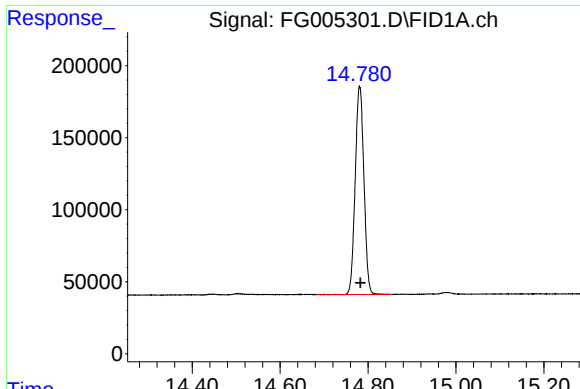

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.781 min
Delta R.T.: -0.002 min
Response: 1990255
Conc: 15.10 ug/ml

Instrument :
FID_G
ClientSampleId :
PB121047BL

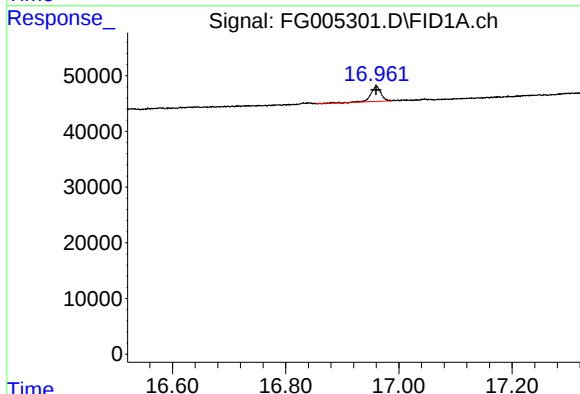


#12 N-OCTACOSANE

R.T.: 16.961 min
Delta R.T.: 0.000 min
Response: 33450
Conc: 0.24 ug/ml

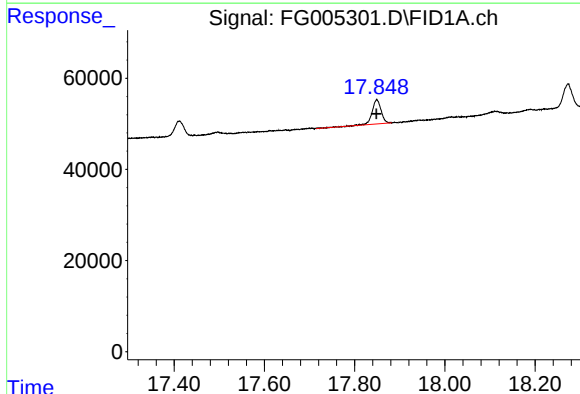


#13 N-TRIACONTANE

R.T.: 17.849 min
Delta R.T.: 0.000 min
Response: 73644
Conc: 0.53 ug/ml

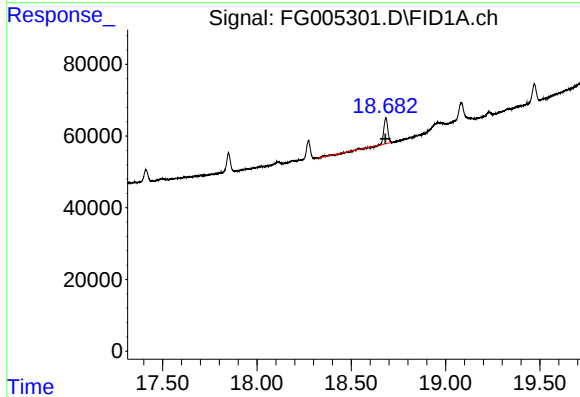

#14 N-DOTRIACONTANE


R.T.: 18.683 min
Delta R.T.: 0.002 min
Response: 96750
Conc: 0.72 ug/ml

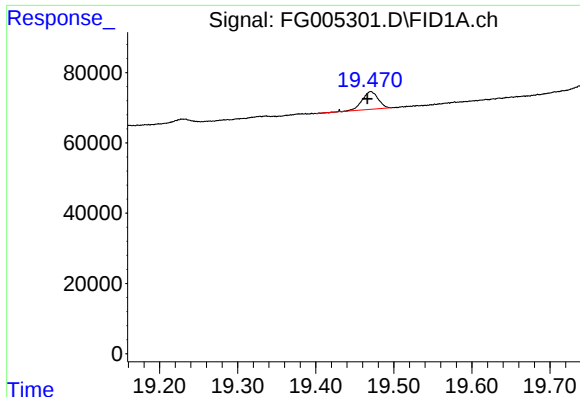

#15 N-TETRATRIACONTANE


R.T.: 19.470 min
Delta R.T.: 0.004 min
Response: 72261
Conc: 0.56 ug/ml

Instrument :
FID_G
ClientSampleId :
PB121047BL

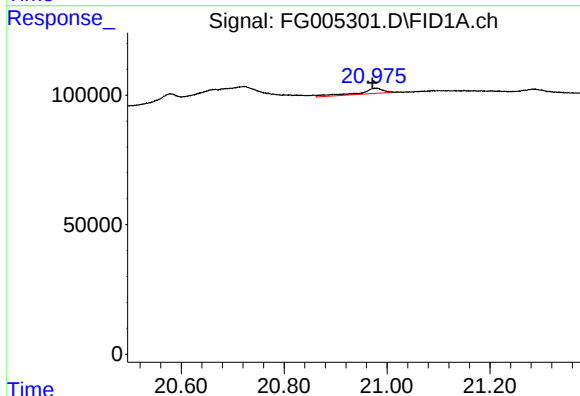

#17 N-OCTATRIACONTANE

R.T.: 20.980 min
Delta R.T.: 0.008 min
Response: 63216
Conc: 0.60 ug/ml

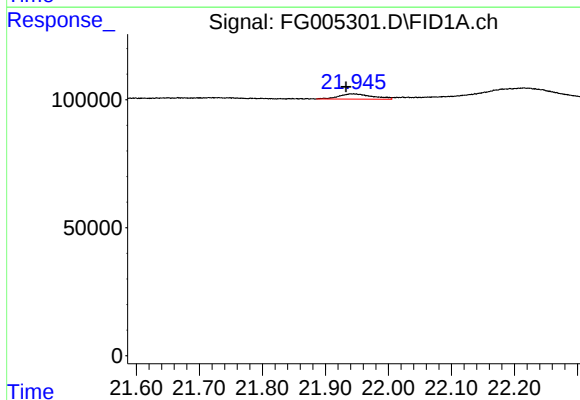

#18 N-TETRACONTANE

R.T.: 21.940 min
Delta R.T.: 0.007 min
Response: 75319
Conc: 0.72 ug/ml