

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070119\
 Data File : FG005288.D
 Signal(s) : FID1A.ch
 Acq On : 01 Jul 2019 21:35
 Operator : DD\AJ
 Sample : PB121045BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 PB121045BS

Integration File: autoint1.e
 Quant Time: Jul 02 01:20:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
 Quant Title :
 QLast Update : Mon Jun 10 08:32:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.785	1963249	14.896 ug/ml
Target Compounds			
2) N-DECANE	4.477	2457380	16.976 ug/ml
3) N-DODECANE	6.509	2475789	16.661 ug/ml
4) N-TETRADECANE	8.312	2437041	16.254 ug/ml
5) N-HEXADECANE	9.920	2399159	15.772 ug/ml
6) N-OCTADECANE	11.367	2365133	15.646 ug/ml
7) N-EICOSANE	12.681	2336146	15.332 ug/ml
8) N-DOCOSANE	13.883	2290385	15.208 ug/ml
10) N-TETRACOSANE	14.989	2288947	15.383 ug/ml
11) N-HEXACOSANE	16.014	2237040	15.358 ug/ml
12) N-OCTACOSANE	16.966	2271276	15.968 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070119\
Data File : FG005288.D
Signal(s) : FID1A.ch
Acq On : 01 Jul 2019 21:35
Operator : DD\AJ
Sample : PB121045BS
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB121045BS

Integration File: autoint1.e
Quant Time: Jul 02 01:20:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

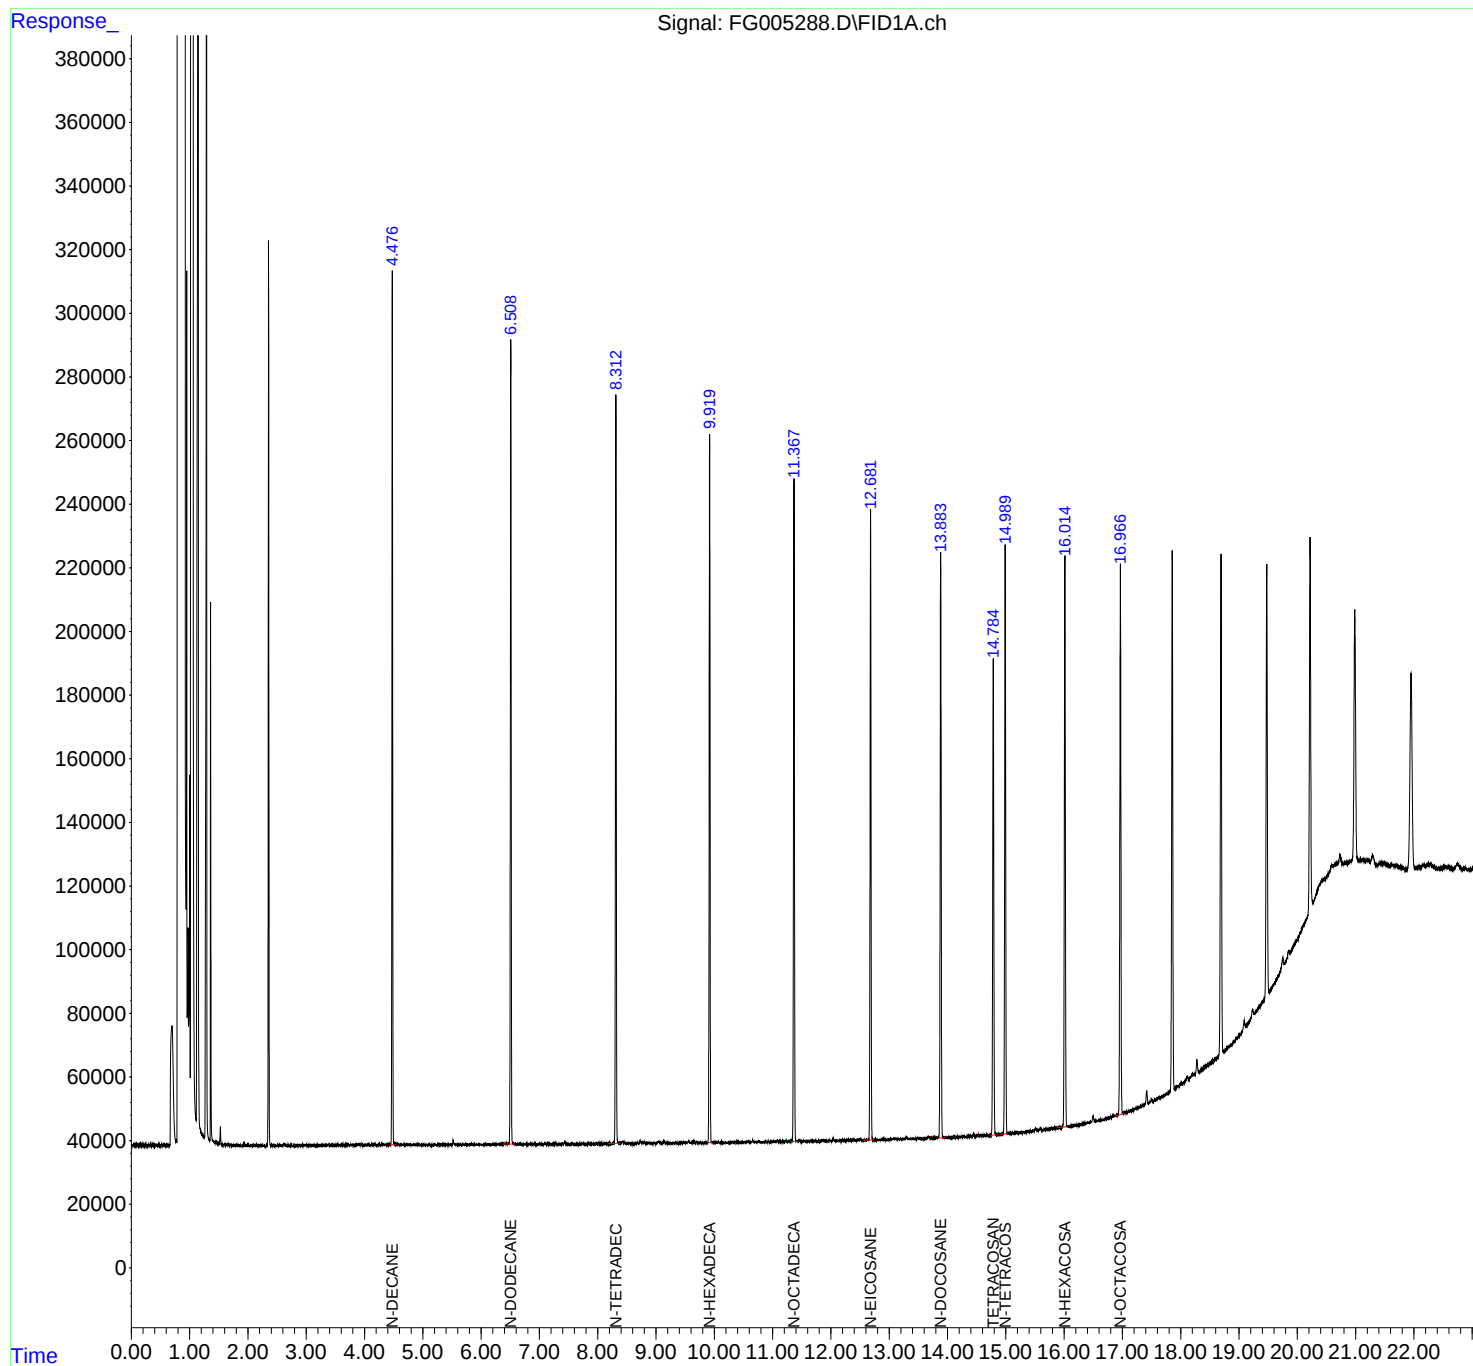


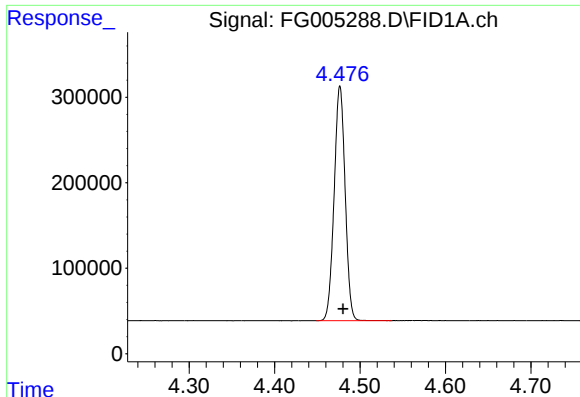

#2 N-DECANE


R.T.: 4.477 min
Delta R.T.: -0.004 min
Response: 2457380
Conc: 16.98 ug/ml

Instrument :
FID_G
ClientSampleId :
PB121045BS

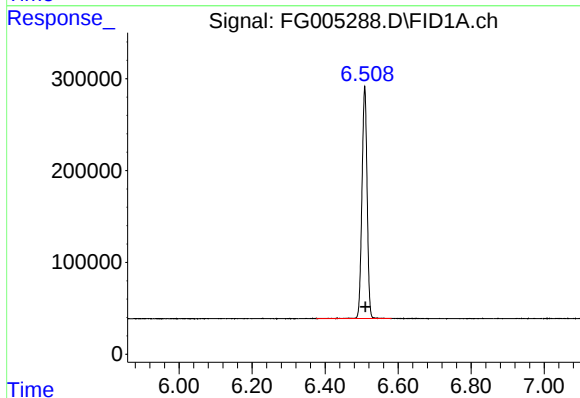


#3 N-DODECANE

R.T.: 6.509 min
Delta R.T.: -0.002 min
Response: 2475789
Conc: 16.66 ug/ml

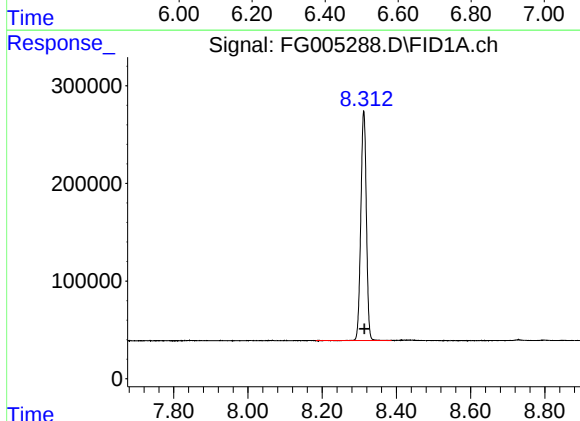


#4 N-TETRADECANE

R.T.: 8.312 min
Delta R.T.: -0.002 min
Response: 2437041
Conc: 16.25 ug/ml

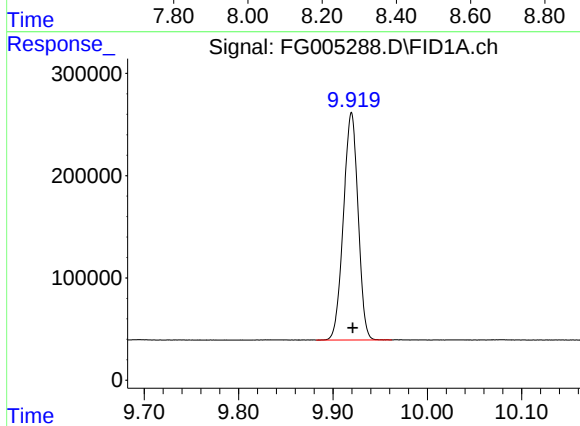

#5 N-HEXADECANE


R.T.: 9.920 min
Delta R.T.: -0.001 min
Response: 2399159
Conc: 15.77 ug/ml

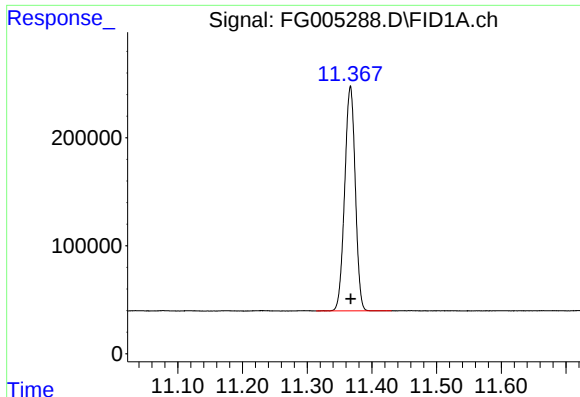

#6 N-OCTADECANE


R.T.: 11.367 min
Delta R.T.: 0.000 min
Response: 2365133
Conc: 15.65 ug/ml

Instrument :
FID_G
ClientSampleId :
PB121045BS

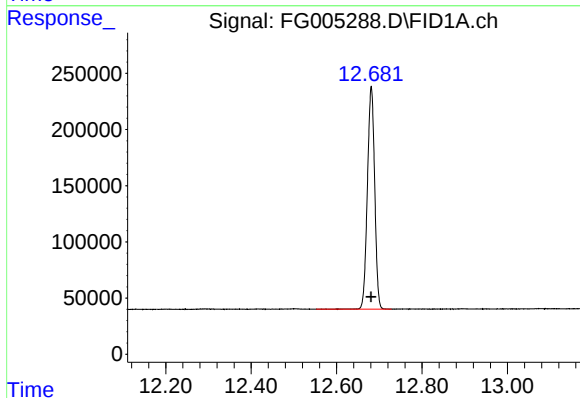


#7 N-EICOSANE

R.T.: 12.681 min
Delta R.T.: 0.000 min
Response: 2336146
Conc: 15.33 ug/ml

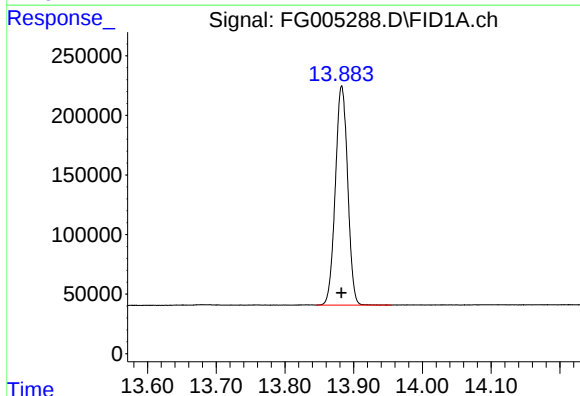


#8 N-DOCOSANE

R.T.: 13.883 min
Delta R.T.: 0.000 min
Response: 2290385
Conc: 15.21 ug/ml

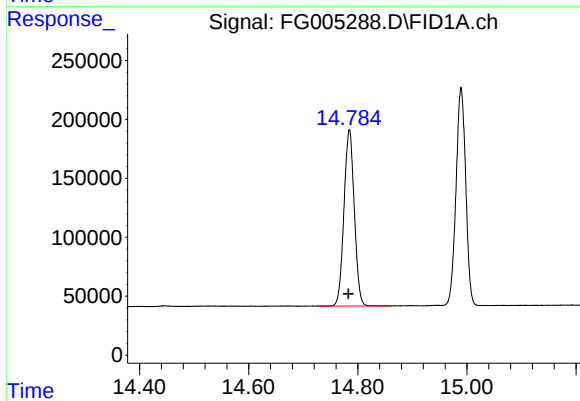

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.785 min
Delta R.T.: 0.002 min
Response: 1963249
Conc: 14.90 ug/ml

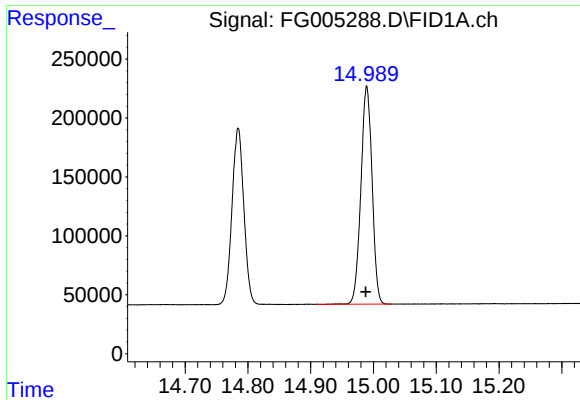

#10 N-TETRACOSANE


R.T.: 14.989 min
Delta R.T.: 0.001 min
Response: 2288947
Conc: 15.38 ug/ml

Instrument :
FID_G
ClientSampleId :
PB121045BS

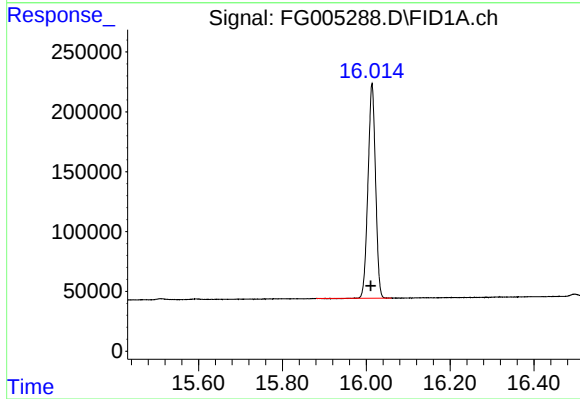

#11 N-HEXACOSANE

R.T.: 16.014 min
Delta R.T.: 0.003 min
Response: 2237040
Conc: 15.36 ug/ml

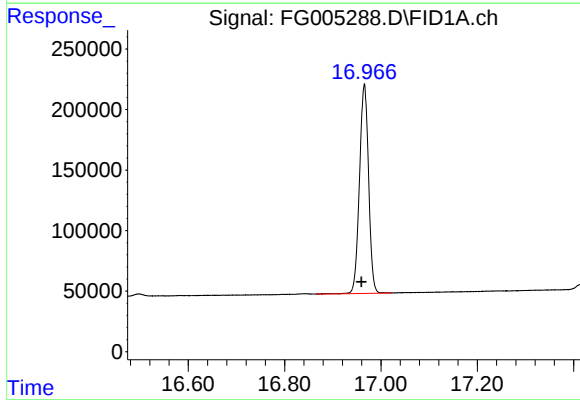

#12 N-OCTACOSANE

R.T.: 16.966 min
Delta R.T.: 0.006 min
Response: 2271276
Conc: 15.97 ug/ml