

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070119\
Data File : FG005307.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2019 06:55
Operator : DD\AJ
Sample : K3163-15 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SU-01-062719-B

Integration File: autoint1.e
Quant Time: Jul 02 08:14:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.781	160019	1.214 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070119\
Data File : FG005307.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2019 06:55
Operator : DD\AJ
Sample : K3163-15 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SU-01-062719-B

Integration File: autoint1.e
Quant Time: Jul 02 08:14:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

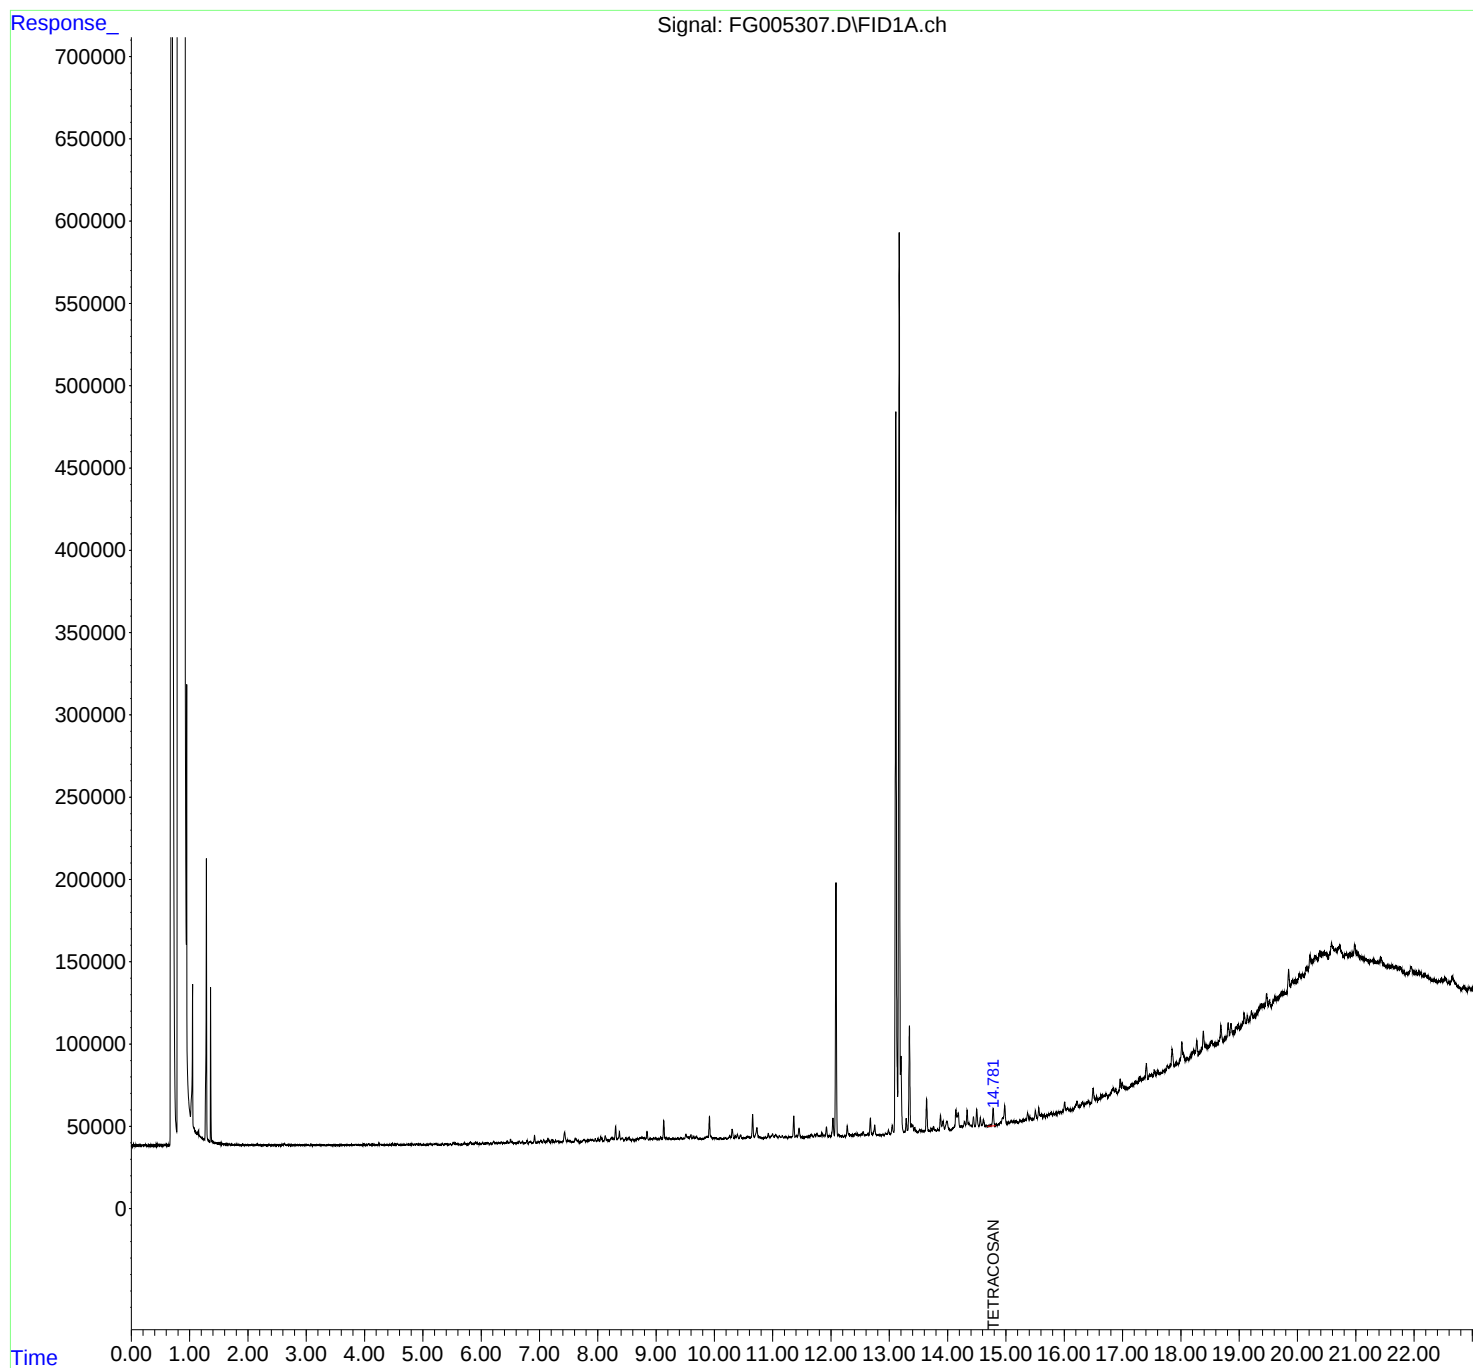

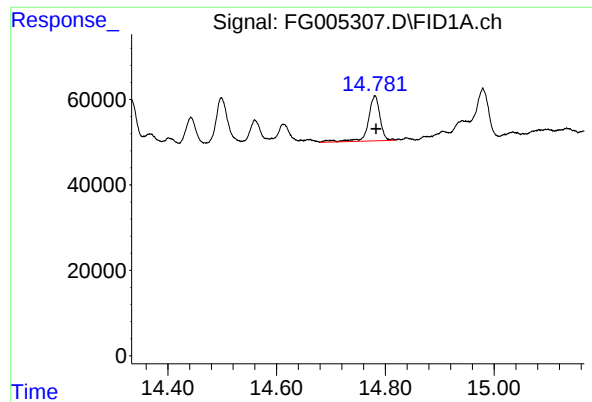

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.781 min
Delta R.T.: -0.002 min
Response: 160019
Conc: 1.21 ug/ml

Instrument :
FID_G
ClientSampleId :
SU-01-062719-B