

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070119\
Data File : FG005317.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2019 12:04
Operator : DD\AJ
Sample : K3606-02 5X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
HJDC-COMP-1

Integration File: autoint1.e
Quant Time: Jul 02 12:25:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.786	377775	2.866 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070119\
Data File : FG005317.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2019 12:04
Operator : DD\AJ
Sample : K3606-02 5X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
HJDC-COMP-1

Integration File: autoint1.e
Quant Time: Jul 02 12:25:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

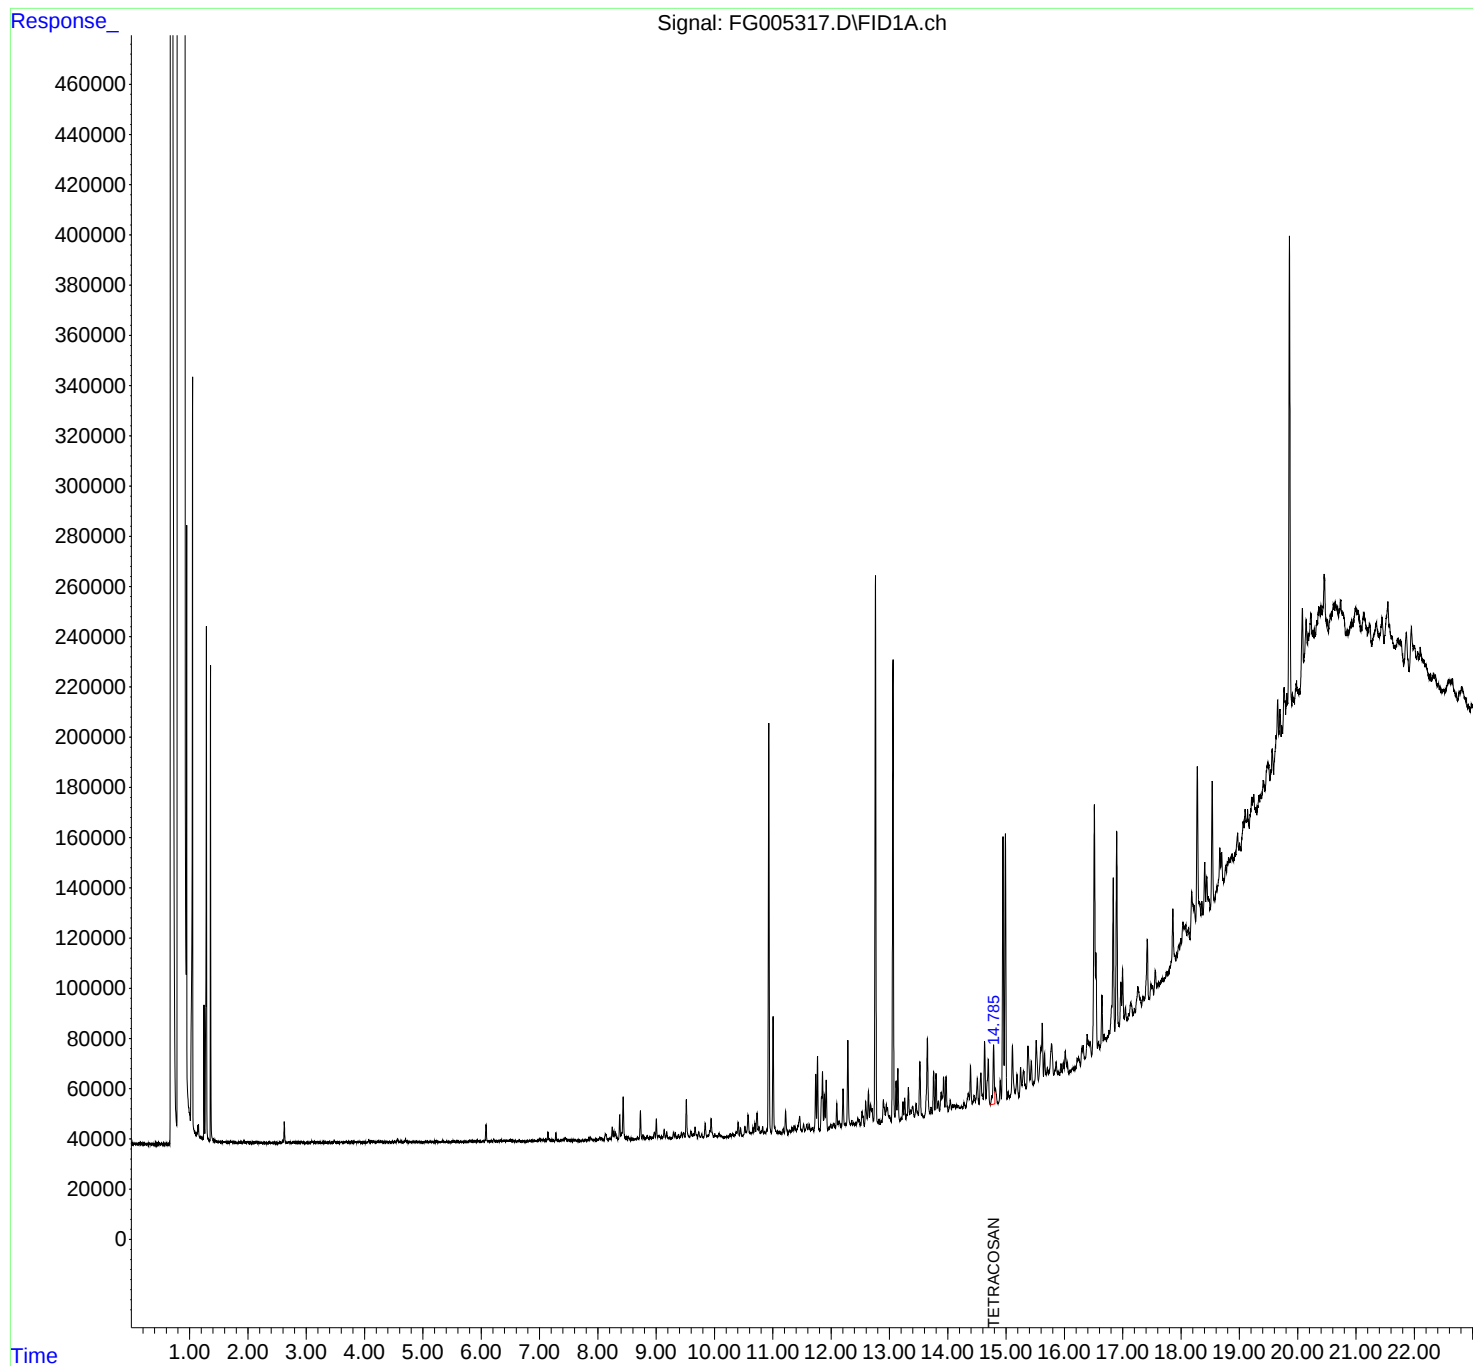

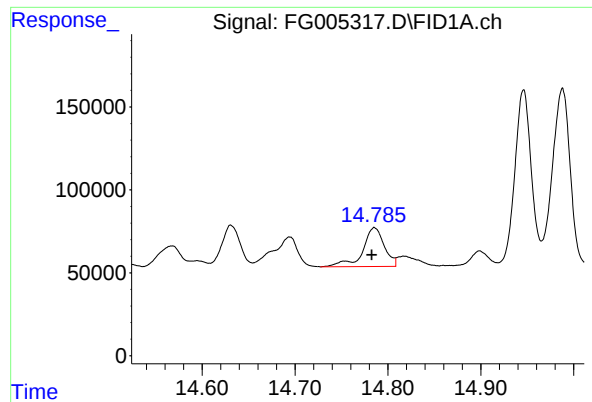

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.786 min
Delta R.T.: 0.003 min
Response: 377775
Conc: 2.87 ug/ml

Instrument :
FID_G
ClientSampleId :
HJDC-COMP-1