

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070122\
Data File : FG010053.D
Signal(s) : FID1A.ch
Acq On : 01 Jul 2022 13:39
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 01:46:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.812	2778142	23.364 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.710	103568	0.876 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070122\
Data File : FG010053.D
Signal(s) : FID1A.ch
Acq On : 01 Jul 2022 13:39
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 01:46:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

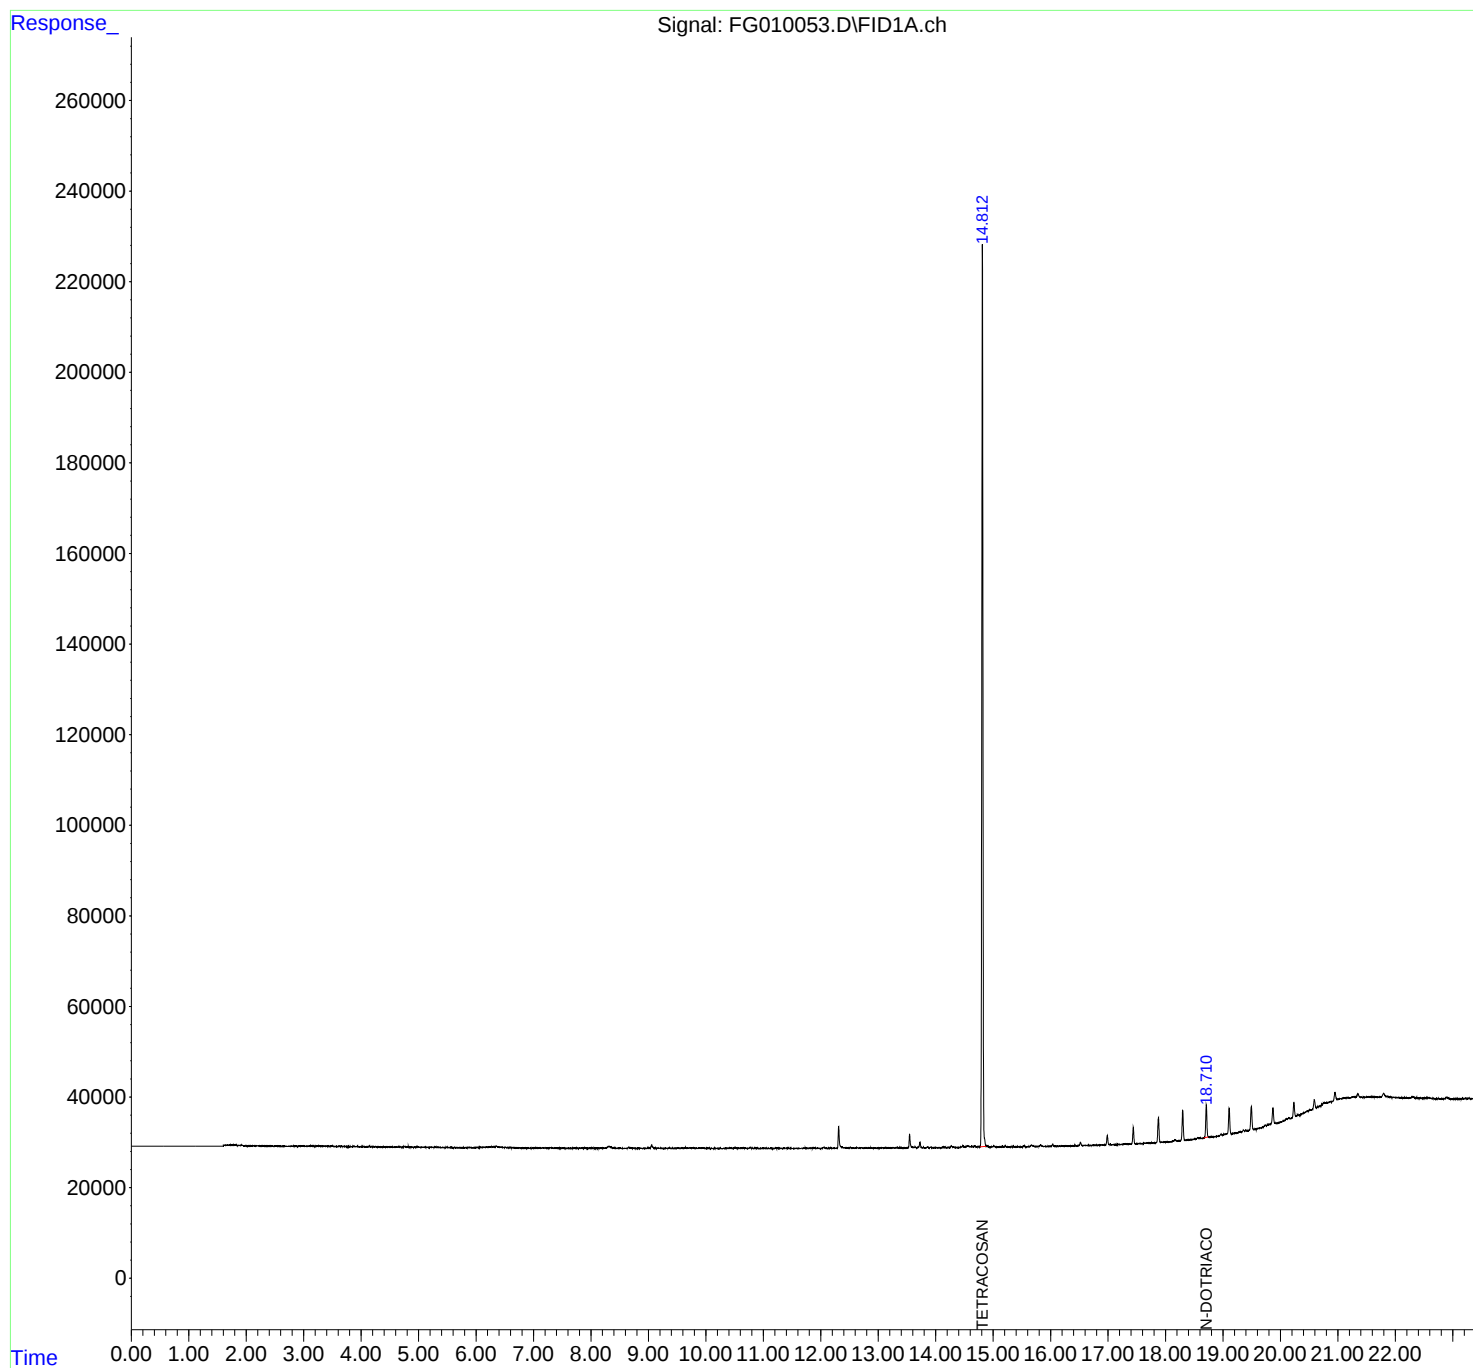


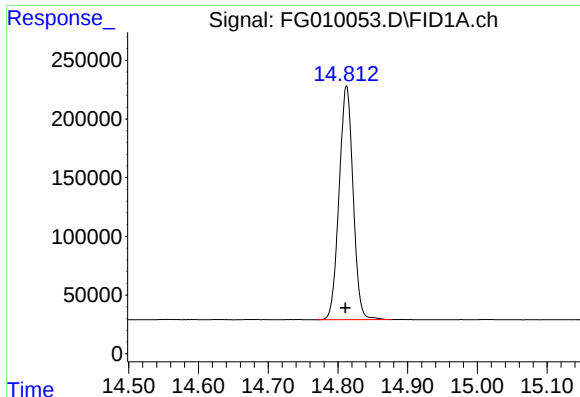

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.812 min
Delta R.T.: 0.002 min
Response: 2778142
Conc: 23.36 ug/ml

Instrument :
FID_G
ClientSampleId :

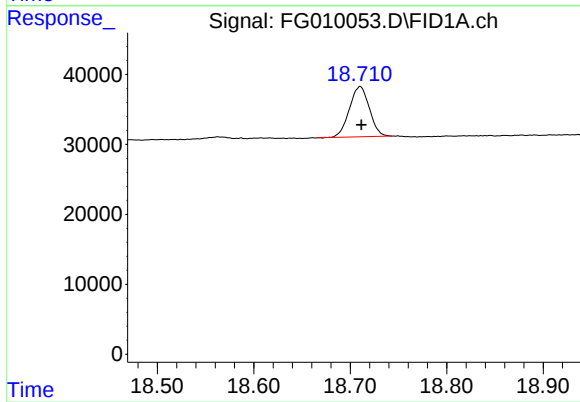

#14 N-DOTRIACONTANE

R.T.: 18.710 min
Delta R.T.: -0.001 min
Response: 103568
Conc: 0.88 ug/ml