

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070122\
Data File : FG010068.D
Signal(s) : FID1A.ch
Acq On : 01 Jul 2022 23:48
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/05/2022
Supervised By :Ankita Jodhani 07/05/2022

Integration File: autoint1.e
Quant Time: Jul 02 01:49:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.810	1919941	16.147 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070122\
Data File : FG010068.D
Signal(s) : FID1A.ch
Acq On : 01 Jul 2022 23:48
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/05/2022
Supervised By :Ankita Jodhani 07/05/2022

Integration File: autoint1.e
Quant Time: Jul 02 01:49:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG062922.M
Quant Title :
QLast Update : Thu Jun 30 04:15:08 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

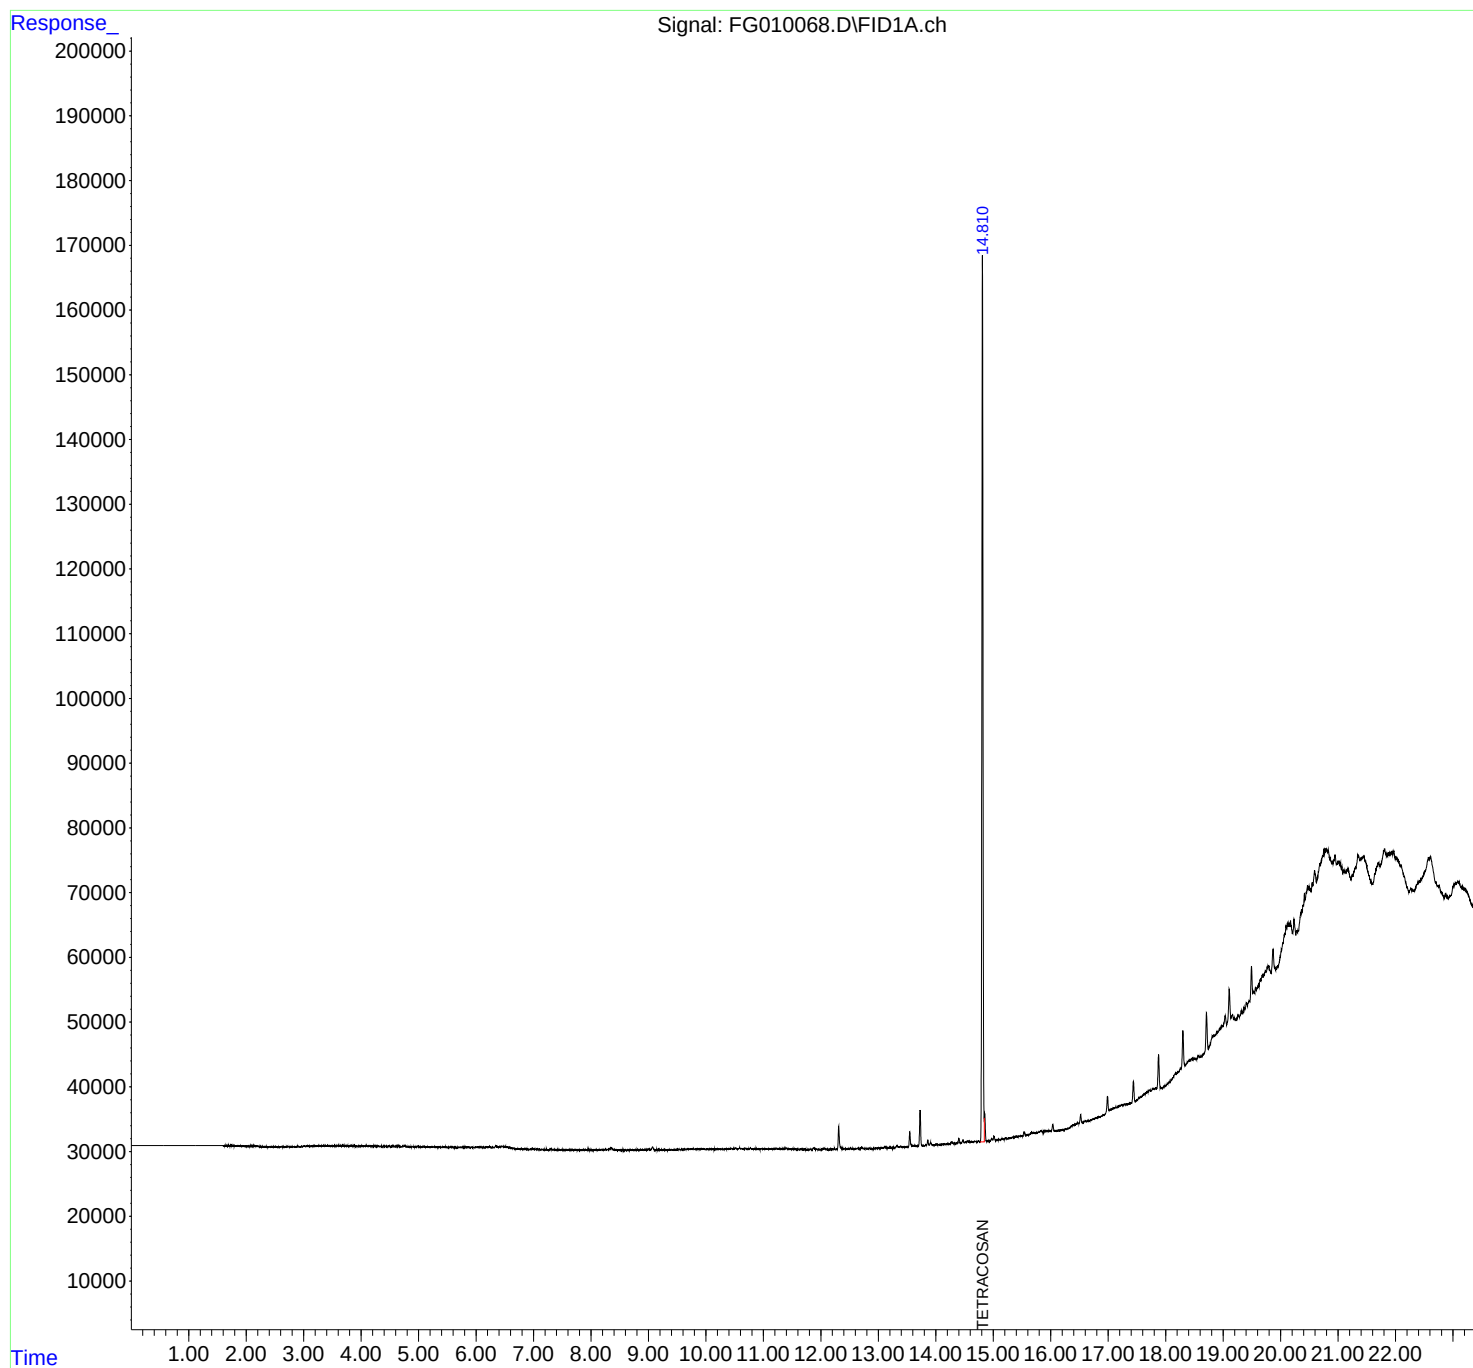

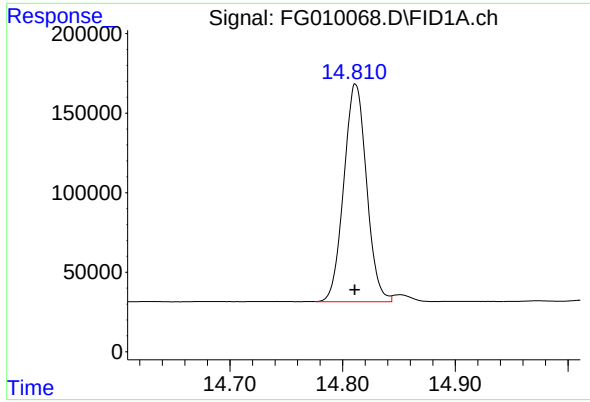

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.810 min
Delta R.T.: 0.000 min
Response: 1919941
Conc: 16.15 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/05/2022
Supervised By :Ankita Jodhani 07/05/2022