

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070218\
 Data File : FG001555.D
 Signal(s) : FID1A.ch
 Acq On : 02 Jul 2018 18:21
 Operator : UA\AJ
 Sample : J3790-01 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 01:01:02 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
 Quant Title :
 QLast Update : Mon Jul 02 14:11:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.523	522734	4.493 ug/ml
Target Compounds			
4) N-TETRADECANE	8.131f	133654	1.010 ug/ml
7) N-EICOSANE	12.467	960063	7.192 ug/ml
10) N-TETRACOSANE	14.687	396890	3.002 ug/ml
11) N-HEXACOSANE	15.749	216931	1.648 ug/ml
12) N-OCTACOSANE	16.701	378660	2.896 ug/ml
13) N-TRIACONTANE	17.587	416708	3.198 ug/ml
14) N-DOTRIACONTANE	18.421	405876	3.189 ug/ml
15) N-TETRATRIACONTANE	19.215	348897	2.772 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070218\
Data File : FG001555.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2018 18:21
Operator : UA\AJ
Sample : J3790-01 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 01:01:02 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

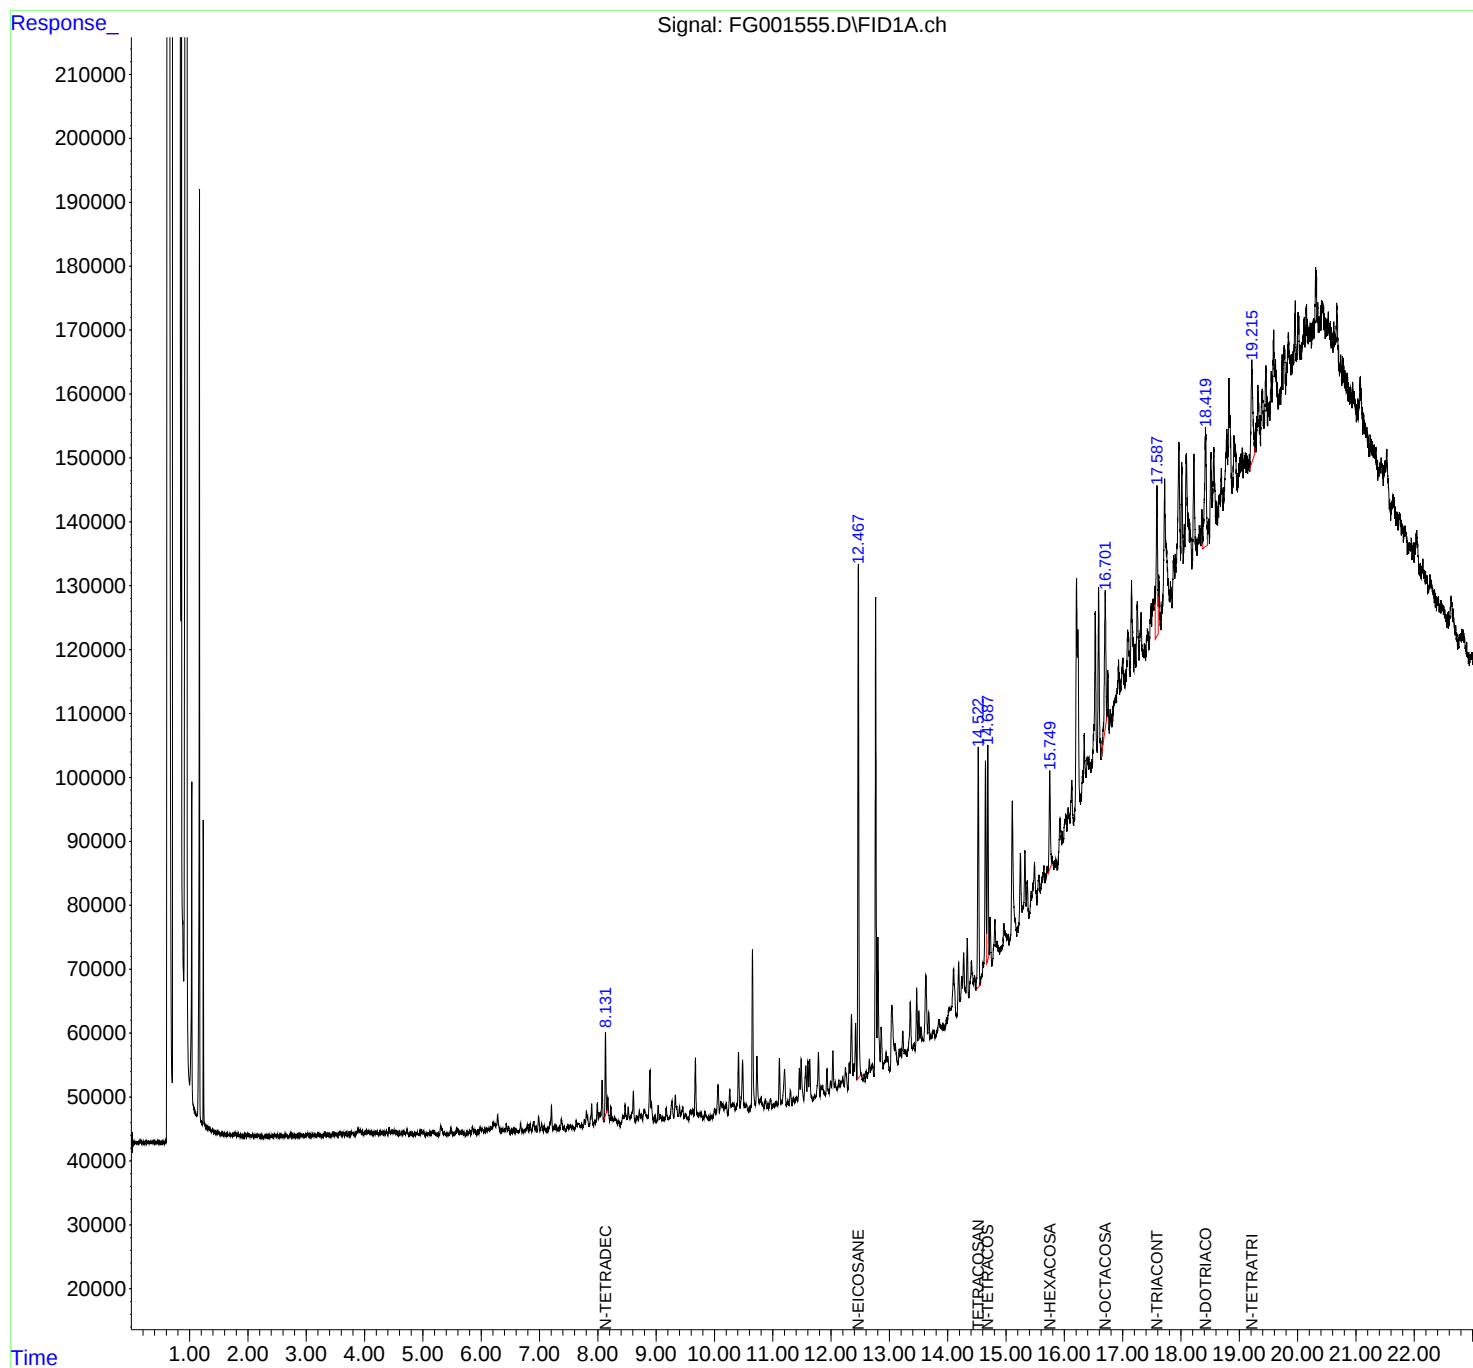


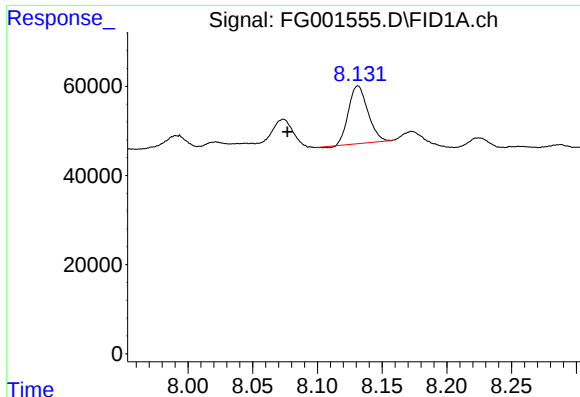

#4 N-TETRADECANE


R.T.: 8.131 min
Delta R.T.: 0.055 min
Response: 133654
Conc: 1.01 ug/ml

Instrument :
FID_G
ClientSampleId :

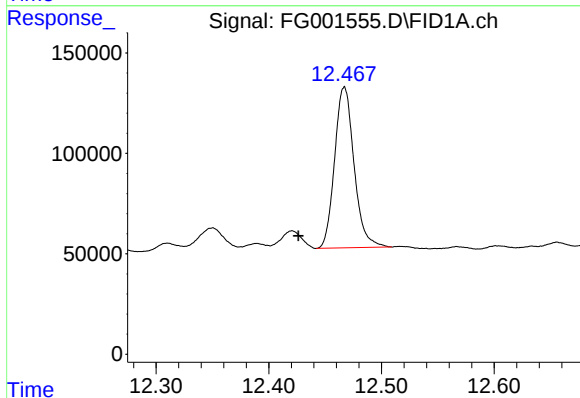


#7 N-EICOSANE

R.T.: 12.467 min
Delta R.T.: 0.041 min
Response: 960063
Conc: 7.19 ug/ml

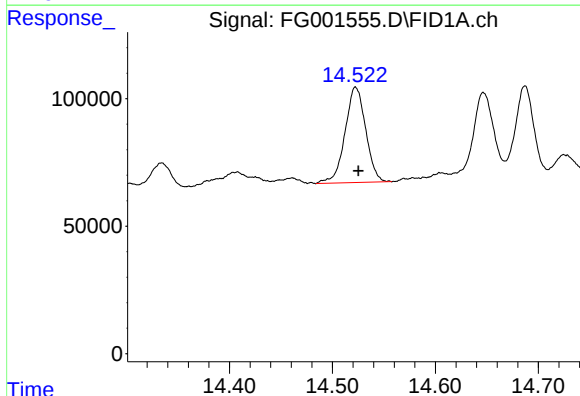


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.523 min
Delta R.T.: -0.003 min
Response: 522734
Conc: 4.49 ug/ml

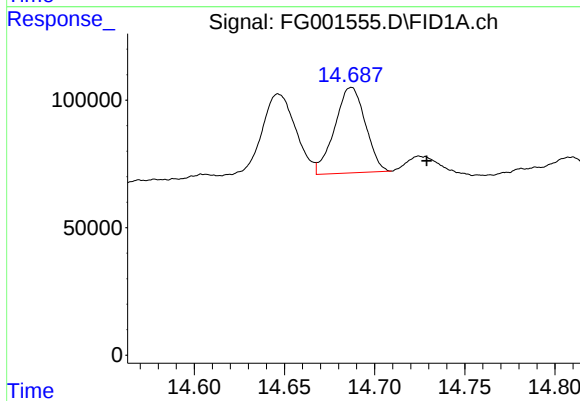

#10 N-TETRACOSANE


R.T.: 14.687 min
Delta R.T.: -0.042 min
Response: 396890
Conc: 3.00 ug/ml

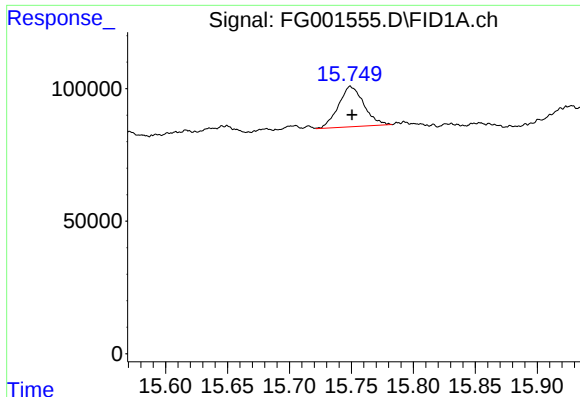

#11 N-HEXACOSANE


R.T.: 15.749 min
Delta R.T.: -0.001 min
Response: 216931
Conc: 1.65 ug/ml

Instrument :
FID_G
ClientSampleId :

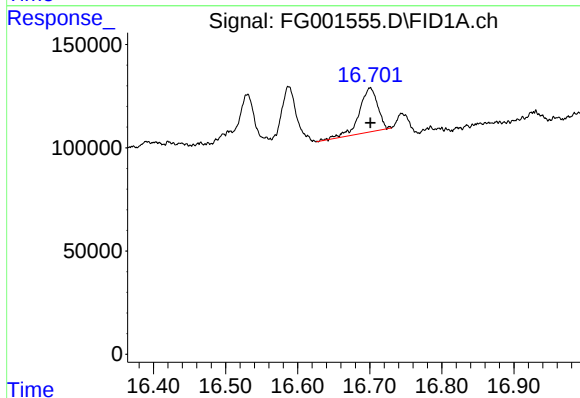


#12 N-OCTACOSANE

R.T.: 16.701 min
Delta R.T.: 0.000 min
Response: 378660
Conc: 2.90 ug/ml

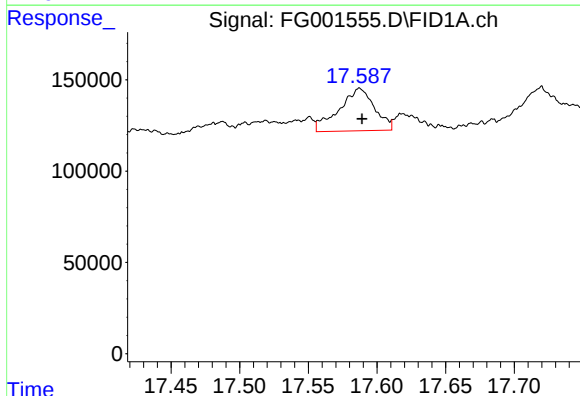


#13 N-TRIACONTANE

R.T.: 17.587 min
Delta R.T.: -0.002 min
Response: 416708
Conc: 3.20 ug/ml

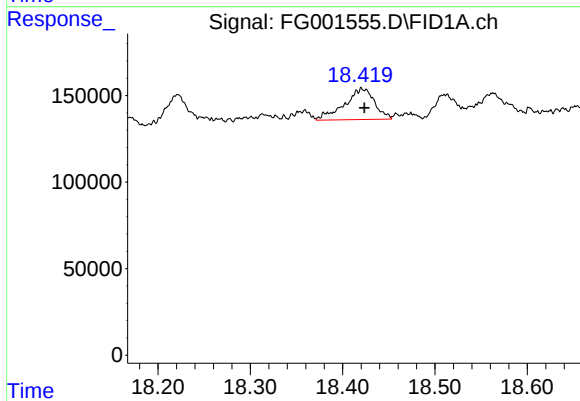

#14 N-DOTRIACONTANE

R.T.: 18.421 min
Delta R.T.: -0.003 min
Response: 405876
Conc: 3.19 ug/ml

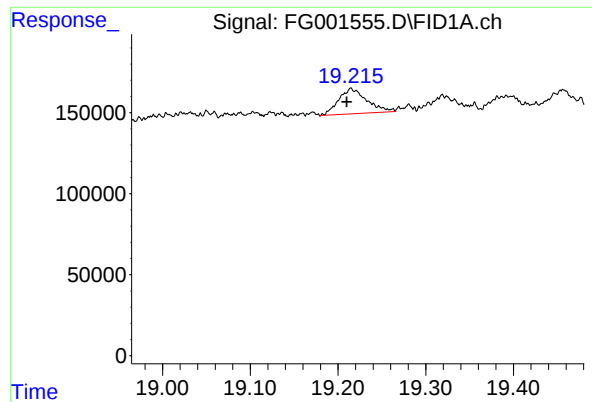

#15 N-TETRATRIACONTANE

R.T.: 19.215 min
Delta R.T.: 0.005 min
Response: 348897
Conc: 2.77 ug/ml

Instrument :
FID_G
ClientSampleId :