

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070218\
 Data File : FG001557.D
 Signal(s) : FID1A.ch
 Acq On : 02 Jul 2018 19:23
 Operator : UA\AJ
 Sample : J3749-02 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 01:01:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
 Quant Title :
 QLast Update : Mon Jul 02 14:11:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.526	563711	4.845 ug/ml
Target Compounds			
4) N-TETRADECANE	8.132f	162575	1.229 ug/ml
7) N-EICOSANE	12.472	1611881	12.075 ug/ml
8) N-DOCOSANE	13.638	197313	1.483 ug/ml
10) N-TETRACOSANE	14.693	1285593	9.724 ug/ml
12) N-OCTACOSANE	16.697	474708	3.631 ug/ml
13) N-TRIACONTANE	17.590	316541	2.430 ug/ml
14) N-DOTRIACONTANE	18.358f	268727	2.111 ug/ml
15) N-TETRATRIACONTANE	19.217	322079	2.559 ug/ml
16) N-HEXATRIACONTANE	19.916	110585	0.921 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070218\
Data File : FG001557.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2018 19:23
Operator : UA\AJ
Sample : J3749-02 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 01:01:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

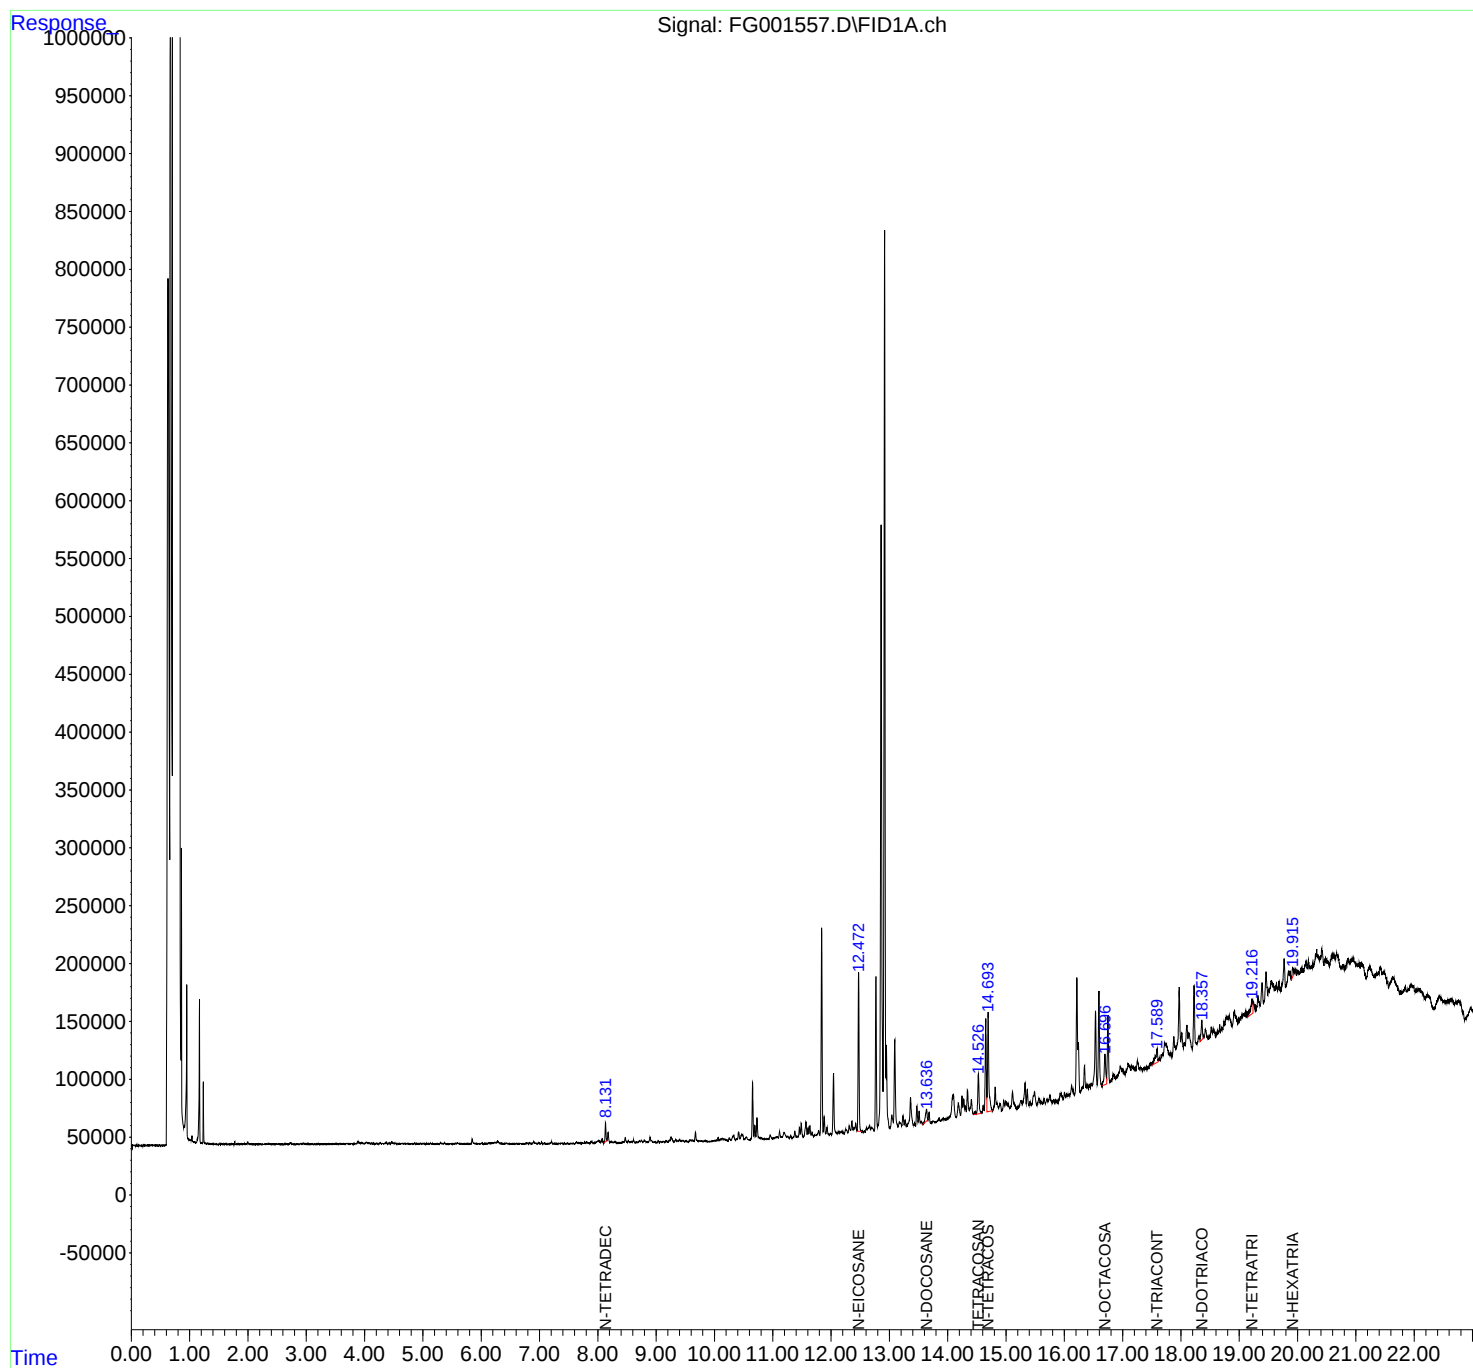


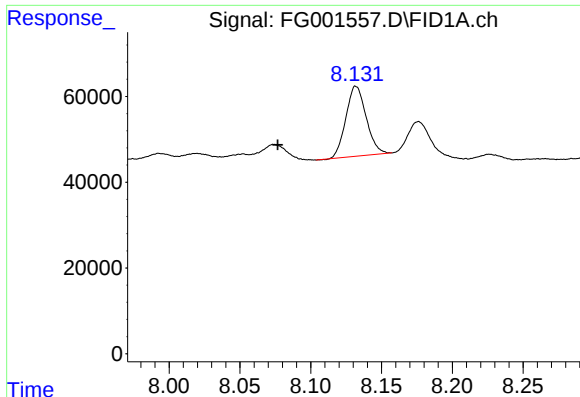

#4 N-TETRADECANE


R.T.: 8.132 min
Delta R.T.: 0.055 min
Response: 162575
Conc: 1.23 ug/ml

Instrument :
FID_G
ClientSampleId :

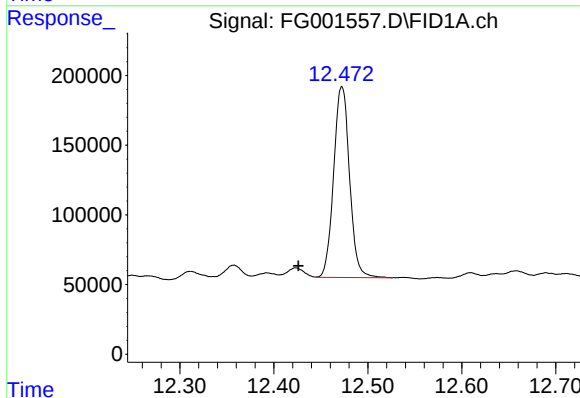


#7 N-EICOSANE

R.T.: 12.472 min
Delta R.T.: 0.046 min
Response: 1611881
Conc: 12.08 ug/ml

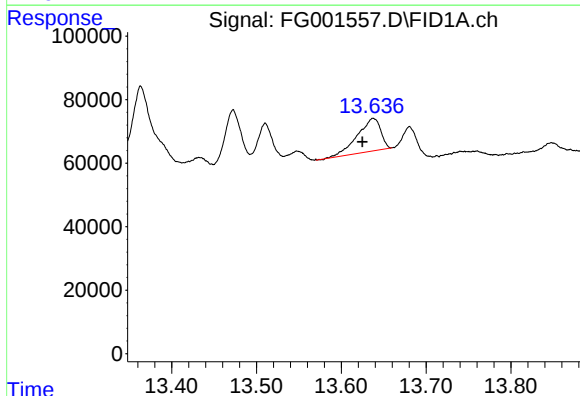


#8 N-DOCOSANE

R.T.: 13.638 min
Delta R.T.: 0.013 min
Response: 197313
Conc: 1.48 ug/ml

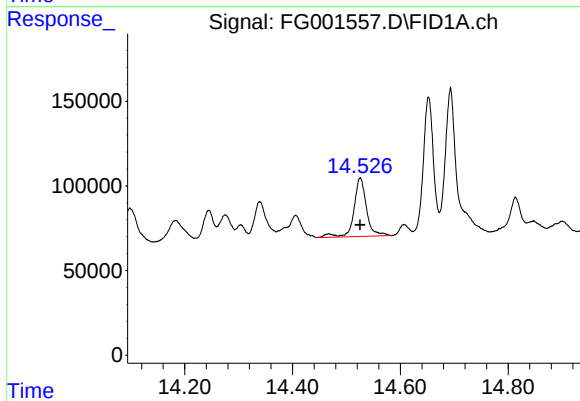

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.526 min
Delta R.T.: 0.000 min
Response: 563711
Conc: 4.85 ug/ml

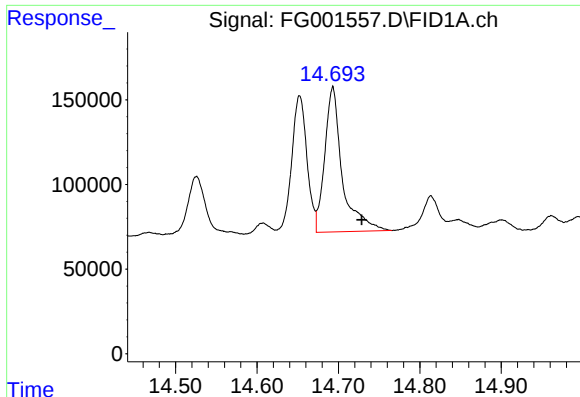

#10 N-TETRACOSANE


R.T.: 14.693 min
Delta R.T.: -0.036 min
Response: 1285593
Conc: 9.72 ug/ml

Instrument :
FID_G
ClientSampleId :

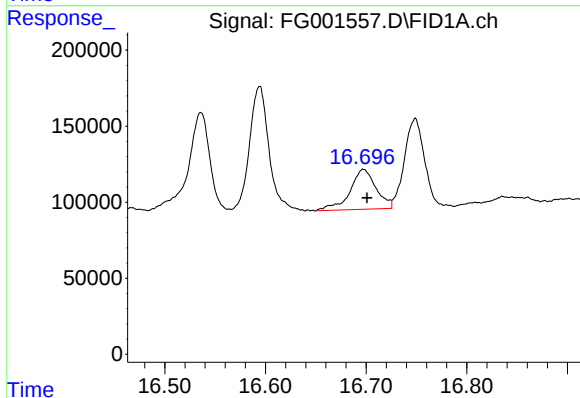


#12 N-OCTACOSANE

R.T.: 16.697 min
Delta R.T.: -0.003 min
Response: 474708
Conc: 3.63 ug/ml

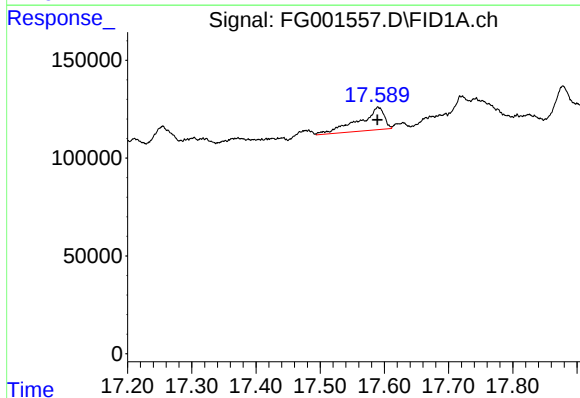


#13 N-TRIACONTANE

R.T.: 17.590 min
Delta R.T.: 0.000 min
Response: 316541
Conc: 2.43 ug/ml

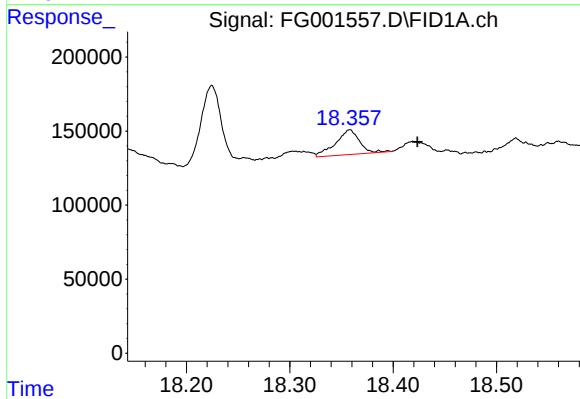

#14 N-DOTRIACONTANE


R.T.: 18.358 min
Delta R.T.: -0.066 min
Response: 268727
Conc: 2.11 ug/ml

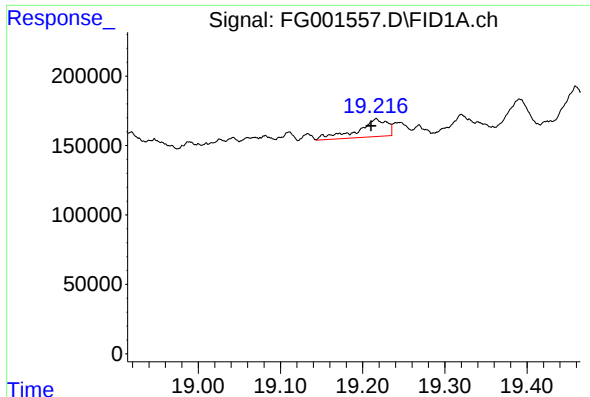

#15 N-TETRATRIACONTANE

R.T.: 19.217 min
Delta R.T.: 0.006 min
Response: 322079
Conc: 2.56 ug/ml

Instrument :
FID_G
ClientSampleId :

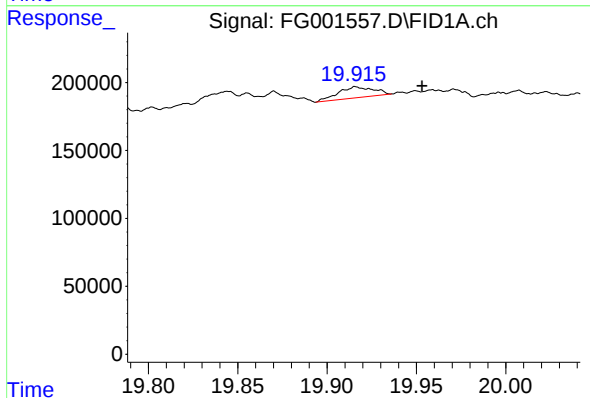

#16 N-HEXATRIACONTANE

R.T.: 19.916 min
Delta R.T.: -0.037 min
Response: 110585
Conc: 0.92 ug/ml