

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070218\
 Data File : PL037590.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2018 14:35
 Operator : UA\AJ
 Sample : J3742-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 14:53:04 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 21 02:27:11 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.344	3.935	128.1E6	54984823	16.196	19.874
28)	SA Decachlor...	8.025	8.952	109.1E6	33150421	18.085	16.709
Target Compounds							
4)	MA Heptachlor	4.347	0.000	4697815	0	0.459	N.D. #
5)	MB Aldrin	4.568	0.000	13180066	0	1.295	N.D. #
6)	B beta-BHC	4.263f	0.000	70718480	0	15.505	N.D. #
10)	B gamma-Chl...	5.268f	0.000	26850498	0	2.867	N.D. #
11)	B alpha-Chl...	5.268	0.000	26850498	0	2.957	N.D. #
17)	MA 4,4'-DDT	6.265f	0.000	58855535	0	9.116	N.D. #
18)	B Endrin al...	6.265	0.000	58855535	0	10.380	N.D. #
24)	Chlordane-2	4.615	0.000	988576	0	2.777	N.D. #
25)	Chlordane-3	5.268	0.000	26850498	0	25.261	N.D. #
26)	Chlordane-4	5.268	0.000	26850498	0	27.867	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL070218\
Data File : PL037590.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2018 14:35
Operator : UA\AJ
Sample : J3742-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 14:53:04 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\ECD_L\methods\PL062018.M
Quant Title : GC Extractables
QLast Update : Thu Jun 21 02:27:11 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

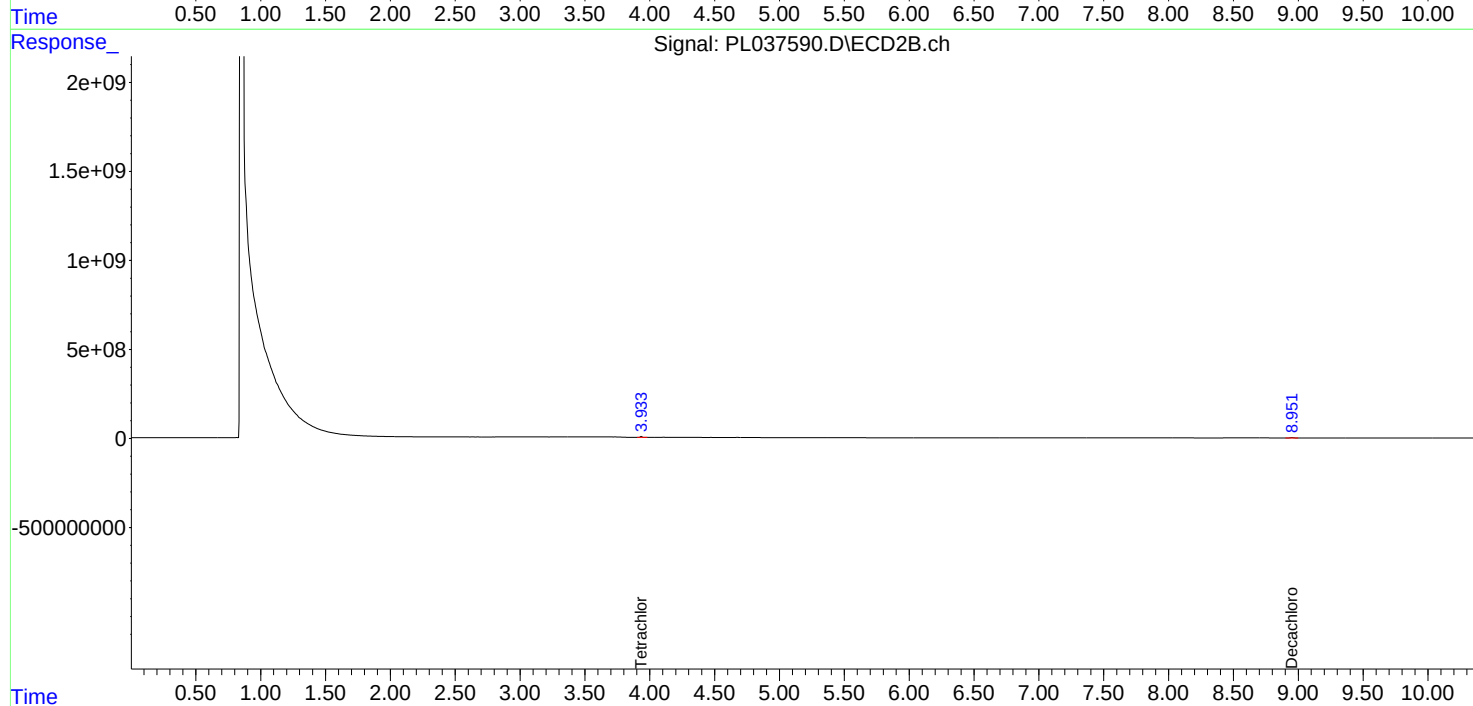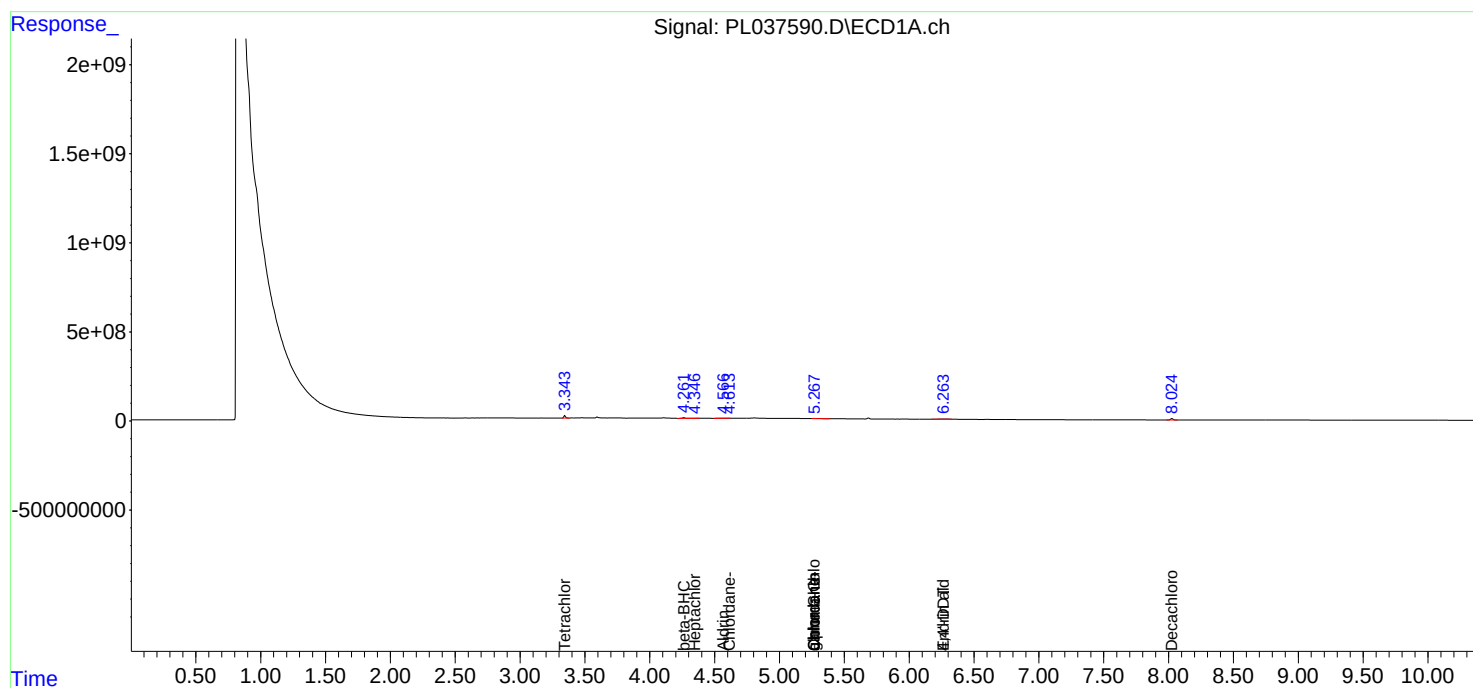


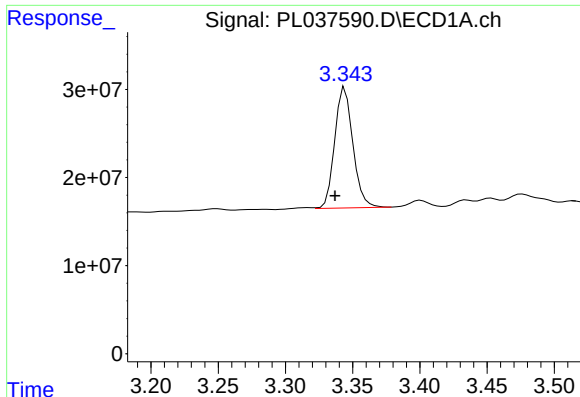

#1 Tetrachloro-m-xylene


R.T.: 3.344 min
Delta R.T.: 0.007 min
Response: 128113999
Conc: 16.20 ng/ml

Instrument :
FID_G
ClientSampleId :

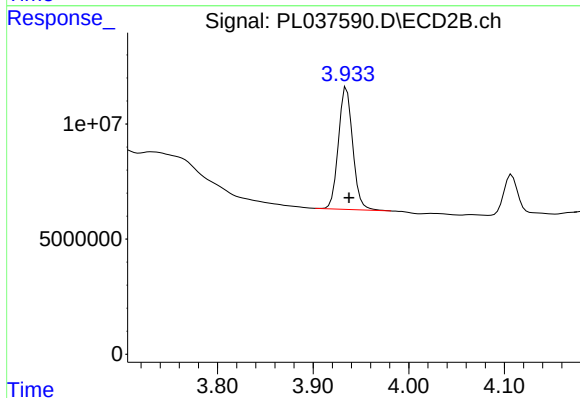


#1 Tetrachloro-m-xylene

R.T.: 3.935 min
Delta R.T.: -0.003 min
Response: 54984823
Conc: 19.87 ng/ml

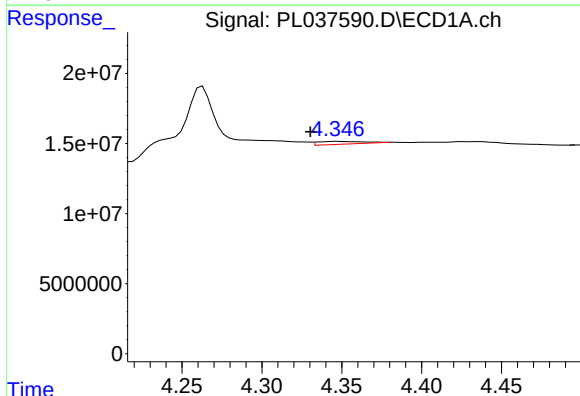


#4 Heptachlor

R.T.: 4.347 min
Delta R.T.: 0.017 min
Response: 4697815
Conc: 0.46 ng/ml

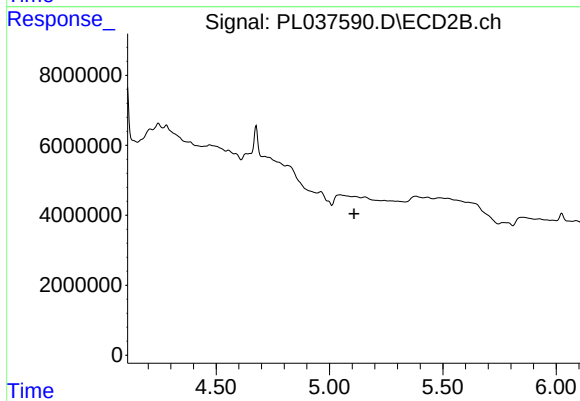

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.108 min
Response: 0
Conc: N.D.

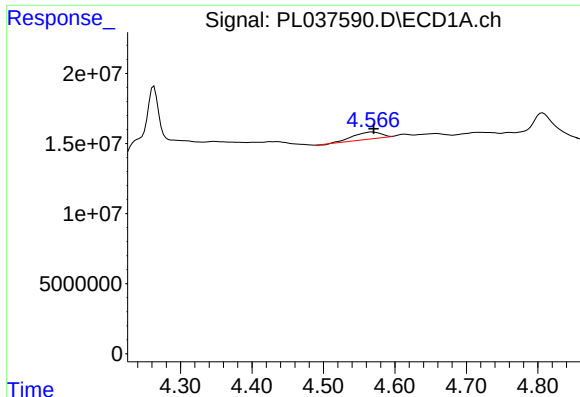

#5 Aldrin


R.T.: 4.568 min
Delta R.T.: -0.002 min
Response: 13180066
Conc: 1.29 ng/ml

Instrument :
FID_G
ClientSampleId :

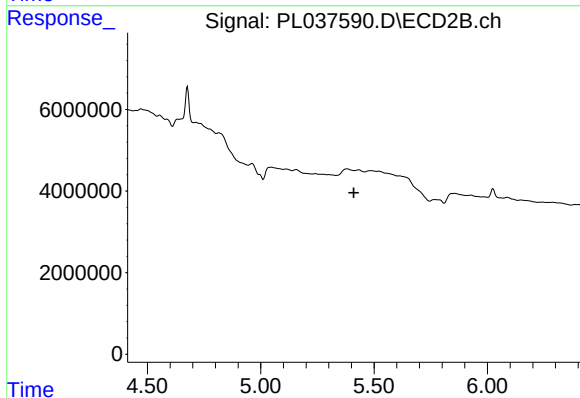


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.411 min
Response: 0
Conc: N.D.

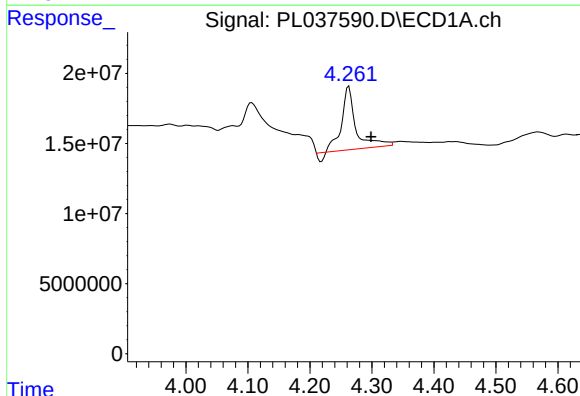


#6 beta-BHC

R.T.: 4.263 min
Delta R.T.: -0.036 min
Response: 70718480
Conc: 15.51 ng/ml

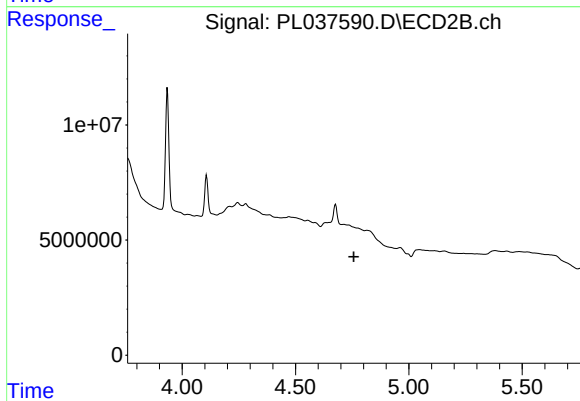

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.758 min
Response: 0
Conc: N.D.

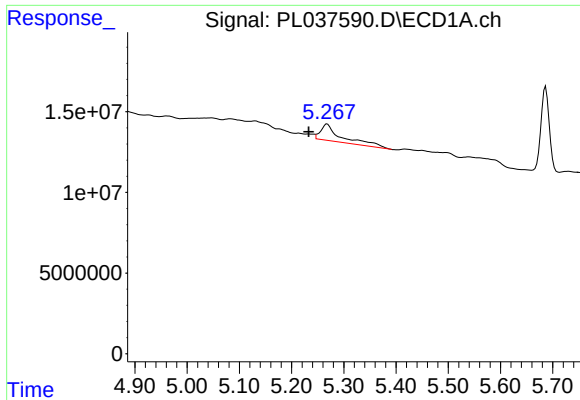

#10 gamma-Chlordane


R.T.: 5.268 min
Delta R.T.: 0.036 min
Response: 26850498
Conc: 2.87 ng/ml

Instrument :
FID_G
ClientSampleId :

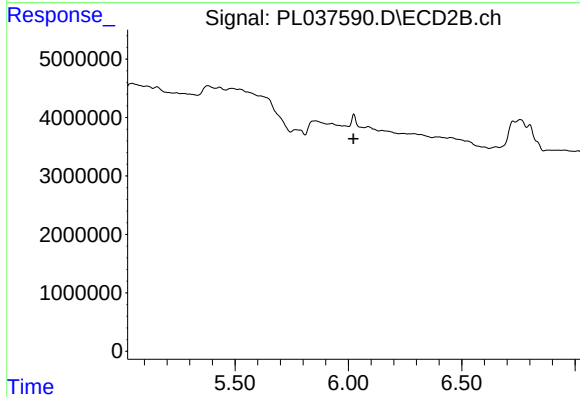


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

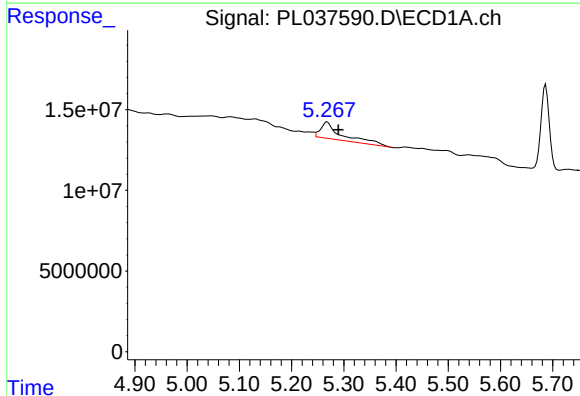


#11 alpha-Chlordane

R.T.: 5.268 min
Delta R.T.: -0.022 min
Response: 26850498
Conc: 2.96 ng/ml

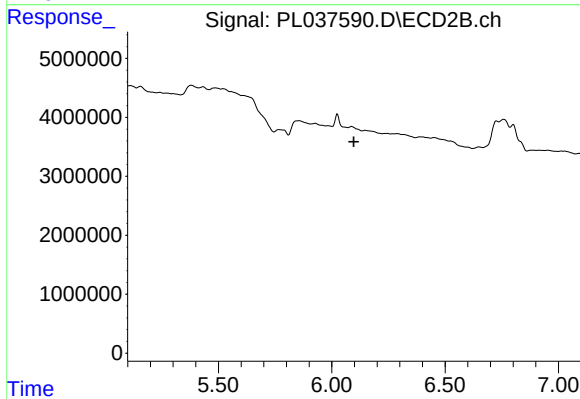

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.097 min
Response: 0
Conc: N.D.

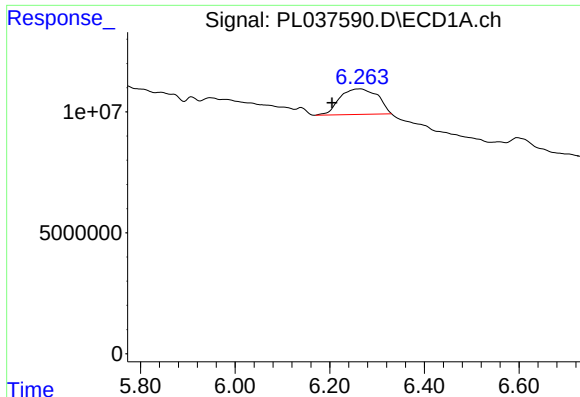

#17 4,4'-DDT


R.T.: 6.265 min
Delta R.T.: 0.059 min
Response: 58855535
Conc: 9.12 ng/ml

Instrument :
FID_G
ClientSampleId :

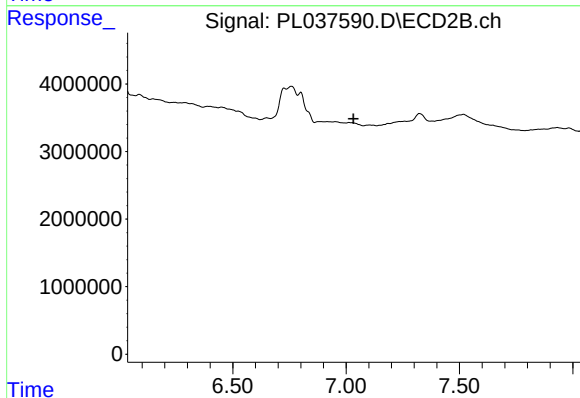


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.033 min
Response: 0
Conc: N.D.

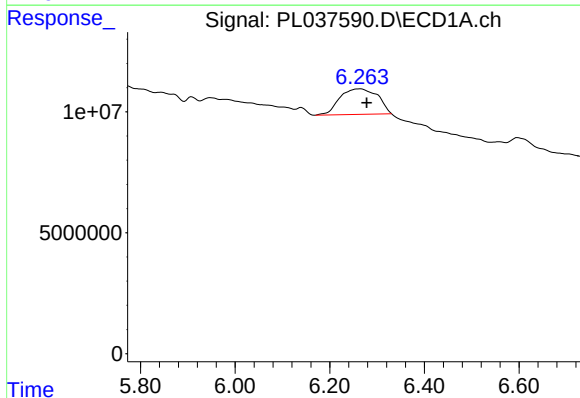


#18 Endrin aldehyde

R.T.: 6.265 min
Delta R.T.: -0.014 min
Response: 58855535
Conc: 10.38 ng/ml

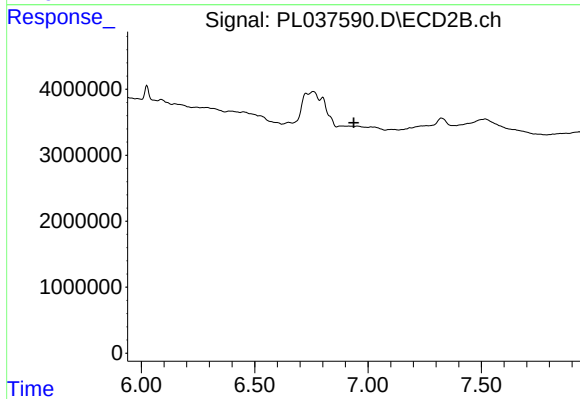

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.937 min
Response: 0
Conc: N.D.

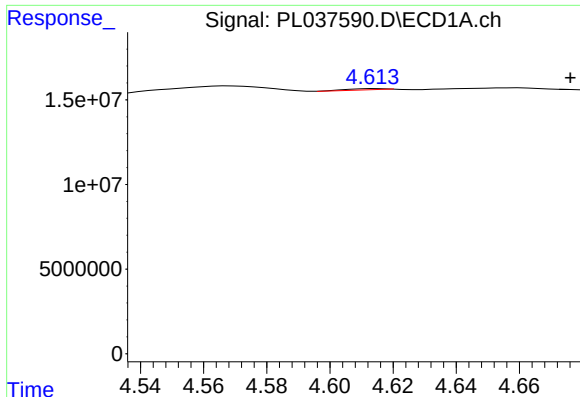

#24 Chlordane-2


R.T.: 4.615 min
Delta R.T.: -0.061 min
Response: 988576
Conc: 2.78 ng/ml

Instrument :
FID_G
ClientSampleId :

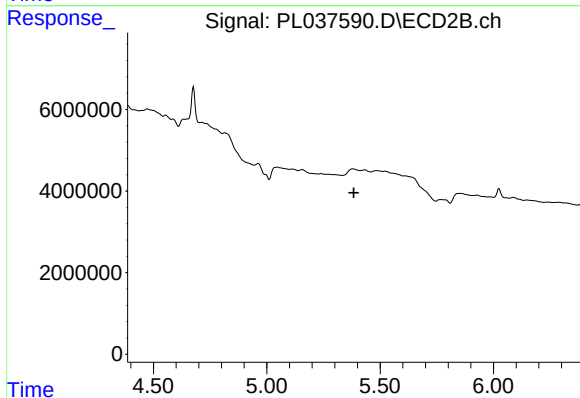


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.384 min
Response: 0
Conc: N.D.

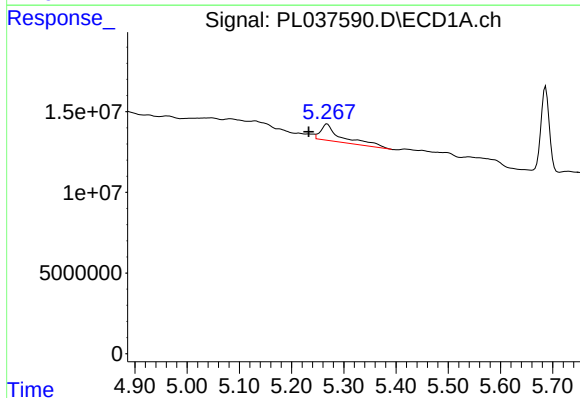


#25 Chlordane-3

R.T.: 5.268 min
Delta R.T.: 0.035 min
Response: 26850498
Conc: 25.26 ng/ml

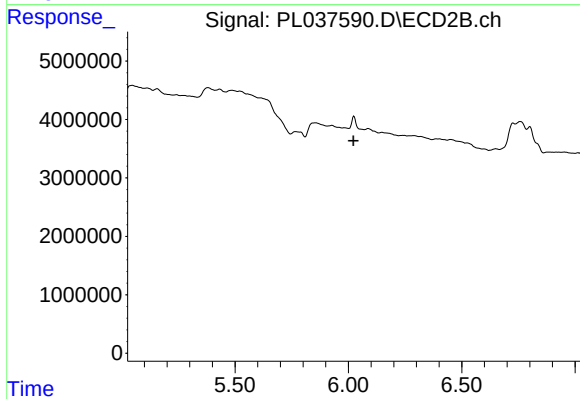

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

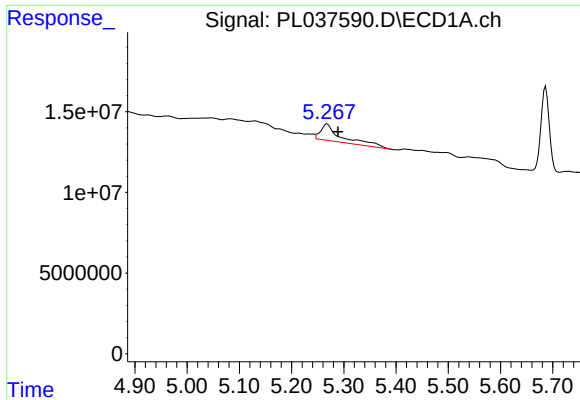

#26 Chlordane-4


R.T.: 5.268 min
Delta R.T.: -0.021 min
Response: 26850498
Conc: 27.87 ng/ml

Instrument :
FID_G
ClientSampleId :

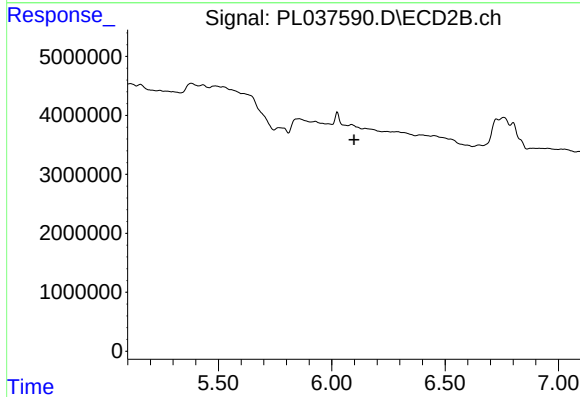


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.099 min
Response: 0
Conc: N.D.

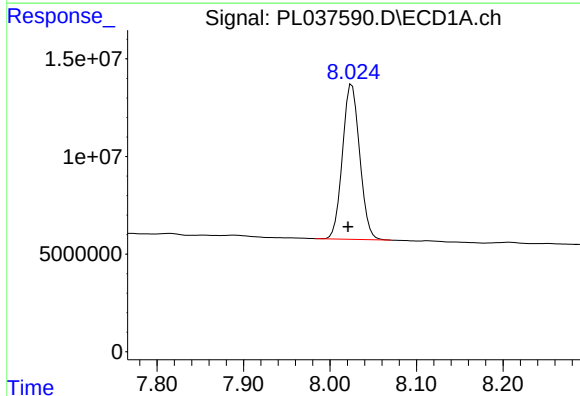

#28 Decachlorobiphenyl

R.T.: 8.025 min
Delta R.T.: 0.005 min
Response: 109126471
Conc: 18.09 ng/ml

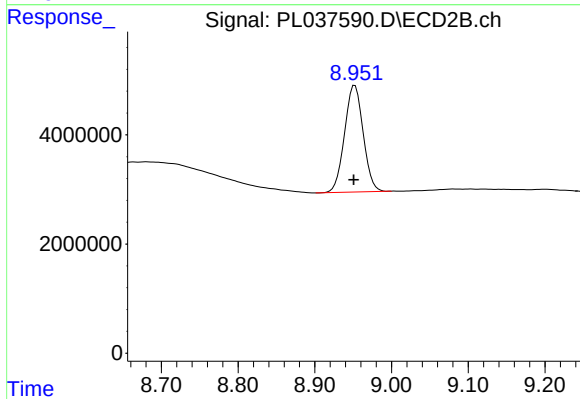

#28 Decachlorobiphenyl

R.T.: 8.952 min
Delta R.T.: 0.001 min
Response: 33150421
Conc: 16.71 ng/ml