

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070218\
Data File : FG001553.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2018 17:20
Operator : UA\AJ
Sample : J3761-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
256-CONCORD-COMP

Integration File: autoint1.e
Quant Time: Jul 03 01:00:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.522	2217261	19.058 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070218\
Data File : FG001553.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2018 17:20
Operator : UA\AJ
Sample : J3761-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
256-CONCORD-COMP

Integration File: autoint1.e
Quant Time: Jul 03 01:00:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

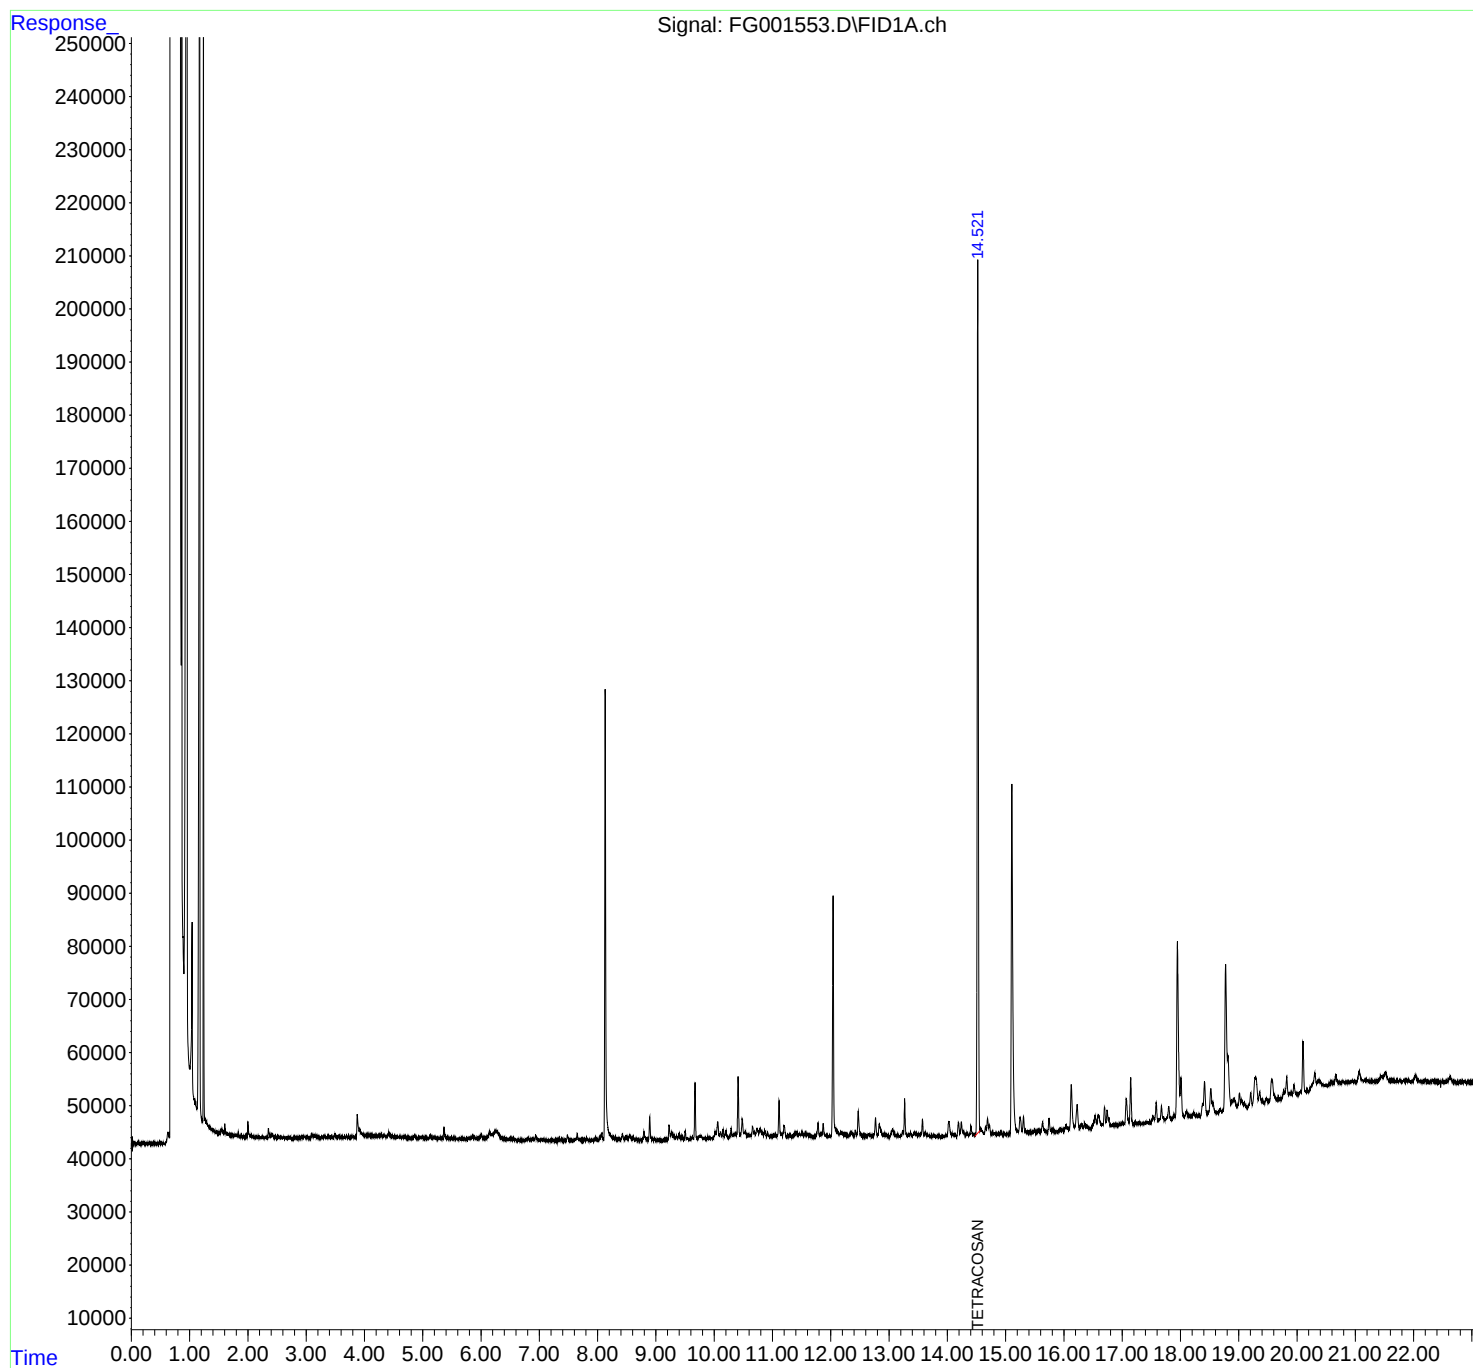

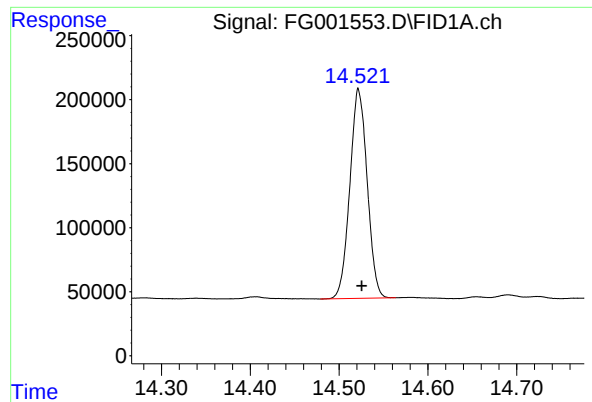

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.522 min
Delta R.T.: -0.004 min
Response: 2217261
Conc: 19.06 ug/ml

Instrument :
FID_G
ClientSampleId :
256-CONCORD-COMP