

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070219\
 Data File : FG005325.D
 Signal(s) : FID1A.ch
 Acq On : 02 Jul 2019 16:39
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 00:33:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
 Quant Title :
 QLast Update : Mon Jun 10 08:32:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.783	1953280	14.820 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.977	54693	0.368 ug/ml
12) N-OCTACOSANE	16.962	28553	0.201 ug/ml
13) N-TRIACONTANE	17.853	21239	0.152 ug/ml
14) N-DOTRIACONTANE	18.688	64454	0.479 ug/ml
15) N-TETRATRIACONTANE	19.477	25041	0.195 ug/ml
16) N-HEXATRIACONTANE	20.245	49523	0.416 ug/ml
17) N-OCTATRIACONTANE	20.990	13853	0.131 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070219\
Data File : FG005325.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2019 16:39
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampled :

Integration File: autoint1.e
Quant Time: Jul 03 00:33:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

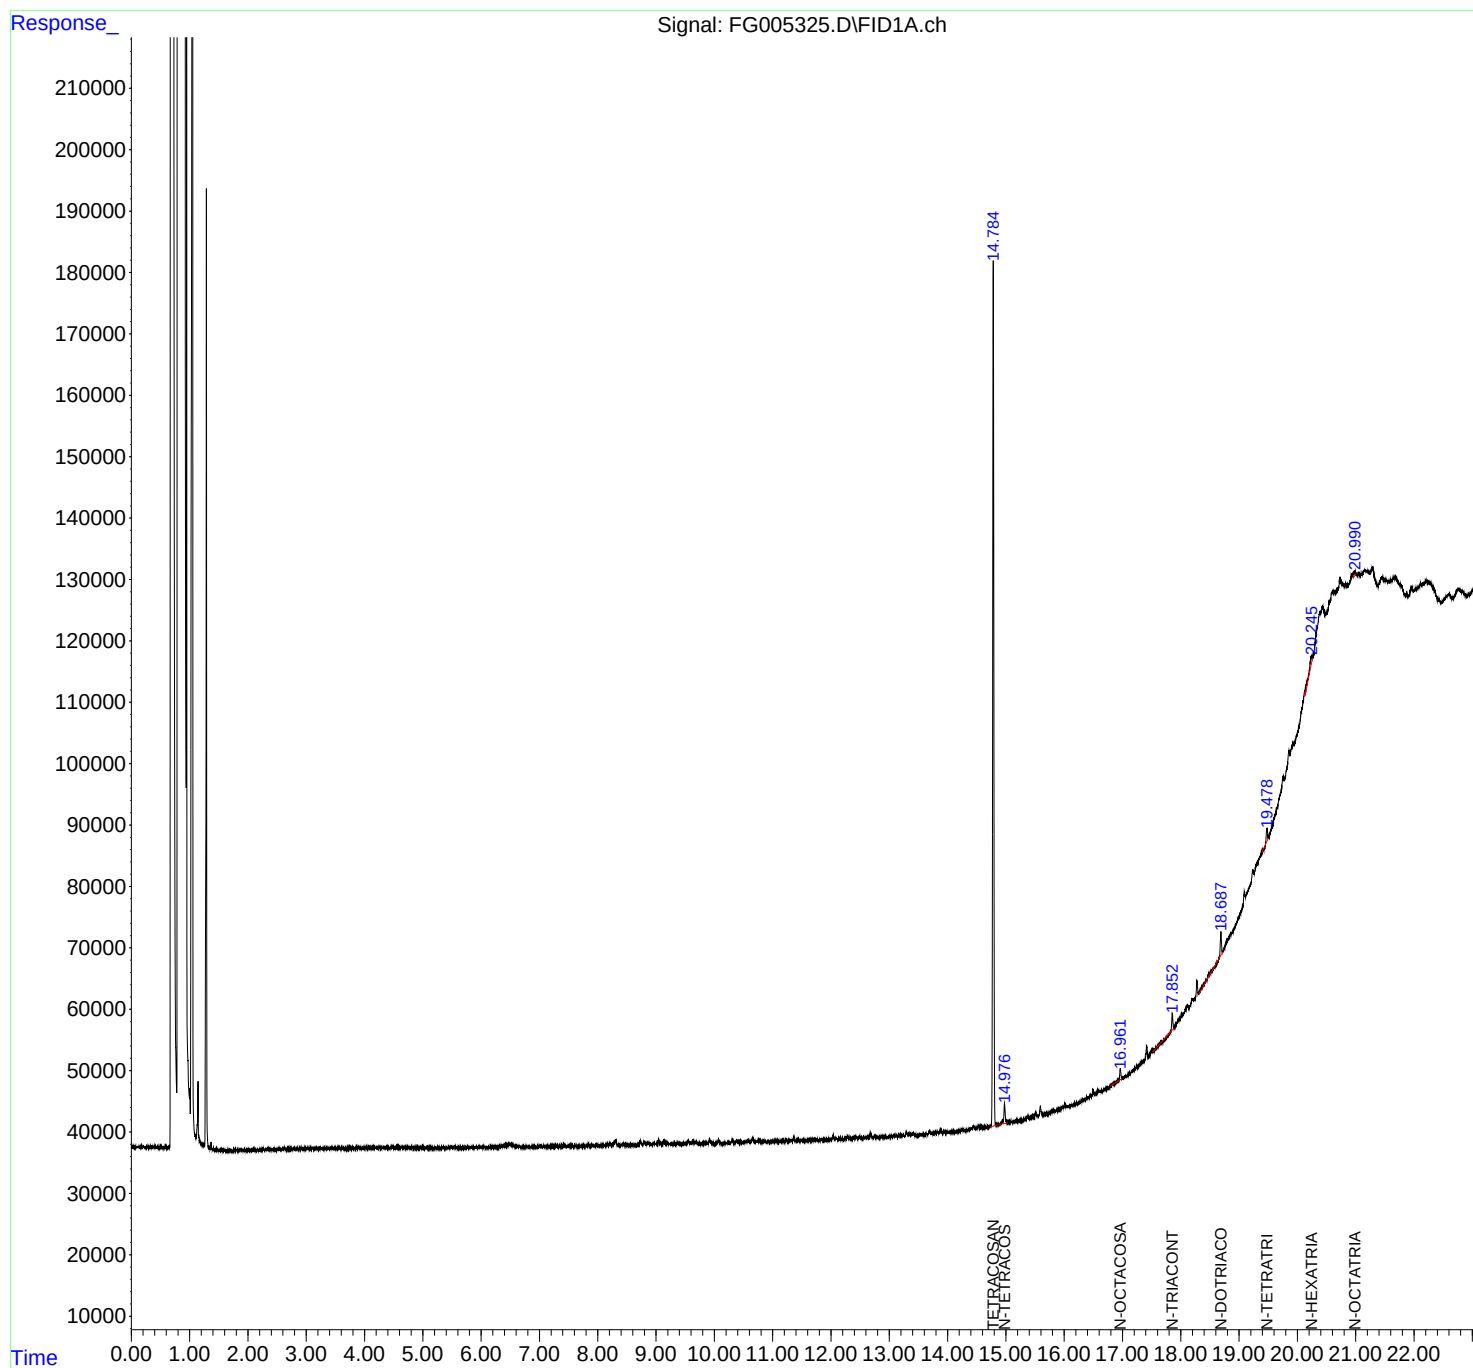


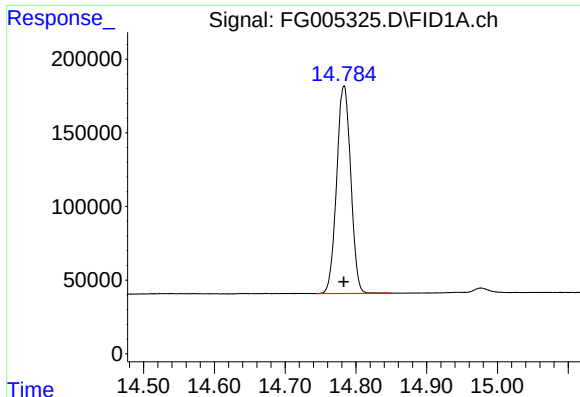

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.783 min
Delta R.T.: 0.000 min
Response: 1953280
Conc: 14.82 ug/ml

Instrument :
FID_G
ClientSampleId :

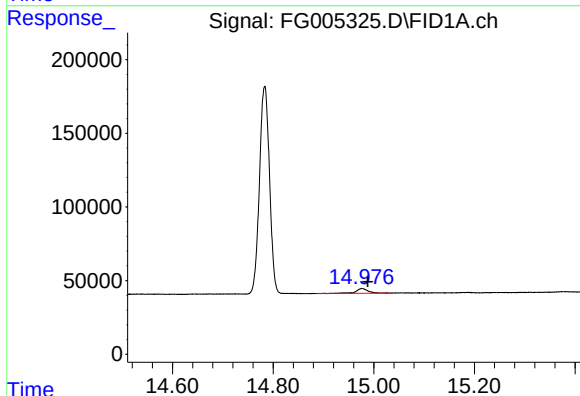


#10 N-TETRACOSANE

R.T.: 14.977 min
Delta R.T.: -0.011 min
Response: 54693
Conc: 0.37 ug/ml

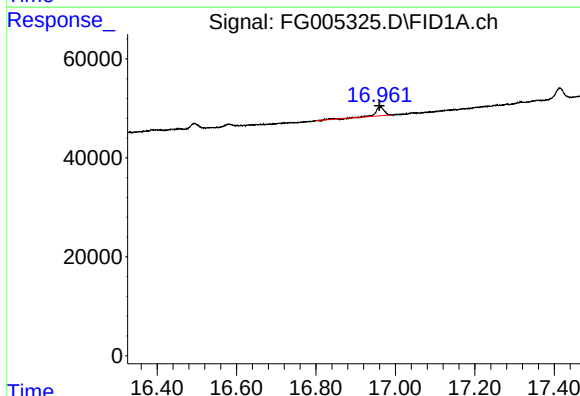


#12 N-OCTACOSANE

R.T.: 16.962 min
Delta R.T.: 0.002 min
Response: 28553
Conc: 0.20 ug/ml

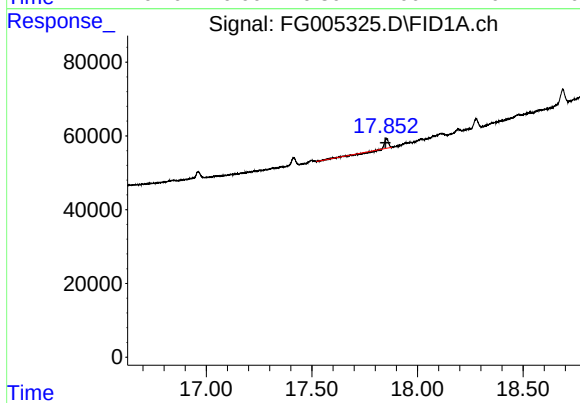

#13 N-TRIACONTANE


R.T.: 17.853 min
Delta R.T.: 0.004 min
Response: 21239
Conc: 0.15 ug/ml

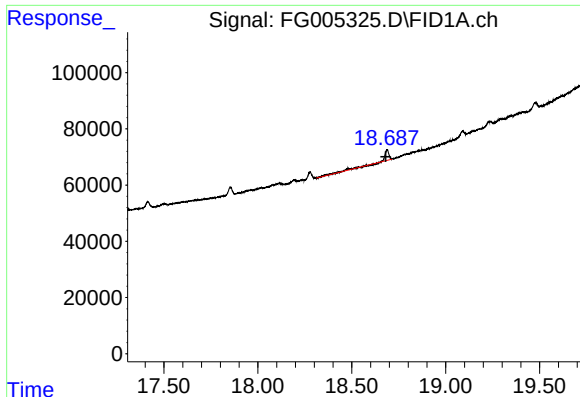

#14 N-DOTRIACONTANE


R.T.: 18.688 min
Delta R.T.: 0.007 min
Response: 64454
Conc: 0.48 ug/ml

Instrument :
FID_G
ClientSampleId :

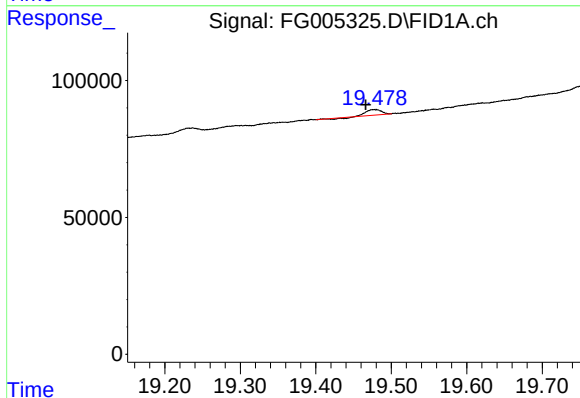


#15 N-TETRATRIACONTANE

R.T.: 19.477 min
Delta R.T.: 0.011 min
Response: 25041
Conc: 0.20 ug/ml

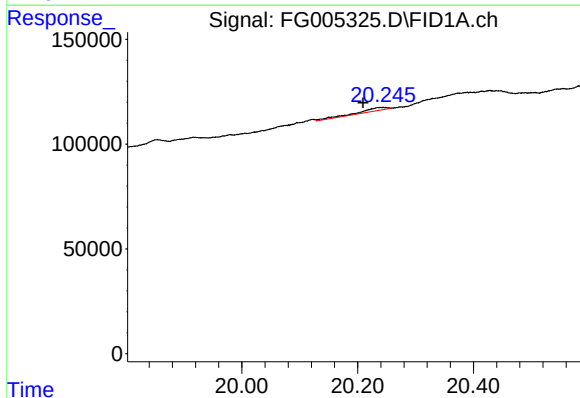

#16 N-HEXATRIACONTANE

R.T.: 20.245 min
Delta R.T.: 0.035 min
Response: 49523
Conc: 0.42 ug/ml

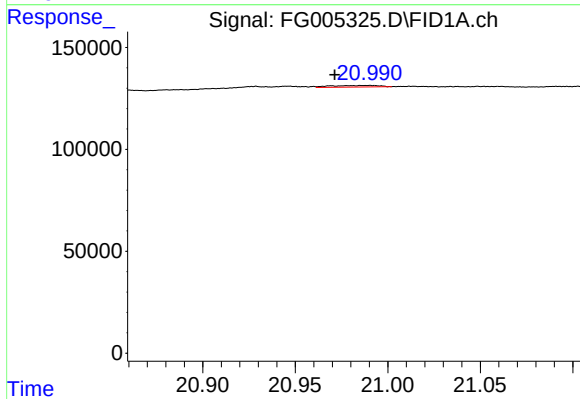

#17 N-OCTATRIACONTANE

R.T.: 20.990 min
Delta R.T.: 0.019 min
Response: 13853
Conc: 0.13 ug/ml