

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070219\
 Data File : FG005329.D
 Signal(s) : FID1A.ch
 Acq On : 02 Jul 2019 18:38
 Operator : DD\AJ
 Sample : K3555-22
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 00:34:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
 Quant Title :
 QLast Update : Mon Jun 10 08:32:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.781	2079277	15.776 ug/ml
Target Compounds			
4) N-TETRADECANE	8.274	25800	0.172 ug/ml
5) N-HEXADECANE	9.915	24162	0.159 ug/ml
6) N-OCTADECANE	11.362	29395	0.194 ug/ml
8) N-DOCOSANE	13.878	62621	0.416 ug/ml
10) N-TETRACOSANE	14.975	245533	1.650 ug/ml
11) N-HEXACOSANE	16.008	88357	0.607 ug/ml
12) N-OCTACOSANE	16.961	235869	1.658 ug/ml
13) N-TRIACONTANE	17.849	278339	1.989 ug/ml
14) N-DOTRIACONTANE	18.683	249161	1.852 ug/ml
15) N-TETRATRIACONTANE	19.471	43419	0.339 ug/ml
16) N-HEXATRIACONTANE	20.231	9818	0.082 ug/ml
17) N-OCTATRIACONTANE	20.980	35540	0.335 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070219\
Data File : FG005329.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2019 18:38
Operator : DD\AJ
Sample : K3555-22
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 00:34:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

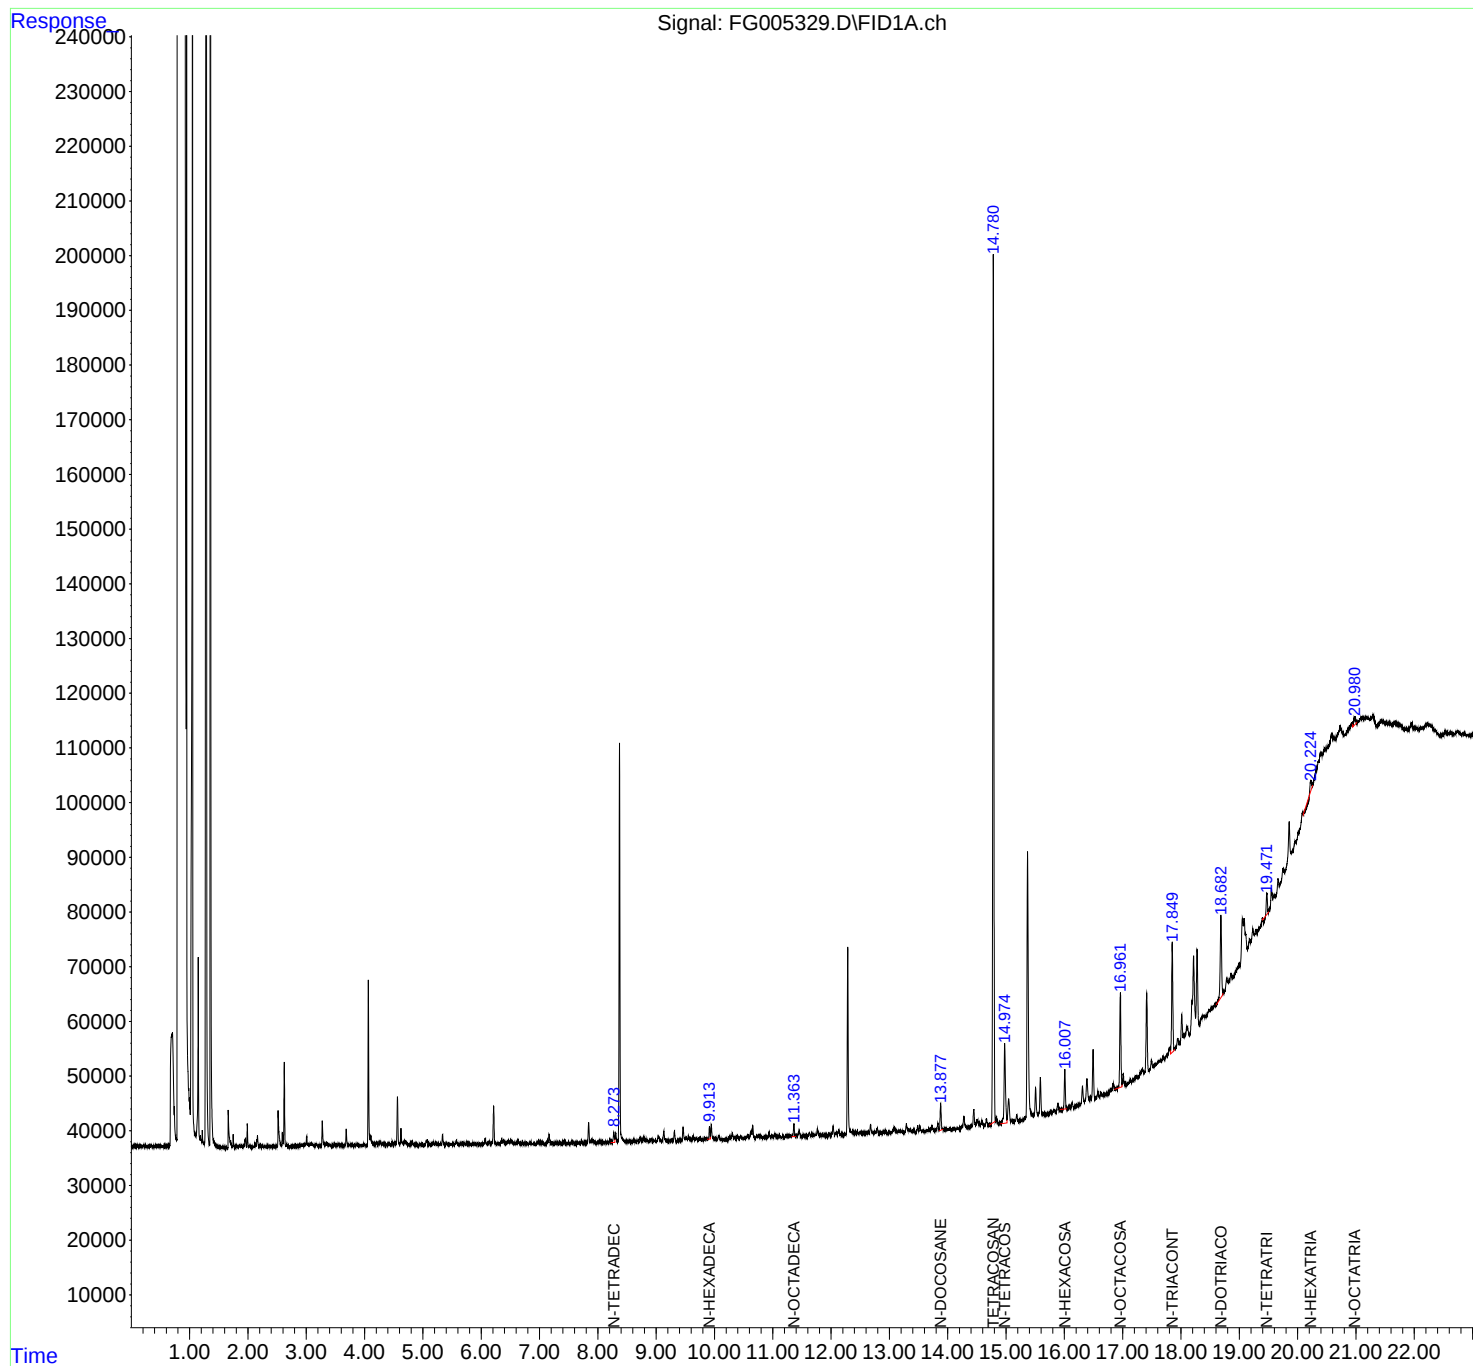


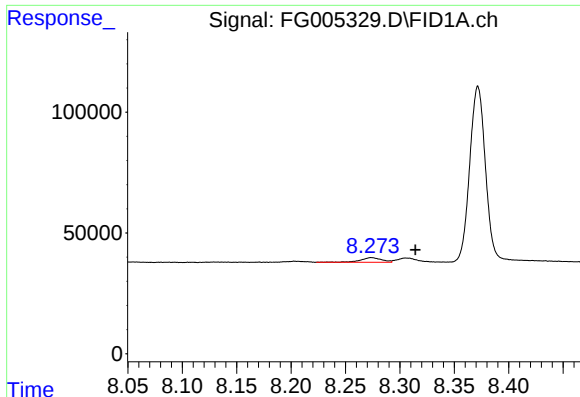

#4 N-TETRADECANE


R.T.: 8.274 min
Delta R.T.: -0.040 min
Response: 25800
Conc: 0.17 ug/ml

Instrument :
FID_G
ClientSampleId :

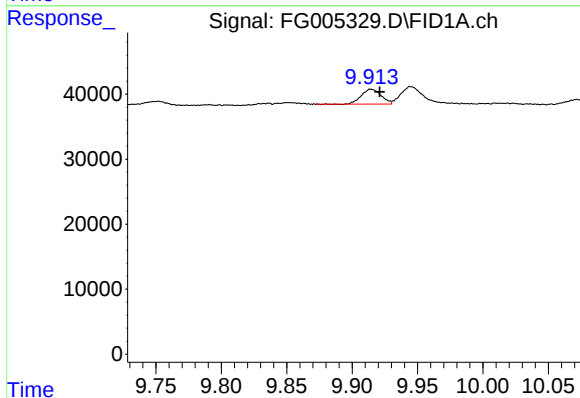


#5 N-HEXADECANE

R.T.: 9.915 min
Delta R.T.: -0.006 min
Response: 24162
Conc: 0.16 ug/ml

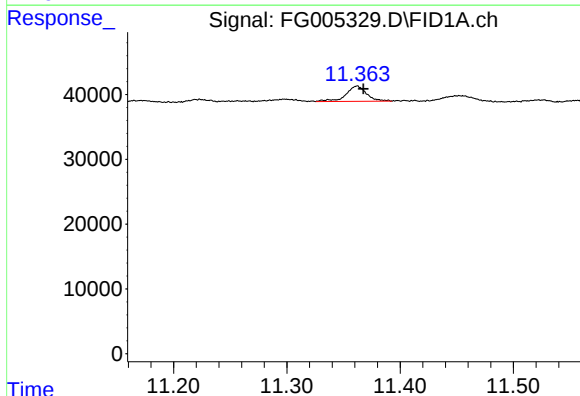


#6 N-OCTADECANE

R.T.: 11.362 min
Delta R.T.: -0.006 min
Response: 29395
Conc: 0.19 ug/ml

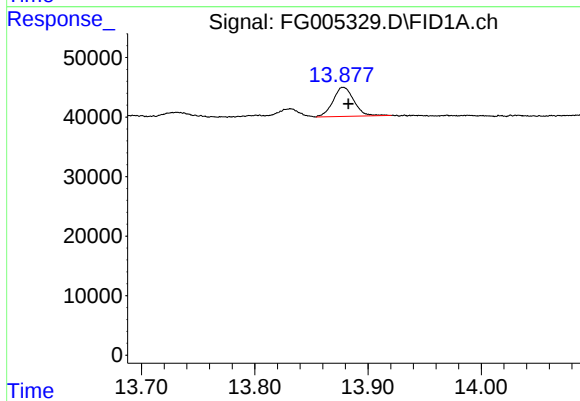

#8 N-Docosane


R.T.: 13.878 min
Delta R.T.: -0.004 min
Response: 62621
Conc: 0.42 ug/ml

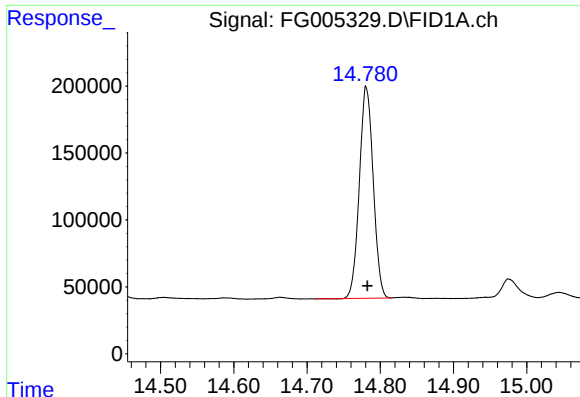

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.781 min
Delta R.T.: -0.002 min
Response: 2079277
Conc: 15.78 ug/ml

Instrument :
FID_G
ClientSampleId :

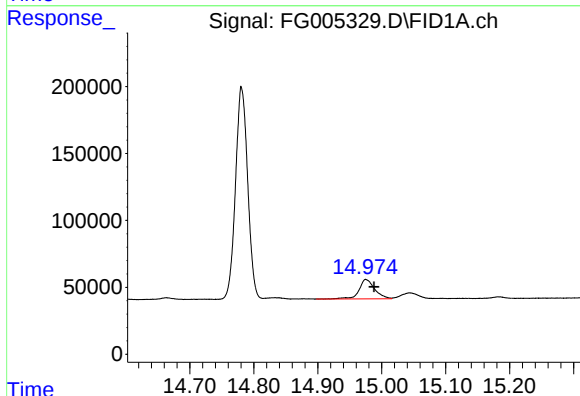


#10 N-TETRACOSANE

R.T.: 14.975 min
Delta R.T.: -0.013 min
Response: 245533
Conc: 1.65 ug/ml

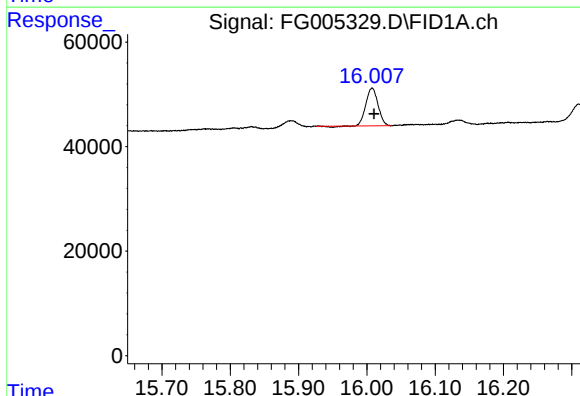


#11 N-HEXACOSANE

R.T.: 16.008 min
Delta R.T.: -0.003 min
Response: 88357
Conc: 0.61 ug/ml

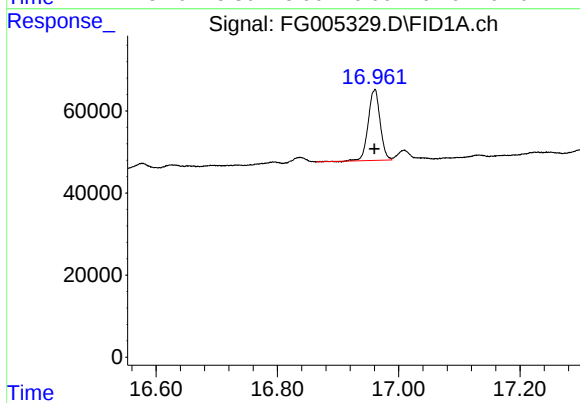

#12 N-OCTACOSANE


R.T.: 16.961 min
Delta R.T.: 0.000 min
Response: 235869
Conc: 1.66 ug/ml

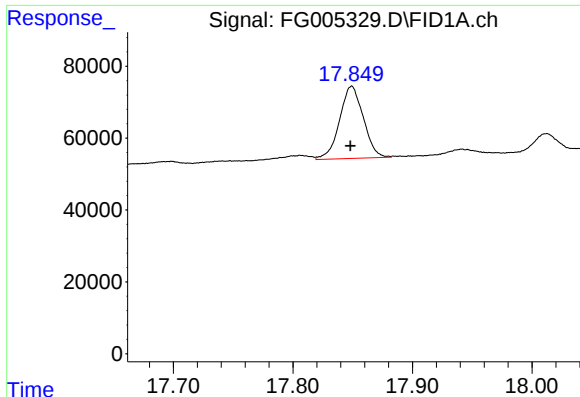

#13 N-TRIACONTANE


R.T.: 17.849 min
Delta R.T.: 0.000 min
Response: 278339
Conc: 1.99 ug/ml

Instrument :
FID_G
ClientSampleId :

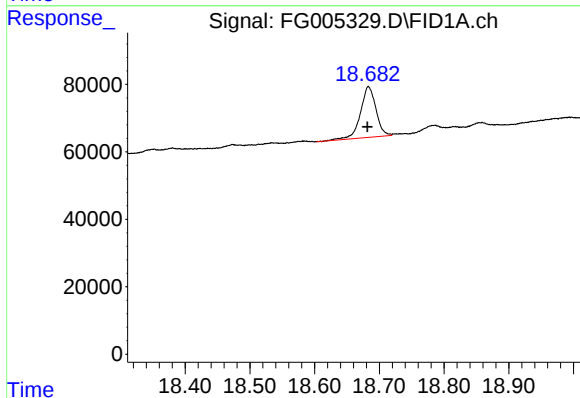


#14 N-DOTRIACONTANE

R.T.: 18.683 min
Delta R.T.: 0.002 min
Response: 249161
Conc: 1.85 ug/ml

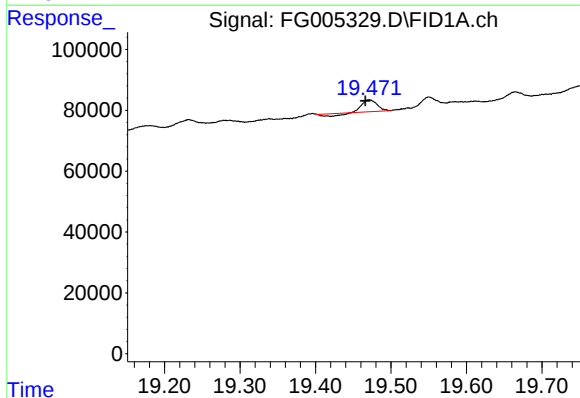


#15 N-TETRATRIACONTANE

R.T.: 19.471 min
Delta R.T.: 0.005 min
Response: 43419
Conc: 0.34 ug/ml

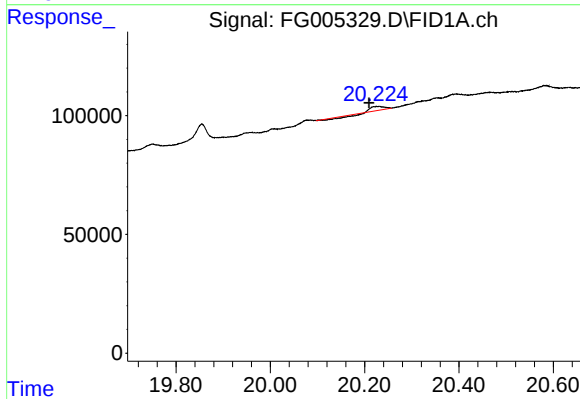

#16 N-HEXATRIACONTANE

R.T.: 20.231 min
Delta R.T.: 0.022 min
Response: 9818
Conc: 0.08 ug/ml

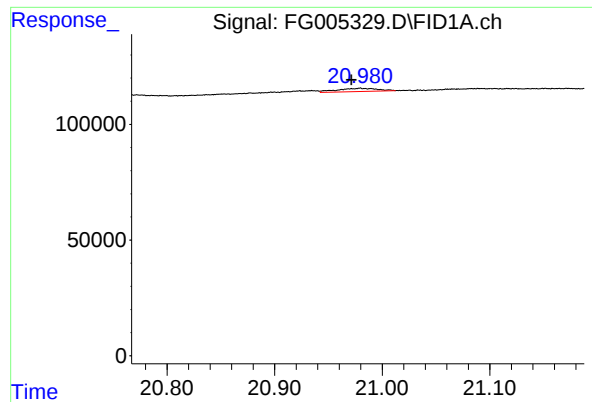

#17 N-OCTATRIACONTANE

R.T.: 20.980 min
Delta R.T.: 0.008 min
Response: 35540
Conc: 0.34 ug/ml

Instrument :
FID_G
ClientSampleId :