

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070219\
 Data File : FG005333.D
 Signal(s) : FID1A.ch
 Acq On : 02 Jul 2019 20:36
 Operator : DD\AJ
 Sample : PB121081BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 00:35:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
 Quant Title :
 QLast Update : Mon Jun 10 08:32:25 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.780	1762815	13.375 ug/ml
Target Compounds			
10) N-TETRACOSANE	14.975	45564	0.306 ug/ml
12) N-OCTACOSANE	16.961	26349	0.185 ug/ml
13) N-TRIACONTANE	17.847	19188	0.137 ug/ml
14) N-DOTRIACONTANE	18.681	58183	0.433 ug/ml
15) N-TETRATRIACONTANE	19.469	12769	0.100 ug/ml
17) N-OCTATRIACONTANE	20.977	66029	0.623 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG070219\
Data File : FG005333.D
Signal(s) : FID1A.ch
Acq On : 02 Jul 2019 20:36
Operator : DD\AJ
Sample : PB121081BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 00:35:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG060719.M
Quant Title :
QLast Update : Mon Jun 10 08:32:25 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

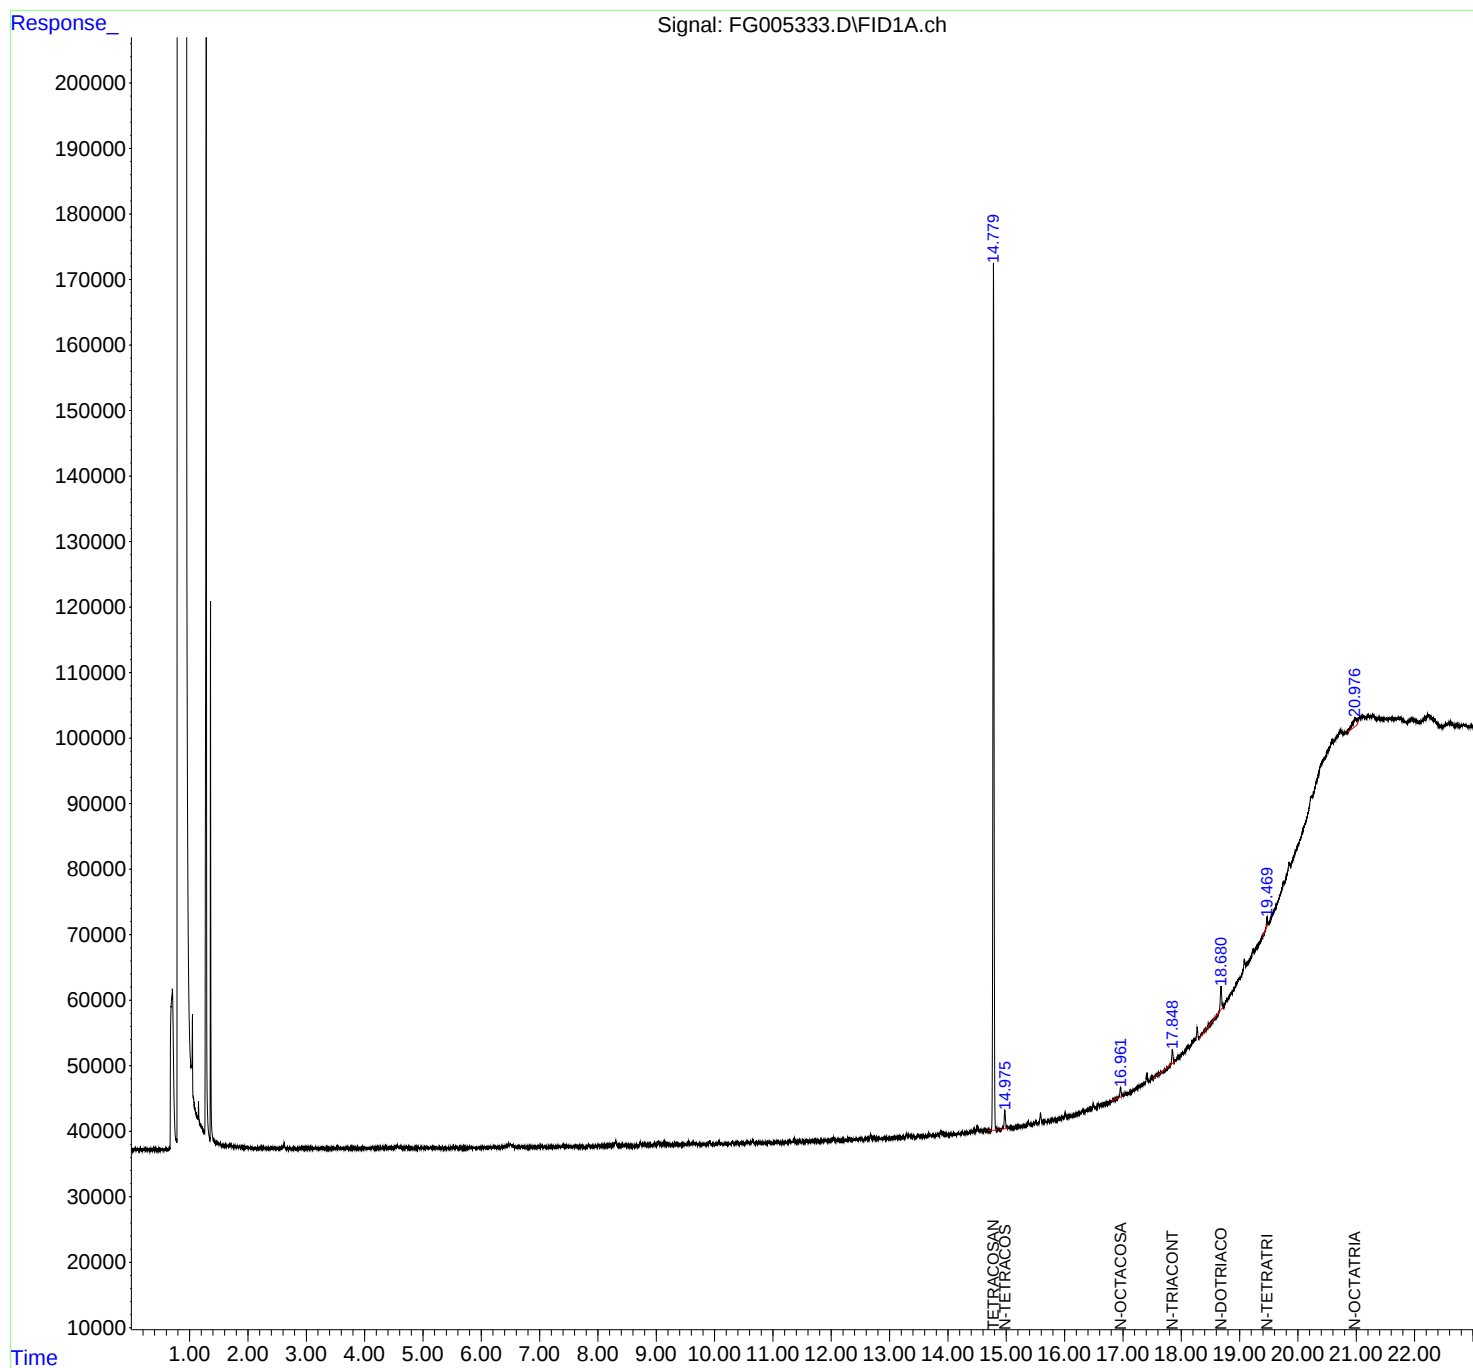


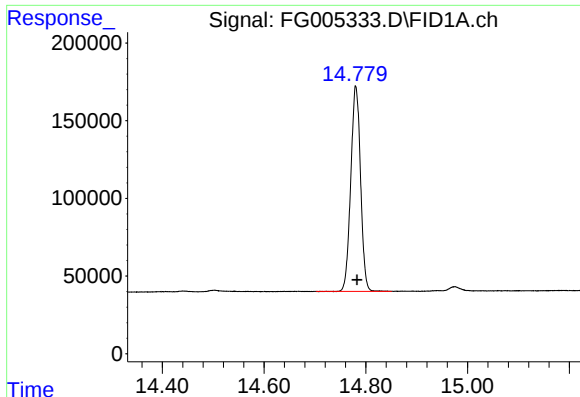

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.780 min
Delta R.T.: -0.002 min
Response: 1762815
Conc: 13.38 ug/ml

Instrument :
FID_G
ClientSampleId :

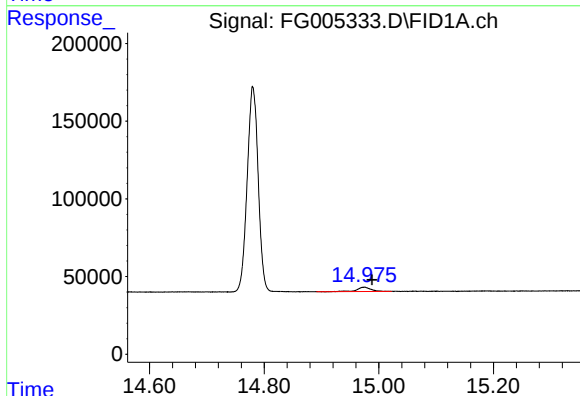


#10 N-TETRACOSANE

R.T.: 14.975 min
Delta R.T.: -0.013 min
Response: 45564
Conc: 0.31 ug/ml

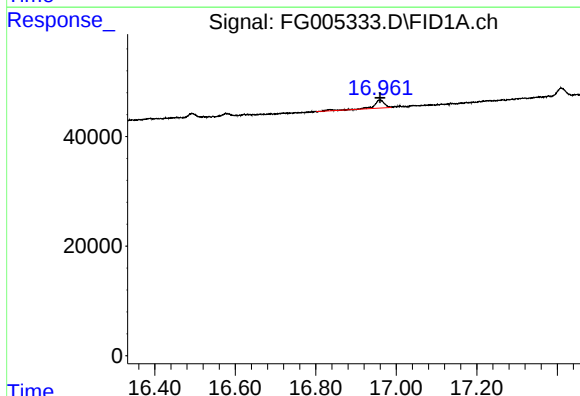


#12 N-OCTACOSANE

R.T.: 16.961 min
Delta R.T.: 0.001 min
Response: 26349
Conc: 0.19 ug/ml

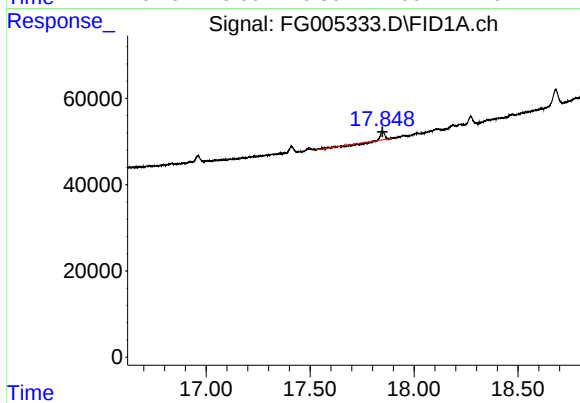

#13 N-TRIACONTANE


R.T.: 17.847 min
Delta R.T.: 0.000 min
Response: 19188
Conc: 0.14 ug/ml

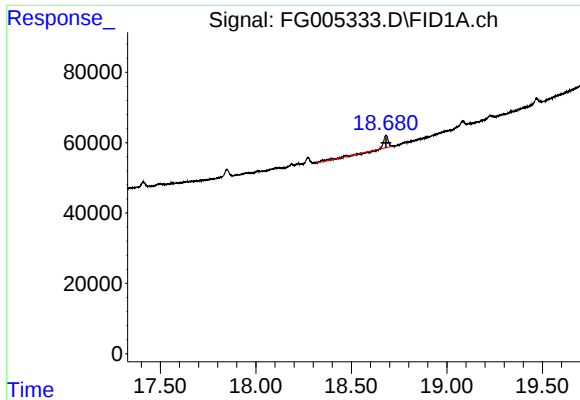

#14 N-DOTRIACONTANE


R.T.: 18.681 min
Delta R.T.: 0.000 min
Response: 58183
Conc: 0.43 ug/ml

Instrument :
FID_G
ClientSampleId :

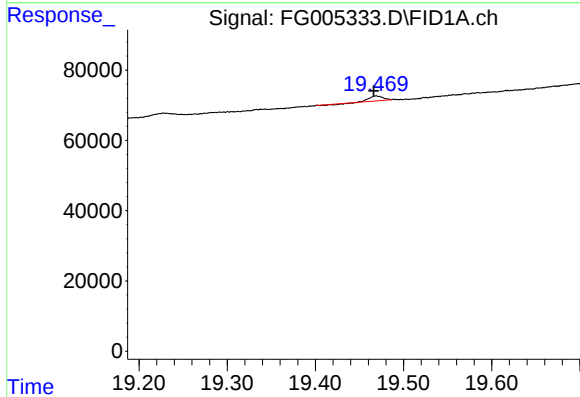

#15 N-TETRATRIACONTANE

R.T.: 19.469 min
Delta R.T.: 0.003 min
Response: 12769
Conc: 0.10 ug/ml

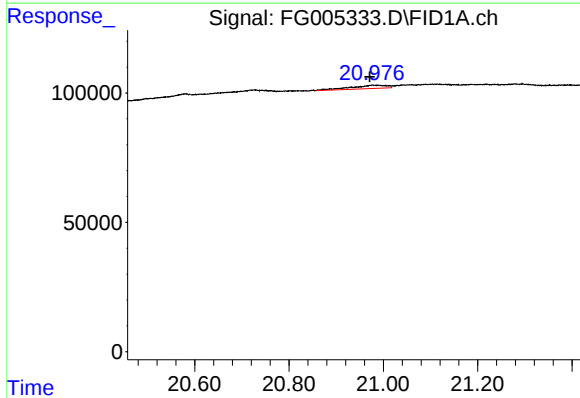

#17 N-OCTATRIACONTANE

R.T.: 20.977 min
Delta R.T.: 0.005 min
Response: 66029
Conc: 0.62 ug/ml